ADVANTEST_®

ADVANTEST CORPORATION

U3700 Series OPT10/OPT11 OPT53/OPT54/OPT55/OPT56 User's Guide

MANUAL NUMBER FOE-8440273C02

Applicable Models

U3741

U3751

U3771

U3772

Safety Summary

To ensure thorough understanding of all functions and to ensure efficient use of this instrument, please read the manual carefully before using. Note that Advantest bears absolutely no responsibility for the result of operations caused due to incorrect or inappropriate use of this instrument.

If the equipment is used in a manner not specified by Advantest, the protection provided by the equipment may be impaired.

Warning Labels

Warning labels are applied to Advantest products in locations where specific dangers exist. Pay careful attention to these labels during handling. Do not remove or tear these labels. If you have any questions regarding warning labels, please ask your nearest Advantest dealer. Our address and phone number are listed at the end of this manual.

Symbols of those warning labels are shown below together with their meaning.

DANGER: Indicates an imminently hazardous situation which will result in death or serious personal injury.

WARNING: Indicates a potentially hazardous situation which will result in death or serious personal injury.

CAUTION: Indicates a potentially hazardous situation which will result in personal injury or a damage to property including the product.

Basic Precautions

Please observe the following precautions to prevent fire, burn, electric shock, and personal injury.

- Use a power cable rated for the voltage in question. Be sure however to use a power cable conforming to safety standards of your nation when using a product overseas.
- When inserting the plug into the electrical outlet, first turn the power switch OFF and then
 insert the plug as far as it will go.
- When removing the plug from the electrical outlet, first turn the power switch OFF and then pull it out by gripping the plug. Do not pull on the power cable itself. Make sure your hands are dry at this time.
- Before turning on the power, be sure to check that the supply voltage matches the voltage requirements of the instrument.
- Connect the power cable to a power outlet that is connected to a protected ground terminal. Grounding will be defeated if you use an extension cord which does not include a protected ground terminal.
- Be sure to use fuses rated for the voltage in question.
- Do not use this instrument with the case open.
- Do not place anything on the product and do not apply excessive pressure to the product. Also, do not place flower pots or other containers containing liquid such as chemicals near this

product.

- When the product has ventilation outlets, do not stick or drop metal or easily flammable objects into the ventilation outlets.
- When using the product on a cart, fix it with belts to avoid its drop.
- When connecting the product to peripheral equipment, turn the power off.

Caution Symbols Used Within this Manual

Symbols indicating items requiring caution which are used in this manual are shown below together with their meaning.

DANGER: Indicates an item where there is a danger of serious personal injury (death or serious injury).

WARNING: Indicates an item relating to personal safety or health.

CAUTION: Indicates an item relating to possible damage to the product or instrument or relating to a restriction on operation.

· Safety Marks on the Product

The following safety marks can be found on Advantest products.



ATTENTION - Refer to manual.



Protective ground (earth) terminal.



DANGER - High voltage.



CAUTION - Risk of electric shock.

· Replacing Parts with Limited Life

The following parts used in the instrument are main parts with limited life.

Replace the parts listed below before their expected lifespan has expired to maintain the performance and function of the instrument.

Note that the estimated lifespan for the parts listed below may be shortened by factors such as the environment where the instrument is stored or used, and how often the instrument is used. The parts inside are not user-replaceable. For a part replacement, please contact the Advantest sales office for servicing.

Each product may use parts with limited life.

For more information, refer to the section in this document where the parts with limited life are described.

Main Parts with Limited Life

Part name	Life
Unit power supply	5 years
Fan motor	5 years
Electrolytic capacitor	5 years
LCD display	6 years
LCD backlight	2.5 years
Floppy disk drive	5 years
Memory backup battery	5 years

Hard Disk Mounted Products

The operational warnings are listed below.

- Do not move, shock and vibrate the product while the power is turned on.

 Reading or writing data in the hard disk unit is performed with the memory disk turning at a high speed. It is a very delicate process.
- Store and operate the products under the following environmental conditions.

An area with no sudden temperature changes.

An area away from shock or vibrations.

An area free from moisture, dirt, or dust.

An area away from magnets or an instrument which generates a magnetic field.

• Make back-ups of important data.

The data stored in the disk may become damaged if the product is mishandled. The hard disc has a limited life span which depends on the operational conditions. Note that there is no guarantee for any loss of data.

Precautions when Disposing of this Instrument

When disposing of harmful substances, be sure dispose of them properly with abiding by the state-provided law.

Harmful substances: (1) PCB (polycarbon biphenyl)

(2) Mercury

(3) Ni-Cd (nickel cadmium)

(4) Other

Items possessing cyan, organic phosphorous and hexadic chromium and items which may leak cadmium or arsenic (excluding lead in solder).

Example: fluorescent tubes, batteries

Environmental Conditions

This instrument should be only be used in an area which satisfies the following conditions:

- · An area free from corrosive gas
- An area away from direct sunlight
- A dust-free area
- An area free from vibrations
- Altitude of up to 2000 m

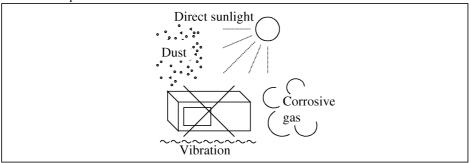


Figure-1 Environmental Conditions

• Operating position

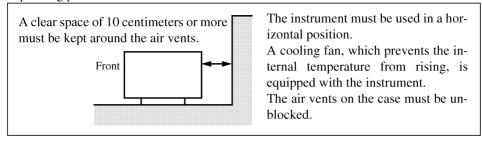


Figure-2 Operating Position

• Storage position

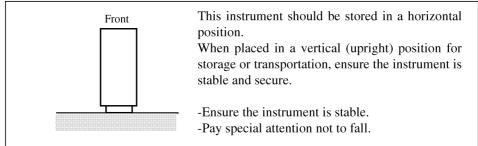


Figure-3 Storage Position

• The classification of the transient over-voltage, which exists typically in the main power supply, and the pollution degree is defined by IEC61010-1 and described below.

Impulse withstand voltage (over-voltage) category II defined by IEC60364-4-443

Pollution Degree 2

Types of Power Cable

Replace any references to the power cable type, according to the following table, with the appropriate power cable type for your country.

Plug configuration	Standards	Rating, color and length	Model number (Option number)
[L N]	PSE: Japan Electrical Appliance and Material Safety Law	125 V at 7 A Black 2 m (6 ft)	Straight: A01402 Angled: A01412
[]L N[]	UL: United States of America CSA: Canada	125 V at 7 A Black 2 m (6 ft)	Straight: A01403 (Option 95) Angled: A01413
	CEE: Europe DEMKO: Denmark NEMKO: Norway VDE: Germany KEMA: The Netherlands CEBEC: Belgium OVE: Austria FIMKO: Finland SEMKO: Sweden	250 V at 6 A Gray 2 m (6 ft)	Straight: A01404 (Option 96) Angled: A01414
(E 8)	SEV: Switzerland	250 V at 6 A Gray 2 m (6 ft)	Straight: A01405 (Option 97) Angled: A01415
	SAA: Australia, New Zealand	250 V at 6 A Gray 2 m (6 ft)	Straight: A01406 (Option 98) Angled:
	BS: United Kingdom	250 V at 6 A Black 2 m (6 ft)	Straight: A01407 (Option 99) Angled: A01417
	CCC:China	250 V at 10 A Black 2 m (6 ft)	Straight: A114009 (Option 94) Angled: A114109

ADVANTEST®

ADVANTEST CORPORATION

U3700 Series User's Guide

MANUAL NUMBER FOE-8440185J01

Applicable Models U3741

U3751

U3771

U3772

Certificate of Conformity



This is to certify, that

Spectrum Analyzer

U3700 Series

instrument, type, designation

complies with the provisions of the EMC Directive 2004/108/EC in accordance with EN61326 and Low Voltage Directive 2006/95/EC in accordance with EN61010.

ADVANTEST Corp.

Tokyo, Japan

ROHDE&SCHWARZ International Operations GmbH

Munich, Germany

KC Class B

B 급 기기(가정용 방송통신기기)

이 기기는 가정용(B 급)으로 전자파적합등록을 한 기기로서 주로 가정에서 사용하는 것을 목적으로 하며, 모든 지역에서 사용할 수 있습니다.

Applicant: ADVANTEST corporation
 Registration No.: KCC-REM-qa2-U3772
 Equipment Name: Spectrum Analyzer

Basic Model Number: U3741/U3751/U3771/U3772
 Manufacturer: ADVANTEST corporation

• Country of Origin: Japan

• Year and month of manufacture: Refer to the product label

有害物质含量信息说明书

• 本说明书是为了贯彻 [电器电子产品有害物质限制使用管理办法] 而 编制的。 This document is made for Chinese Administration on the Control of Pollution Caused by Electronic Information Products, unofficially called "China-RoHS".

この文書は、中国の「電器電子製品有害物質使用制限管理弁法」のための文書です。

适用机种	U3741, U3751, U3771, U3772

1. 产品中贴有电子电气产品有害物质限制使用标志及产品中有害物质的名称及含量

由乙由层立旦右宝	部件名称	有害物质					
电子电气产品有害物质限制使用标志		铅 (Pb)	汞 (Hg)	镉 (Cd)	六价铬 (Cr(VI))	多溴联苯 (PBB)	多溴二苯醚 (PBDE)
	Main frame	X	0	0	0	0	0
	Boards	×	0	0	0	0	0
	Power supply parts	X	0	X	0	0	0
420	Cable	X	0	0	0	0	0
	LCD Panel	X	×	0	0	0	0
	Module	X	0	0	0	0	0
	Parts	X	0	0	0	0	0
	CD-ROM	0	0	0	0	0	0

本表格依据 SJ/T11364 的规定编制。

〇:表示该有害物质在该部件所有均质材料中的含量均在 GB/T26572 规定的限量要求以下。

×:表示该有害物质至少在该部件的某一均质材料中的含量超出 GB/T26572 规定的限量要求。(企业可在此处,根据实际情况对上表中打×的技术原因进行进一步说明。)

本表对此次发送产品中所有部件中有害物质的含量,全部作了注明。另外,也有可能包含了与本次发送的产品无关的部件的相关信息。

2. 环保使用期限内的使用条件

二 <i>比</i> 工4克	温度范围	0°C ~ +50°C
运作环境	相对湿度	在85%以下(但是,不得结霜)
沙里 亚拉	温度范围	-20°C ~ +60°C
设置环境	相对湿度	在85%以下(但是,不得结霜)
周围环境		不会产生腐蚀性气体的地方 不是直射阳关的地方 灰尘少的地方 没有震动的地方

TABLE OF CONTENTS

1.	INTRODUCTION1-1
1.1	Contents of This Manual
1.2	Product Overview
1.3	Conventions of Notation Used in This Document 1-2
1.4	Advantest Homepage 1-3
1,7	Advancest Homepage
2.	PRECAUTIONS WHEN USING THE U3700 2-1
2.1	If a Fault Occurs
2.2	Removing the Case 2-1
2.3	Electromagnetic Interference 2-1
2.4	Note when Turning on the Power
3.	SETUP
3.1	Inspection on Delivery
3.2	Locating This Instrument
3.2.1	Operating Environment 3-3
3.3	Power Supply
3.3.1	Using the AC Power Supply
3.3.1.1	AC Power Requirements
3.3.1.2	Connecting the Power Cable
3.3.2	Using a Battery
3.3.2.1	Battery Mount System 3-6
3.3.2.2	Charging the Battery 3-7
3.3.3 3.3.3.1	Using the External DC Power Supply 3-8 DC Power Requirements 3-8
3.3.3.2	Connecting the DC Power Cable
3.4	Caution when Connecting Peripherals
3.5	Checking Operations
	5
4.	INSTRUMENT CONFIGURATION AND BASIC OPERATIONS 4-1
4.1	Panel and Screen Descriptions 4-1
4.1.1	Names and Functions of Each Part on the Front Panel 4-1
4.1.2	Names and Functions of Each Part on the Screen 4-7
4.1.3 4.2	Names and Functions of Each Part on the Rear Panel 4-9 Basic Operation 4-10
4.2.1	Menu Operation and Data Entry 4-10
4.2.1	Basic Measurement 4-13
4.3.1	Calibration 4-13
4.3.2	Displaying Spectrum and Operating Markers 4-17
4.3.3	How to Cancel the UNCAL Message
4.3.4	Identifying an Image Signal 4-25
4.3.5	Hard Copy Output4-27
4.3.5.1	Output to a Printer 4-27
4.3.5.2	File Output to USB Memory

4.3.6 4.3.7	Measuring by using the TG (OPT76/OPT77)
4.4	Measurement Examples
4.4.1	Using the Normalize Function and Level Correction Table
4.4.2	W-CDMA Channel Power Measurement
4.4.3	W-CDMA Adjacent Channel Leakage Power (ACP) Measurement
4.4.4	W-CDMA Spurious Measurement
4.4.5	CN Measurement in Terrestrial Digital Broadcasting
4.4.6	Television Signal Measurement
4.4.7	VSWR Measurement
5.	MENU MAP, FUNCTIONAL EXPLANATION
5.1	Menu Index
5.2	Functional Descriptions
5.2.1	SYSTEM
5.2.2	APPLI
5.2.3	FILE
5.2.4	COPY
5.2.5	HELP
5.2.6	MEAS 1
5.2.7	MEAS 2
5.2.8	TRACE
5.2.9	MKR
5.2.10	PEAK
5.2.11	MKR→
5.2.12	TG (Option)
5.2.13	FREQUENCY
5.2.14	SPAN
5.2.15	AMPLITUDE
5.2.16	EXT CFG (Extended Configuration options)
5.2.17	CPL (Coupled function)
5.2.17	CI L (Coupled function)
6.	OVERVIEW OF REMOTE CONTROL
6.1	Remote Control
6.1.1	Types of Systems
6.1.2	Selecting the Command Set
6.2	GPIB Remote Control System
6.2.1	What is the GPIB?
6.2.2	Setting up the GPIB
6.2.3	GPIB Bus Functions
6.2.3.1	GPIB Interface Functions
6.2.3.2	
6.3	LAN Remote Control System
6.3.1	Setting up the LAN
6.3.2	Setting the IP Address
6.3.3	Control from a Controller
6.4	Message Exchanging Protocol
6.4.1	
0.4.1	Buffers

Message Exchange	6-10
	6-11
	6-11
	6-12
	6-13
	6-19
AT Command Index	6-19
AT Command List	6-25
Frequency	6-25
Level	6-27
Bandwidth	6-28
Sweep	6-29
Trigger	6-29
Trace	6-30
Pass/Fail	6-33
Display	6-34
Marker	6-35
Peak and Marker Move	6-37
Peak	6-38
Measurement	6-39
	6-42
	6-43
EMC	6-47
Calibration	6-47
Save/Recall	6-48
File Management	6-50
Config	6-50
	6-51
	6-51
Others	6-52
TG	6-53
Units	6-54
Example of Remote Control Programs	6-55
Basic Steps for GPIB Bus Control	6-55
Reading the GPIB Control Library for Visual Basic	6-55
	6-55
	6-58
	6-63
	6-70
Example Program Which Uses the TS (Take Sweep) Command	6-71
Example Programs Which Use the Status Byte	6-72
Program Examples Using the LAN	6-73
SCPI Command Reference	6-76
Command Reference Syntax	6-76
	6-78
	6-79
	6-79
	6-85
	6-86
4 Subsystem-COUPle	6-86
	Command Syntax Command Syntax Data Formatis Status Byte GPIB Remote Programming AT Command List Frequency Level Bandwidth Sweep Trigger Trace Pass/Fail Display Marker Peak and Marker Move Peak Measurement Counter Power EMC Calibration Save/Recall File Management Config Preset GPIB Others TG Units Example of Remote Control Programs Basic Steps for GPIB Bus Control Reading the GPIB Control Library for Visual Basic Programs Examples Using VB Sample Programs For Reading Data Sample Programs For Reading Data Sample Programs Which Uses the TS (Take Sweep) Command Example Program Which Uses the TS (Take Sweep) Command Example Program Which Uses the TS (Take Sweep) Command Example Program Which Uses the TS (Take Sweep) Command Example Program Which Uses the TS (Take Sweep) Command Example Programs Which Uses the TS (Take Sweep) Command Example Programs Which Uses the TS (Take Sweep) Command Example Programs Which Uses the TS (Take Sweep) Command Example Programs Which Uses the TS (Take Sweep) Command Example Programs Which Uses the TS (Take Sweep) Command Example Programs Which Uses the TS (Take Sweep) Command Example Programs Which Uses the TS (Take Sweep) Command Example Programs Which Uses the TS (Take Sweep) Command Example Programs Which Uses the TS (Take Sweep) Command Example Programs Which Uses the TS (Take Sweep) Command Example Programs Which Uses the TS (Take Sweep) Command Example Programs Which Uses the TS (Take Sweep) Command Example Programs Which Uses the TS (Take Sweep) Command Example Programs Examples Using the LAN SCPI Command Reference Command Reference Syntax Common Commands List of Commands Subsystem-CALCulate 2 Subsystem-CALIbration 3 Subsystem-CALIbration

6.10.3. 6.10.3. 6.10.3. 6.10.3. 6.10.3. 6.10.3. 6.10.3. 6.10.3. 6.10.3. 6.10.3. 6.10.3. 6.10.3. 6.10.3.	6 Subsystem-FETch 7 Subsystem-FORMat 8 Subsystem-HCOPy 9 Subsystem-INITiate 10 Subsystem-MMEMory 11 Subsystem-OUTPut 13 Subsystem-READ 14 Subsystem-SENSe 15 Subsystem-SOURce 16 Subsystem-SYSTem 17 Subsystem-TRACe 18 Subsystem-TRIGger 19 Subsystem-UNIT	6-1 6-1 6-1 6-1 6-1 6-1 6-1 6-1 6-1
7.	SPECIFICATIONS	7
7.1	U3741 Performance Specifications	7
7.1.1	Frequency	7
7.1.2	Sweep	7
7.1.3 7.1.4	Amplitude Accuracy	7 7
7.1.4	Amplitude Accuracy	7
7.1.5	Input and Output	7
7.1.0	U3751 Performance Specifications	7
7.2.1	Frequency	7
7.2.2	Sweep	7
7.2.3	Amplitude	7
7.2.4	Amplitude Accuracy	7
7.2.5	Dynamic Range	7
7.2.6	Input and Output	7
7.3	U3771/U3772 Performance Specifications	7-
7.3.1	Frequency	7-
7.3.2	Sweep	7-
7.3.3	Amplitude	7-
7.3.4	Amplitude Accuracy	7-
7.3.5	Dynamic Range	7-
7.3.6	Input and Output	7-
7.4	General Specifications	7-
7.5	Options	7-
7.5.1	Option 10 2-Channel Input	7-
7.5.2	Option 11 75 Ω 2-Channel Input (Can be Installed only in the U3741)	7-
7.5.3	Option 15 75 Ω Input	7-
7.5.4	Option 20 High Stability Frequency Reference	7-
7.5.5	Option 28 EMC Filter	7-
7.5.6	Option 53 Time Domain Analysis	_
	Option 54 2-Channel Time Domain Analysis	7-

7.5.7	Option 55 Wide Band Time Domain Analysis Option 56 2-Channel Wide Band Time Domain Analysis	-
7.5.8	Option 70 High C/N	
7.5.9	Option 71 2-Channel High C/N Option 75 75 Ω Tracking Generator	•
7.5.10	Option 76 Tracking Generator	
7.5.11	Option 77 6 GHz Tracking Generator	-
8.	OPTIONS AND ACCESSORIES	•
8.1	Options	
8.2	Accessories	•
9.	MAINTENANCE	
9.1	Cleaning	
9.1.1	Cabinet Cleaning	
9.1.2	Cleaning of Other Parts	
9.2	About Calibration	
9.3	About Replacement of Limited-Life Parts	
9.4	Method of Storing the Instrument	
9.5	Transportation	
9.6	Notes for Requesting Repair, Replacement of Parts, and Periodic Calibration	
9.6.1	Work Request	
9.6.2	Destination and Phone Number for Contact	
9.7	List of Error Messages	
9.8	In Case of Difficulty	
9.9	Product Disposal and Recycle	•
APPE	NDIX	•
A.1	Initial Setting List	
A.2	Principle of Operation	
A.2.1	Input Saturation	
A.2.2	Root Nyquist Filter	
A.3	Glossary	
A.4	dB Conversion Formula	
A.5	Menu Map List	
A.6	TV Channel Table (Japan)	
A.6.1	CATV Channel Number and Frequency	
A.6.2	VHF/UHF Channel Number and Frequency	•
A.6.3 A.6.4	Terrestrial Digital Broadcasting Channel Number and Frequency	
A.6.4 A.6.5	Satellite Broadcasting (BS-IF Band) Channel Number and Frequency	
U374	1 DIMENSIONAL OUTLINE DRAWING	. E
11275	1 DIMENGIONAL OUTLINE DRAWING	-
U3/3	1 DIMENSIONAL OUTLINE DRAWING	. E.

U3771 DIMENSIONAL OUTLINE DRAWING	. EXT-3
U3772 DIMENSIONAL OUTLINE DRAWING	. EXT-4
U3741/U3751/U3771/U3772 QUICK GUIDE	.GUIDE-1
ALPHABETICAL INDEX	. I-1

LIST OF ILLUSTRATIONS

No.	Title				
3-1	Operating Environment	3-:			
3-2	Connecting the Power Cable				
3-3	Attachment of a Ferrite Core 1				
3-4	Attachment of a Ferrite Core 2				
3-5	POWER Switch				
3-6	Initial Screen	3-1			
3-7	Connecting the CAL Signal	3-12			
4-1	Front Panel				
4-2	Extended Function Key Block				
4-3	Soft Key Block				
4-4	Input and Output Connectors Block				
4-5	Operation Key Block				
4-6	Screen Display				
4-7	Rear Panel				
4-8	Initial Setting Screen				
4-9	Connecting the CAL Signal (RF INPUT 1 connector)				
4-10	Connecting the CAL Signal (RF INPUT 2 connector)				
4-11	Connecting the CAL Signal				
4-12	Setting the Center Frequency	4-19			
4-13	Completing the Setting of the measurement conditions				
4-14	Displaying the Peak Search				
4-15	Measuring the Difference of Frequency and Level by Using the Delta Marker				
4-16	Connecting the CAL Signal				
4-17	Displaying the UNCAL Message				
4-18	Canceling the UNCAL Message				
4-19	Connecting the TG Mesurement				
4-20	Connecting the Unit Under Test				
4-21	Measurement Display for Channel Power	4-52			
4-22 4-23	Measurement Display for Noise Power Converted into 5.6 MHz BandwidthVSWR Measurement				
6-1	GPIB Connection				
6-2	LAN Setup				
6-3	Connection of Cross-over Cables				
6-4	Status Register Arrangement				
6-5	Details of Status Register	6-1:			
6-6	Structure of the Status Byte Register				
6-7	Relationship between the Screen Graticule and Trace Data	6-6.			
A-1	Block Diagram of the Input Section				
A-2	Relation Between Input and Output of the Mixer				
A-3	Characteristics of the Root Nyquist Filter				
A-4	Resolution Bandwidth				
A-5	IF Gain Uncertainty				
A-6	Noise Sidebands	A-8			

U3700 Series User's Guide

List of Illustrations

No.	Title	Page
A-7	Spurious Response	A-9
A-8	Occupied Bandwidth	A-10
A-9	Bandwidth Selectivity	A-10
A-10	Bandwidth Switching Uncertainty	A-11
A-11	VSWR	A-12

LIST OF TABLES

No.	Title	Page
3-1	Standard Accessories	3-2
3-2	Option Accessories	3-2
3-3	Power Requirements	3-4
4-1	USB Memory Devices Whose Operation with this Instrument has Already Checked	4-29
5-1	Character allocation table	5-22
6-1	GPIB Interface Functions	6-4
6-2	Connection of 10BASE-T Cross-over Cables	6-7
6-3	Connection of 10BASE-T Straight Cables	6-7
6-4	Trace Point Specification Codes	6-64
6-5	Binary Data Output Format Specified Code	6-64
6-6	I/O Format	6-65
6-7	Absolute Value Output Format	6-66
8-1	Options	8-1
8-2	Accessories	8-2
9-1	Limited-Life Parts	9-2

1. INTRODUCTION

This chapter describes the contents of this manual and the product overview of the U3700 series Spectrum Analyzer to help you get the most out of this manual.

1.1 Contents of This Manual

This manual can be used by novices or experienced users of this instrument. You may read through this manual from Chapter 1 to learn more about this instrument or you may refer to the table of contents, which is found at the beginning of each chapter and directly jump to the section that you need.

The contents of each chapter are as follows:

CHAPTER 1. INTRODUCTION	This chapter describes the contents of this manual and the product overview.
CHAPTER 2. PRECAUTIONS WHEN USING THE U3700	This chapter describes precautions when using this instrument. Read this chapter before using this instrument.
CHAPTER 3. SETUP	This chapter describes how to setup this instrument. After setting up this instrument in an appropriate location, turn on the power and check that this instrument starts correctly.
CHAPTER 4. INSTRUMENT CONFIGURATION AND BASIC OPERATIONS	This chapter describes the functions of each part of the panel and the screen of this instrument. You can learn how to operate this instrument from the operations and simple examples.
CHAPTER 5. MENU MAP, FUNCTIONAL EXPLANATION	This chapter describes the menu structure and functions of soft keys.
CHAPTER 6. OVERVIEW OF REMOTE CONTROL	This chapter describes how to connect and set the GPIB and LAN interfaces, and also describes the program examples used when programming and table of commands.
CHAPTER 7. SPECIFICATIONS	This chapter describes the specifications of this instrument.
CHAPTER 8. OPTIONS AND ACCESSORIES	This chapter describes options and accessories which are sold separately.
CHAPTER 9. MAINTENANCE	This chapter describes how to care for this instrument such as cleaning, calibration, and storage to maintain the high performance and smooth functioning of this instrument. Also this chapter describes how to identify problems and the relevant procedures to follow.
APPENDIX	This chapter describes the following information: Initial Setting List Principles of measurement Technical terms used in this manual Menu Map List

1.2 Product Overview

1.2 Product Overview

The U3700 series spectrum analyzers are compact, lightweight, and portable.

The U3700 series spectrum analyzers are ideal for use in the field because they operate on battery and can be used anywhere.

The main features of this instrument are as follows:

• Wide frequency measurement range

U3741: 9 kHz - 3 GHz U3751: 9 kHz - 8 GHz U3771: 9 kHz - 31.8 GHz U3772: 9 kHz - 43 GHz

· High-speed and high-accuracy sweep

Frequency span accuracy: 1% or less 20 ms sweep time

- Extremely low noise level:
 - -135 dBm @ 5 GHz (typical value, built-in preamplifier ON)
 - -120 dBm @ 40 GHz (typical value)
- High measurement level accuracy

±0.8 dB Frequency range 10 MHz - 3.1 GHz ±1.0 dB Frequency range 3.1 GHz - 8 GHz

- 3-way power supply system: AC, DC, and attachable battery
- Compact: Approximately 308 mm (W) × 175 mm (H) × 209 mm (D)
- Lightweight:

U3741: Approximately 5.0 kg or less (without option)
U3751: Approximately 5.6 kg or less (without option)
U3771/U3772: Approximately 6 kg or less (without option)

1.3 Conventions of Notation Used in This Document

The panel and soft key notations used in this manual are described below.

Panel key: Bold Example: FREQUENCY, SPAN

Soft keys: Bold italics Example: Center, Span

NOTE: Screen displays and diagrams such as external view of the main unit in this manual are those of the U3771 in the U3700 series.

1.4 Advantest Homepage

1.4 Advantest Homepage

The product information for the U3700 series Spectrum Analyzer is published on the Advantest homepage (http://www.advantest.co.jp).

On the homepage, sample software can be downloaded and the following information can be browsed: Application notes such as the GP-IB command table and technical notes.

How to access

Select "English", "PRODUCTS & SUPPORTS", "Electronic Measuring Instruments", and "Product" from the top page, and then choose a product model to be browsed.

2. PRECAUTIONS WHEN USING THE U3700

This chapter describes precautions when using this instrument. Read this chapter before using this instrument.

2.1 If a Fault Occurs

If any smoke, smell, or noise emanates from this instrument, turn off the MAIN POWER switch, remove the power cable from the AC power connector, and then contact an Advantest sales representative immediately.

2.2 Removing the Case

The case of this instrument should only be opened by Advantest service engineers.

2.3 Electromagnetic Interference

This instrument may cause electromagnetic interference and affect television and radio. If this instrument's power is turned off and any electromagnetic interference that may be present is reduced, then this instrument has caused the interference.

Electromagnetic interference from this instrument may be prevented by the following precautions.

- Changing the direction of the antenna of the television or radio.
- Placing this instrument on the other side of the television or radio.
- Placing this instrument away from the television or radio.
- Using a different power source for the television or radio, and this instrument.

2.4 Note when Turning on the Power

When turning on the power, do not connect a DUT to this instrument.

3. SETUP

This chapter describes how to set up this instrument on delivery. Topics covered in this chapter are:

- 3.1 Inspection on Delivery
- 3.2 Locating This Instrument
- 3.3 Power Supply
- 3.4 Caution when Connecting Peripherals
- 3.5 Checking Operations

3.1 Inspection on Delivery

After receiving the product, inspect the outside and the accessories according to the following procedure.

1. Check that the shipping container and the cushioning material are not damaged.

IMPORTANT: If the shipping container or the cushioning material is damaged, keep them until the following inspections are complete.

2. Check that the outside of the product is not damaged.

WARNING: If any outside components of the product such as the cover, panel (front or rear), LCD display, power switch, or connector are damaged, do not turn on the power. You may receive an electrical shock.

3. Check that the standard accessories listed in Table 3-1 (and option accesories listed in Table 3-2) are complete and they are not damaged.

If any of the following occur, contact an Advantest sales representative.

- The shipping container or the cushioning material is damaged, or signs of stress are found.
- The outside of the product is damaged.
- The standard accessories are incomplete or are damaged.
- Defects are found in the operation check.

3.1 Inspection on Delivery

Table 3-1 Standard Accessories

Name	Model	Quantity			
		U3741	U3751	U3771/U3772	
Power cable	A01412	1	1	1	
Input cable (50 Ω)	A01037-0300	1*1	1	1	
N(m)-BNC(f) adaptor	JUG-201A/U	1*1	1	1	
Ferrite core	ESD-SR-120	3	3	3	
Ferrite core	E04SR150718	1	1	1	
BNC-SMA adaptor	HRM-517	0	0	1	
Adapter for RF INPUT 2	HE-A-PJ	0	0	1	
U3700 Series User's Guide	BU3700S	1	1	1	

^{*1} The quantity decreases to zero when the 75 Ω option (OPT11/OPT15) is included.

Table 3-2 Option Accessories

Name	Model	Quantity				
		OPT10	OPT11	OPT15	OPT75	OPT76/ OPT77
Input cable (75 Ω)	A01045	0	1	1	0	0
N(m)-BNC(f) adaptor	JUG-201A/U	1*1	0	0	0	1
C15-type adapter	NCP-NFJ	0	2	1	1	0
NC-BNC adapter	BA-A165	0	2	1	1	0

^{*1} The quantity decreases to zero for the U3771 and U3772.

3.2 Locating This Instrument

This section describes the installation environment in which this instrument runs successfully.

3.2.1 Operating Environment

Install this instrument in an environment in which the following conditions are satisfied.

- Ambient temperature: 0°C to +50°C (operating temperature) -20°C to +60°C (storage temperature)
- Relative humidity: 85 percent or less with no condensation
- An area free from corrosive gas
- An area away from direct sunlight
- · A dust-free area
- An area free from vibrations
- A low noise area

Although this instrument has been designed to withstand a certain amount of noise from the AC power line, it should be used in a low noise area.

Use a noise cut filter if ambient noise is unavoidable.

• An area in which the airflow is not obstructed

There is an exhaust-cooling fan and exhaust vents on both sides of this instrument. Do not obstruct the fan and vents. If there is insufficient airflow around the vents, the internal temperature will rise and the instrument may operate incorrectly. Keep a space of 10 centimeters between the side panel and the wall. Do not use this instrument on its side.

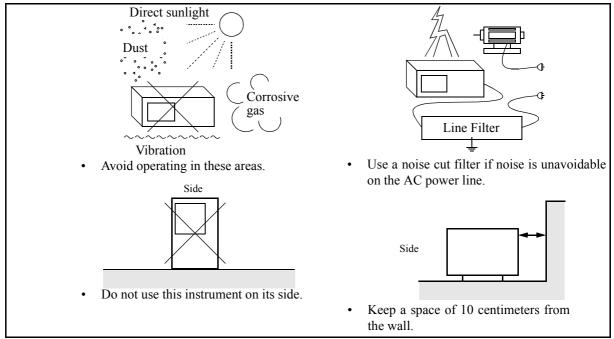


Figure 3-1 Operating Environment

3.3 Power Supply

3.3 Power Supply

This instrument can use the following three types of power sources.

An AC Power Supply
 Automatically switches the power supply voltage between 100 V AC and 200 V AC.

A battery

Use an external battery pack (A870008).

Recommended battery pack: DIONIC90 (Manufactured by Anton Bauer Inc.)

• An external DC power supply

Use an external DC power cable (A114020).

CAUTION: Connect this instrument to an AC power supply, DC power supply, or battery.

3.3.1 Using the AC Power Supply

This section describes power requirements and how to connect the power cable.

3.3.1.1 AC Power Requirements

The AC power requirements of this instrument are shown in Table 3-3. Check that the power supply, which is supplied to this instrument, satisfies the conditions shown in Table 3-3.

Table 3-3 Power Requirements

	100 V AC	200 V AC	Remarks
Power supply voltage range	90 V - 132 V	198 V - 264 V	Automatically switches
Frequency range	47 Hz	the input voltage between 100 V AC and 200 V AC	
Power consumption	100 VA	- 100 V 110 unu 200 V 110.	

WARNING: Make sure the power supply, which is supplied to this instrument, satisfies the power requirements. If the power requirements are not satisfied, this instrument may be damaged.

3.3.1 Using the AC Power Supply

3.3.1.2 Connecting the Power Cable

This instrument includes a three-core power cable with a grounding conductor. To prevent accidents caused by electric shocks, use the included power cable and securely connect to the ground through a three-pin power outlet.

1. Check that the included power cable is not damaged.

WARNING: Never use a damaged power cable. You may receive an electrical shock.

2. Connect the AC power connector on the rear panel of this instrument to a threepin power outlet that has a protected ground terminal by using the included power cable (See Figure 3-2).

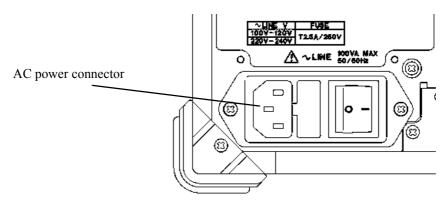


Figure 3-2 Connecting the Power Cable

WARNING:

- Use a suitable power cable for the power supply voltage. Use a power cable that complies with the safety standards in your country (Refer to "Safety Summary").
- To prevent any danger of electrical shock, connect the power cable to a three-pin power outlet that is connected to a protected ground terminal. The instrument will not be grounded if an extension cord, which does not include a protected ground terminal, is used.

3.3.2 Using a Battery

3.3.2 Using a Battery

The U3700 series can use a battery as a power source.

An Anton Bauer's battery pack can be used in the U3700 series. The DIONIC 90 compact lithium-ion battery pack is recommended.



The DIONIC 90 battery pack specifications

Capacity: 90 WH Nominal

Output voltage:14.4 V

Weight: Approx. 0.7 kgDimensions: $133 \times 89 \times 54 \text{ mm}$

For more information, refer to the battery pack operation manual.

INFORMATION:Runtime (hours) U3741: 3 hours U3751: 2.5 hours

U3771/72: 2 hours

NOTE: The battery life varies depending on the usage situation.

If using a battery stored over the long term, check the runtime in advance.


3.3.2.1 Battery Mount System

The QR Gold Mount System, which is included in professional video cameras worldwide, is included in this instrument.

1. How to remove and replace the battery pack

Align the side of the battery pack that contains the connector with the battery mount on the rear panel of this instrument and push it in and down. The battery is attached when a "click" is heard.

Turn off the power supply of this instrument when detaching the battery. To detach the battery, lift the battery up while pushing the eject button on the battery mount.

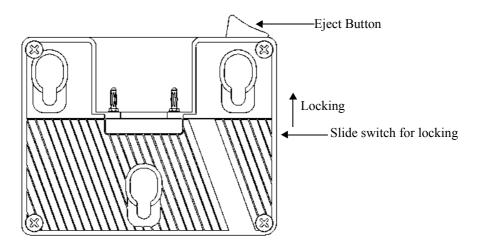

2. Locking the Eject button

The slide switch to lock the Eject button is located on the right side of the battery mount (lower side of the Eject button). The Eject button is locked by setting the slide switch to upper side. Set the slide switch to the lower side and release the lock before the battery pack is attached or detached.

3.3.2.2 Charging the Battery

This instrument cannot charge the external battery pack.

Use a suitable battery charger for the battery pack.

• For the DIONIC 90

The TITAN TWIN charger (A870009) is recommended. When the TITAN TWIN charger is used, the charging time is approximately 5.5 hours.



3.3.3 Using the External DC Power Supply

3.3.3 Using the External DC Power Supply

3.3.3.1 DC Power Requirements


DC power supply	Requirements
Power supply voltage range	+11 V to +17 V
Power consumption	70 W or less

3.3.3.2 Connecting the DC Power Cable

- 1. Remove the AC power cable and detach the battery.
- 2. Connect an A114020 (Sold separately) external DC power cable to the DC power supply input connector on the rear panel.

CAUTION: Do not reverse the polarity of the DC power supply.

3. To remove the DC power cable, turn off the power supply of this instrument and remove the external DC power cable while pushing the button on the cable connector.

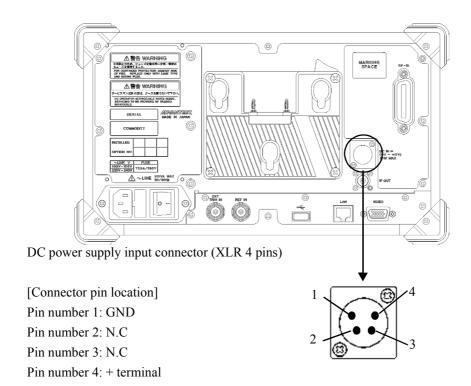

3-8

3.4 Caution when Connecting Peripherals

Use shielded cables when connecting peripherals to the USB and LAN connectors on this instrument. Attach the included ferrite core (ESD-SR-120) to the cable.



Figure 3-3 Attachment of a Ferrite Core 1

When connecting an earphone to the PHONE connector, attach the included ferrite core (E04SR150718) to the earphone cable.



Figure 3-4 Attachment of a Ferrite Core 2

3.5 Checking Operations

3.5 Checking Operations

This section describes how to check operations by using the calibration function of this instrument. Check that this instrument operates correctly by following the procedure below.

Starting this instrument

- 1. Connect the power cable according to "3.3.1.2 Connecting the Power Cable".
- 2. Turn on the AC power switch on the rear panel.
- 3. Three seconds after turning on the AC power switch on the rear panel, press the power switch on the front panel to turn on the instrument. The power supply and the green power light turn on.




Figure 3-5 POWER Switch

4. The system boots up and the program starts.

3.5 Checking Operations

5. The result of the self-diagnostics and the initial screen are displayed. The initial screen display may differ from Figure 3-6 depending on the status of the settings when the power supply was last turned off.

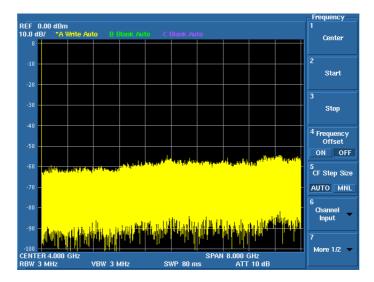


Figure 3-6 Initial Screen

MEMO: If any error message is displayed, refer to "9. MAINTENANCE".

3.5 Checking Operations

Running calibration

Connect as shown in Figure 3-7 by using the included N-BNC adaptor and input cable (A01037-300).

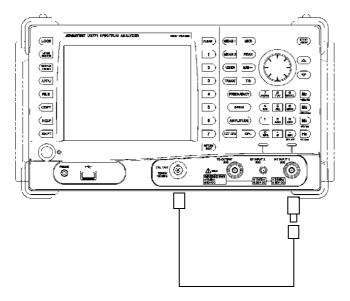


Figure 3-7 Connecting the CAL Signal

IMPORTANT: Perform calibration after allowing a warm up time of at least 5 minutes.

For more information on how to perform autocalibration, refer to "4.3.1 Calibration".

- 7. Press the **SYSTEM** key of this instrument and select *Calibration* from the soft
- 8. Select *Calibrate ALL* on the next soft menu. It takes approximately two minutes to complete the autocalibration.
- 9. Check that no error message is displayed at the end of the calibration.

MEMO: If any error message is displayed, refer to "9. MAINTENANCE".

Turning off the power supply

10. Press the power switch on the front panel. The power supply and the power light turn off.

4. INSTRUMENT CONFIGURATION AND BASIC OPERATIONS

This chapter describes the functions of each part on the panels and screen, and describes the basic operations of this instrument by using measurement examples.

4.1 Panel and Screen Descriptions

This section describes the names and functions of each part on the front panel, screen, and rear panel.

4.1.1 Names and Functions of Each Part on the Front Panel

This section describes the names and functions of each part on the front panel.

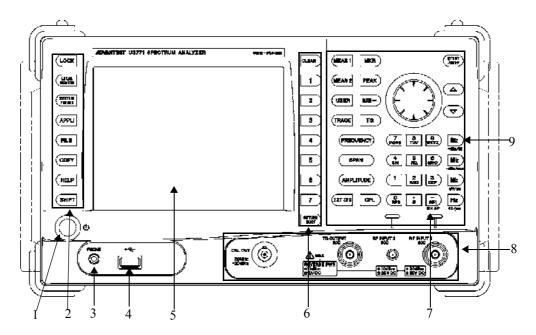


Figure 4-1 Front Panel

1.	POWER switch with lamp	Switches the power supply between ON and OFF. The lamp turns on while the power turns on
2.	Extended function key block	The keys in this block set the extended functions.
3.	PHONE connector	8-ohm earphone terminal for demodulated AM/FM audio signals.
4.	USB connector	Enables a memory device or printer to be connected.
5.	Color LCD	Displays measurement data or setting conditions.
6.	Soft key block	The keys in this block select items from the soft menu on the display.

7. Input connector lamp Indicates the input connector is enabled. U3741/U3751: Only RF INPUT 1 is enabled.

- 8. Input and output connectors block The connectors in this block are used in measurements.
- 9. Operation key block The keys in this block are used for changing settings.

LOCK 1 2 LOCAL REMOTE SYSTEM PRESET 3 4 APPLI 5 FILE 6 COPY 7 HELP 8 SHIFT

Figure 4-2 Extended Function Key Block

1. Key lock key with lamp

Locks the key input.

Toggles the key lock between ON and OFF.
The lamp turns on while the key input is locked.

2. LOCAL key Cancels the remote control function.

REMOTE lamp The lamp turns on when the instrument is in the remote state.

3. SYSTEM setting Sets the operational conditions of an interface.

Preset key Initializes the settings of this instrument.

4. APPLICATION key Switches between the applications of this instrument.

5. FILE key Loads and saves data.

6. COPY key Outputs screen data.

7. HELP key Explains the soft menu.

NOTE: HELP is loaded and functions when the HELP key is pressed at the first time after the power is turned on.

8. SHIFT key with lamp Sets the shift mode which allows the functions indicated by the green font to be selected.

Turns on while the shift mode is set.

4-2

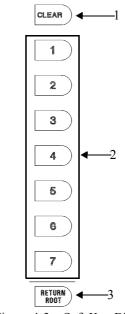


Figure 4-3 Soft Key Block

1. CLEAR key Cancels data entry mode.

The soft key 1 to 7 correspond with the soft menu 1 to 7 indicated to the left respectively. Press the soft key to select the soft menu. 2. Soft menu key

3. RETURN key Returns to the previous soft menu.

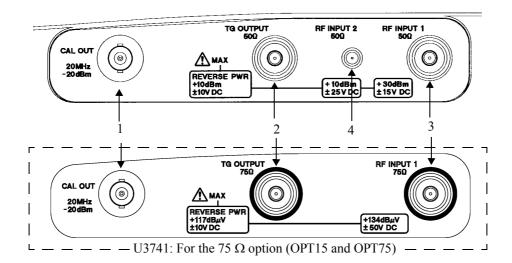


Figure 4-4 Input and Output Connectors Block

1. CAL OUT connector Outputs the calibration signal.

2. TG OUTPUT connector Outputs the tracking generator signal. (Option)

3. RF INPUT 1 connector Input the signal to be measured.

Measurement frequency range:

U3741: 9 kHz - 3 GHz

U3751/U3771/U3772: 9 kHz - 8 GHz

4. RF INPUT 2 connector Input the signal to be measured.

Measurement frequency range U3771: 10 MHz - 31.8 GHz U3772: 10 MHz - 43 GHz

CAUTION:

- Do not apply an RF power or DC voltage that exceeds the limited value to the INPUT and OUTPUT connectors.
 - Be careful of static electricity. Internal circuit components such as the input attenuator and mixer may be damaged.
- The precision microwave connector is used as the RF INPUT 2 connector.
 This connector is compatible with the K connector (K connector is a trademark of Anritsu Corporation.)
 and can be connected to a common SMA connector.
 - Be careful when handling this connector because the connector is delicate and is damaged easily. Use the included adapter (HE-A-PJ) if the connection and disconnection to this connector are performed frequently.
- 3. For the 75 Ω option (OPT15 and OPT75), input and output connectors are changed to 75 Ω type connectors.
 - If a 50 Ω cable or connector is connected to a 75 Ω connector, the center contact of the 75 Ω connector may be damaged.
 - Verify that cables and connectors, which are used, are 75 Ω type.

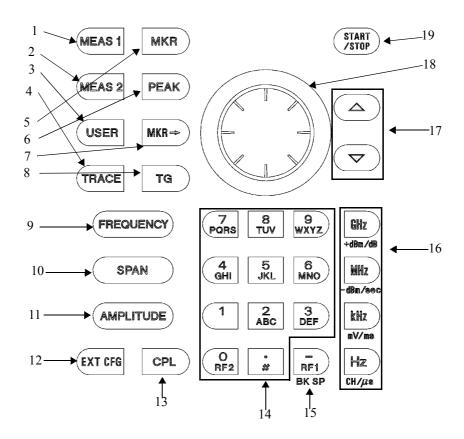


Figure 4-5 Operation Key Block

1.	MEAS 1	Selects a measurement such as Channel Power, OBW or ACP.
2.	MEAS 2	Selects a measurement such as Noise/Hz, X dB down or Counter.
3.	USER	Allocates soft menu keys to be used.
4.	TRACE	Sets the trace function.
5.	MKR	Displays the marker.
6.	PEAK	Searches for a peak on a trace.
7.	$MKR \rightarrow$	Sets the values of the marker to that of another function.
8.	TG	Sets the tracking generator. (Option)
9.	FREQUENCY	Sets the center frequency.
10.	SPAN	Sets the frequency span.
11.	AMPLITUDE	Sets the level.
12.	EXT CFG	Sets the sweep mode and trigger.
13.	CPL	Sets the RBW, VBW, and sweep time.

14. Keypad There are numeric keys (0 to 9) and decimal point key.

15. - (Backspace)key Enters the minus sign and corrects entered data.

16. Unit key Selects a unit and determines the entered value.

GHz Sets a unit of GHz, +dBm, or dB.

MHz Sets a unit of MHz, -dBm, sec, V, or W.

kHzSets a unit of kHz, mV, msec, or mW.HzSets a unit of Hz, μsec, CH, μV, or μW.

Can also be used as the ENTER key

17. Step key Enters data at each step.

18. Data knob Fine tunes the entered data.

19. START/STOP key Starts or stops the sweep.

4.1.2 Names and Functions of Each Part on the Screen

This section describes the names and functions of each part on the screen of this instrument.

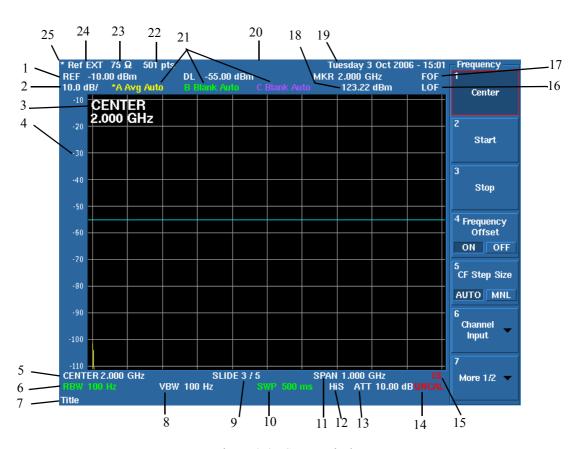


Figure 4-6 Screen Display

- 1. Reference level Displays the reference level setting value.
- 2. Amplitude scale in log mode or linear mode

Displays the amplitude scale setting in log mode.

- 3. Active function Displays the function enabled by the keypad or data knob.
- 4. Level scale Displays the level scale.
- 5. Center frequency or start frequency

Displays the center frequency or start frequency.

6. Resolution bandwidth (RBW) Displays the resolution bandwidth setting value.

Displays the font color of RBW in green if RBW is set in the man-

ual mode.

- 7. User's title Displays the description of the details of the measured data.
- 8. Video bandwidth (VBW) Displays the video bandwidth setting value.

Displays the font color of VBW in green if VBW is set in the man-

ual mode.

4.1.2 Names and Functions of Each Part on the Screen

9. Number of times averaging is performed

Displays the set and current number of times averaging is per-

formed.

10. Sweep time Displays the sweep time setting value.

Displays the font color of SWP in green if SWP is set in the man-

ual mode.

11. Frequency span or stop frequency Displays the frequency span or stop frequency.

12. High-sensitivity (Hi-sensitivity) Displays HiS while the preamplifier is set to On.

13. RF attenuator Displays the attenuator setting value.

Displays the font color of ATT in green if ATT is set in the manual

mode.

14. UNCAL message Displays UNCAL while the manual settings are inappropriate.

15. Image Suppression Displays IS while the image suppression function is set to On.

16. Level offset Displays LOF while the reference offset is set to On.

17. Frequency offset Displays FOF while the frequency offset is set to On.

18. Marker area Displays the marker frequency (time) and level.

19. Date Displays the current date and time.

20. Measurement function display Displays the currently performed measurement function.

21. Trace and trace detector Displays the selected trace mode and trace detector mode.

The trace with * displayed at the beginning is the active trace. For a display of two traces or more, the trace with * is displayed

at the front.

22. Trace point Displays "501 pts" while the number of trace points is set to 501

points

23. Input impedance 75 Ω Displays "75 Ω " while the Input Impedance is set to 75 Ω .

24. External reference signal Displays Ref EX1 while the external reference signal is selected.

25. R3162/R3131 mode ON R3131 mode: Displays "*" while the R3131 mode is set to ON in

U3741.

R3162 mode: Displays "*" while the R3162 mode is set to ON in

U3751/U3771/U3772.

This section describes the names and functions of each part on the rear panel.

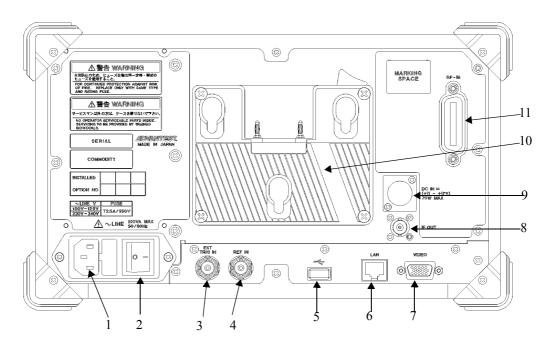


Figure 4-7 Rear Panel

1.	AC power connector	Connects this instrument to the AC power supply by using the included power cable.
2.	AC power switch	Switches the AC power ON and OFF.
3.	EXT TRIG connector	Inputs the external trigger signal (TTL level).
4.	EXT REF connector	Inputs the external reference signal.
5.	USB A connector	Enables a memory device or printer to be connected.
6.	LAN connector	For 10BaseT-specific LAN connector
7.	VIDEO connector	Connects to the monitor for VGA specification.
8.	IF OUT connector	Outputs an IF signal of 21.4 MHz.
9.	DC INPUT connector	Connects to the external DC power supply.
10.	Battery mount	The Anton Bauer's battery pack can be used.
11.	GP-IB connector	Connects to the external controller when the remote-control is used through the GPIB interface.

4.2 Basic Operation

4.2 Basic Operation

This section describes the menu operation, data entry, and usage of the basic measurement functions.

4.2.1 Menu Operation and Data Entry

Panel keys and soft menus are used to operate this instrument.

Press a panel key to display its menu to the right of the screen. Certain panel keys such as the LOCAL key do not display a soft menu.

The menu items are arranged according to the soft keys.

The number of the menu item accords with the number of the related soft key.

Press a soft key to select the related menu.

Certain soft keys display another menu.

The following describes the functions of the panel key and soft key.

1. Selecting a menu

To set the measurement conditions, press the panel key and select the menu.

Press AMPLITUDE.

The reference level setting value is displayed in the active function display area and the following Level menu is displayed to the right of the screen.

1 Ref Level

 $2 ATT \nabla$

3 dB/div ▼

4 Vertical Scale LIN/LOG

5 Units ▼

6 Slide Screen ON/OFF

7 More 1/2 ▼

The frame of the *1 Ref Level* menu is displayed in red. This red frame menu means that data can be entered.

2. Data entry

If the set value is displayed in the active function display area, it can be changed by using keypad, step key, or data knob.

• Data entry by using the keypad

Enter data by using the keypad, decimal point key, BK SP (backspace) key, and minus (-) key. If any wrong numbers are entered by using the keypad, use the BK SP to delete a character to the left and enter the correct number. If no data is entered and BK SP is pressed, "- (minus)" is entered

After entering data, press the unit key (ENTER) to complete the entry.

If any other panel key is pressed before the unit key is pressed, any entered data becomes invalid.

Example: Set the reference level to -20 dBm by using the keypad.

Press -, 2, 0, GHz(+dBM) or 2, 0, MHz(-dBM).

4.2.1 Menu Operation and Data Entry

• Data entry by using the step key

The step key enters data in the defined step size. Pressing ▼ decreases data and pressing ▲ increase data.

Example: Set the reference level to 0.0 dBm by using the step key.

Press the step key ▲. The reference level is set to -10.0 dBm. Press the step

key ▲ again to set to 0.0 dBm.

Data entry by using the data knob

The data knob enters data in the determined display resolution. The data knob is available for the fine adjustment of the entry data.

Example: Set the reference level to 0.5 dBm by using the data knob.

Rotating the data knob in the clockwise direction increases the reference level in steps of 0.1 dBm. Rotate the data knob until the display of the active function display area shows 0.5 dBm.

Rotating the data knob in the counterclockwise direction decreases the refer-

ence level in steps of 0.1 dBm.

ACTIVE OFF

Pressing the CLEAR key hides the active function display area.

Data cannot be entered if the active function display area is hidden.

To redisplay the active function display area, press a panel key or soft key.

3. Menu layer

Certain soft menus have ▼ at the right end and the sub menu is displayed by pressing the soft key. Certain soft menus such as ON/OFF or AUTO/MNL switch the setting by pressing the soft key.

Press MKR. The following Marker menu is displayed.

- 1 Select Marker
- 2 Marker ON/OFF
- 3 Marker Trace A/B/C
- 4 Delta Mode ▼
- 5 Peak Menu ▼
- 6 Clear All
- 7 More 1/2 ▼

Switching the setting

If a menu includes a dual-state button such as ON/OFF or AUTO/MNL, the state can be switched by pressing the soft key. The selected setting is displayed convexly.

The non-selected setting is displayed concavely.

Example: Press 2 Marker ON/OFF.

The setting is turned OFF and the markers disappear.

Press 2 Marker ON/OFF again to turn the setting ON and the markers re-ap-

pear.

Sub menu display

Pressing a soft key, which has ▼ to the right of the menu, displays a sub menu.

Example: Press 4 **Delta Mode** ▼. The following Peak menu is displayed.

1 Delta ON/OFF

4.2.1 Menu Operation and Data Entry

RETURN

Press **RETURN** to return to the previous menu from the sub menu.

4. Using SHIFT

The SHIFT key is used for selecting functions, which are indicated in green on the key.

These functions are described below.

PRESET Returns to the initial settings.

ROOT Returns the soft menu to the top menu.
RF1 Selects RF INPUT 1. (U3771/U3772)
RF2 Selects RF INPUT 2. (U3771/U3772)

To perform the function, which is written on the key in green, press the **SHIFT** key and then press each key.

Pressing the **SHIFT** key turns on its LED and the shift mode is available.

Press the **SHIFT** key again to cancel the shift mode. The green LED turns off and the shift mode is unavailable.

Other keys

Nothing is printed on these keys, but they have the functions shown below.

• USER Sets and cancels the USER menu.

COPY Displays the Copy menu.

• Select Marker Returns one selected marker number.

5. Displaying a dialog box

Pressing certain soft keys displays a dialog box.

- Selecting items Select the horizontal items by using the data knob and select the vertical items by using the step keys.
- Entering numeric values

Enter values by using the keypad and unit key.

Determining the setting

Press the unit key (ENTER) to determine.

4.3 Basic Measurement

4.3 Basic Measurement

This section uses the following measurement examples to describes basic measurement procedures which will allow the user to become familiar with the operation of this instrument.

- 4.3.1 Calibration
- 4.3.2 Displaying Spectrum and Operating Markers
- 4.3.3 How to Cancel the UNCAL Message
- 4.3.4 Identifying an Image Signal
- 4.3.5 Hard Copy Output

4.3.1 Calibration

Correcting the measurement by using the calibration factor, which is acquired from the calibration, can increase the measurement accuracy.

Calibration items

- Total Gain
 Measuring the calibration signal of -20 dBm and acquiring the level difference
- 2. Step ATT Minimizing the level error when switching STEP ATT at 20 MHz
- RBW
 Optimizing the RBW adjustment and minimizing the level error when switching RBW
- 4. PBW (Noise power bandwidth)

IMPORTANT: Perform calibration after allowing a warm up time of 5 minutes or more.

Required equipment

This instrument

Conversion adaptor: N (m)-BNC (f) Conversion adaptor: BNC (f)-SMA (m) Input cable: BNC (m)-BNC (m)

4.3.1 Calibration

Turning on the power supply

- 1. Verify that the AC power switch on the rear panel is set to OFF.
- 2. Connect the included power cable to the AC power connector on the rear panel.

CAUTION: To prevent damage, do not supply a voltage and frequency, which exceed the specified range, to this instrument.

- 3. Connect the power cable to an electrical outlet.
- 4. Turn on the AC power switch on the rear panel.
 After turning on the AC power switch, wait for three seconds or more
- 5. Turn on the power switch on the front panel.

MEMO: The display may be different depending on the state of the instrument when the power was last turned off.

NOTE: Before turning the power on, remove the USB memory key.

Otherwise, the system does not start.

Initialization

Initializes the settings of this instrument.

5. Press **SHIFT** and **SYSTEM(PRESET)**. Initial setting conditions are loaded.

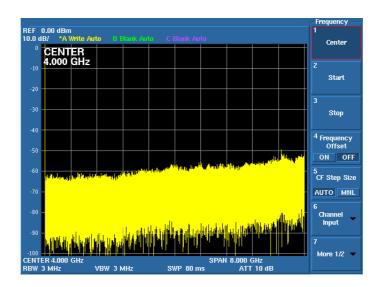


Figure 4-8 Initial Setting Screen

Selecting the input connector

For the U3741 and U3751, only RF INPUT 1 can be used as the input connector. No need to select the input connector.

For the U3771 and U3772, select the input to be performed the calibration.

Press **SHIFT** and **- (RF1)**. RF INPUT 1 is selected. Press **SHIFT** and **0 (RF2)**. RF INPUT 2 is selected.

The calibration of either RF INPUT 1 or RF INPUT 2 can be performed first.

The following describes the procedure in which the calibration of RF INPUT 1 is performed first.

Connecting the input signal

Connect the calibration signal.

7. Attach the N(m)-BNC(f) adaptor to the RF INPUT 1 connector on the front panel. Connect the included BNC (m)-BNC (m) input cable to the CAL OUT connector on the front panel and the N(m)-BNC(f) adaptor.

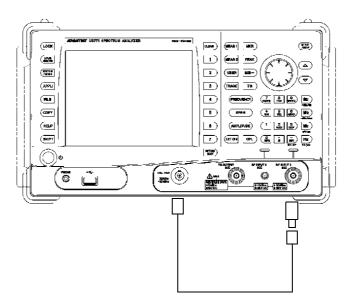


Figure 4-9 Connecting the CAL Signal (RF INPUT 1 connector)

- 8. Press **SYSTEM**.
- 9. Press *6 Calibration* on the soft key menu. The Calibration menu is displayed.

4.3.1 Calibration

10. Press *Calibrate All* on the Calibration menu.

Calibration starts.

The following message is displayed if the calibration of RF INPUT 1 is complete.

First step of calibration completed.

Connect the calibrator to RF2 connector.

Then press OK to continue.

The calibration is canceled if **Hz** is pressed.

To perform the calibration of RF INPUT 2, change the cable connection.

11. Attach the BNC(f)-SMA(m) adapter to the RF INPUT 2 connector on the front

panel.
Connect the included BNC(m)-BNC(m) input cable to the CAL OUT connector on the front panel and the BNC(f)-SMA(m) adapter.

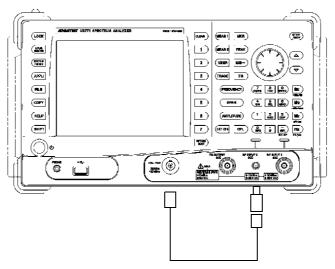


Figure 4-10 Connecting the CAL Signal (RF INPUT 2 connector)

12. Press ▼ and select OK.

Press Hz to start the calibration.

4.3.2 Displaying Spectrum and Operating Markers

This section describes how to display spectrums and use markers by using the CAL signal of this instrument.

The level difference between the CAL signal and its second harmonics are measured as an example.

Required equipment

This instrument Conversion adaptor: N (m)-BNC (f) Input cable: BNC (m)-BNC (m)

Turning on the power supply

IMPORTANT: Use this instrument within a specified temperature range to perform accurate measurements. Perform calibration after allowing a warm up time of 5 minutes or more.

- 1. Verify that the AC power switch on the rear panel is set to OFF.
- 2. Connect the included power cable to the AC power connector on the rear panel.

CAUTION: To prevent damage, do not supply a voltage and frequency, which exceed the specified range, to this instrument.

- 3. Connect the power cable to an electrical outlet.
- 4. Turn on the AC power switch on the rear panel.
 After turning on the AC power switch, wait for three seconds or more.
- 5. Turn on the power switch on the front panel.

MEMO: The display may be different depending on the state of the instrument when the power was last turned off.

Initialization

Initialize the settings of this instrument.

6. Press **SHIFT** and **SYSTEM(PRESET)**. Initial setting conditions are loaded.

Connecting the input signal

Connecting the calibration signal.

7. Attach the N(m)-BNC(f) adaptor to the INPUT connector on the front panel. Connect the included BNC (m)-BNC (m) input cable to the CAL OUT connector on the front panel and the N(m)-BNC(f) adaptor.

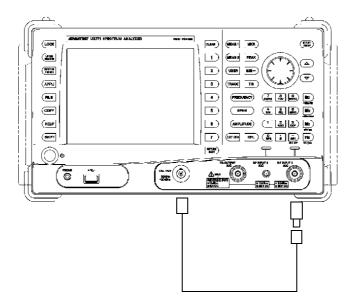


Figure 4-11 Connecting the CAL Signal

Setting measurement conditions

Setting the measurement conditions to observe the input signal more easily.

After initialization, the center frequency can be set.

8. Press **3**, **0**, and **MHz**. The center frequency is set to 30 MHz.

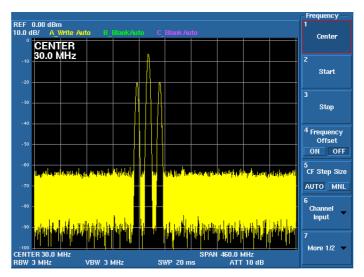


Figure 4-12 Setting the Center Frequency

9. Press SPAN.

The current frequency span is displayed in the active function display area and the Span menu is displayed.

10. Press 4, 0, and MHz.

The frequency span is set to 40 MHz.

11. Press AMPLITUDE.

The current reference level is displayed in the active function display area and the Level menu is displayed.

12. Press -, 1, 0, and GHz(dBm).

The reference level is set to -10 dBm.

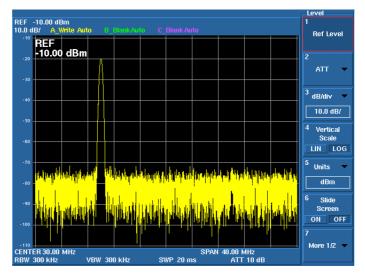


Figure 4-13 Completing the Setting of the measurement conditions

Displaying a marker on the peak

13. Press PEAK.

The marker is displayed on the peak and the frequency (approximately 20 MHz) and level (approximately -20 dBm) of the marker are displayed in the marker area

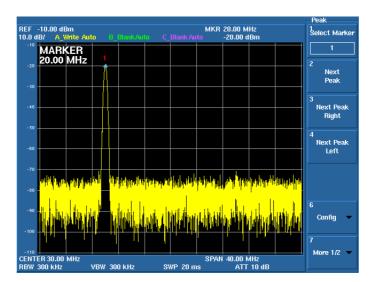


Figure 4-14 Displaying the Peak Search

Displaying a delta marker

14. Press MKR.

The Marker menu used for the marker function is displayed.

Press 4 Delta Mode.

Press 1 Delta ON/OFF.

The delta marker is displayed and the frequency difference and level difference between the marker and delta marker are displayed in the marker area.

MKΔ 0 Hz

0.00 dB

15. Press 2, 0, and MHz.

The active marker is displayed on the second harmonics, which is 20 MHz away from the CAL signal.

The differences of frequency and level between two signals are displayed in the marker area.

 $MK\Delta 20.00 MHz$

-52.21 dB

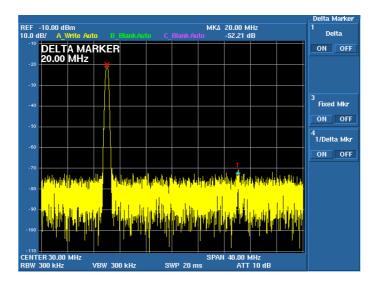


Figure 4-15 Measuring the Difference of Frequency and Level by Using the Delta Marker

4.3.3 How to Cancel the UNCAL Message

4.3.3 How to Cancel the UNCAL Message

The setting among the resolution bandwidth (RBW), video bandwidth (VBW), frequency span (Span), and sweep time (Sweep Time) affect to each other.

If the combination of these settings in the manual setting is inappropriate, the UNCAL message is displayed at the bottom to the right of the scale. If the UNCAL message is displayed, the measurement level accuracy cannot be guaranteed.

Change the following settings to cancel the UNCAL message.

- Expand the resolution bandwidth (RBW).
- Expand the video bandwidth (VBW).
- Slow the sweep time (Sweep Time).
- If RBW or VBW cannot be changed, narrow the frequency span (Span).

IMPORTANT: Accurate measurement data cannot be acquired while the UNCAL message is displayed.

This section describes how to cancel the UNCAL message, which was generated because of the fast sweep time, by changing the RBW setting.

Required instruments

This instrument Conversion adaptor: N (m)-BNC (f) Input cable: BNC (m)-BNC (m)

Turning on the power supply

IMPORTANT: Use this instrument within the specified temperature range to perform accurate measurements.

Perform calibration after allowing a warm up time of 5 minutes or more.

- 1. Verify that the AC power switch on the rear panel is set to OFF.
- 2. Connect the included power cable to the AC power connector on the rear panel.

CAUTION: To prevent damage, do not supply a voltage and frequency, which exceed the specified range, to this instrument.

- 3. Connect the power cable to an electrical outlet.
- 4. Turn on the AC power switch on the rear panel.
 After turning on the AC power switch, wait for three seconds or more.
- 5. Turn on the power switch on the front panel.

MEMO: The display may be different depending on the state of the instrument when the power was last turned off.

4.3.3 How to Cancel the UNCAL Message

Initialization

Initialize the settings of this instrument.

6. Press **SHIFT** and **SYSTEM(PRESET)**. Initial setting conditions are loaded.

Connecting the input signal

Connect the calibration signal.

7. Attach the N(m)-BNC(f) adaptor to the INPUT connector on the front panel. Connect the included BNC (m)-BNC (m) input cable to the CAL OUT connector on the front panel and the N(m)-BNC(f) adaptor.

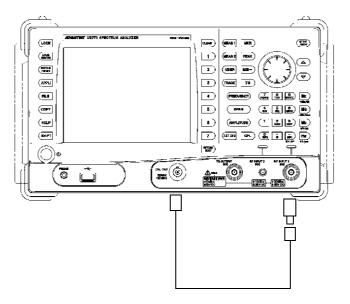


Figure 4-16 Connecting the CAL Signal

Setting measurement conditions

Set the measurement conditions to observe the input signal more easily.

- 8. Press **FREQUENCY**, **2**, **0**, and **MHz**. The center frequency is set to 20 MHz.
- 9. Press CPL, *Sweep Time AUTO/MNL*, **2**, **0**, and kHz (ms). The sweep time is set to 20 ms.
- 10. Press **SPAN**, **1**, **0**, and **kHz**. The span is set to 10 kHz.

The RBW is automatically set to 300 Hz according to the span setting and UNCAL message is displayed.

The sweep time setting of 20 msec is too fast for the set conditions.

4.3.3 How to Cancel the UNCAL Message

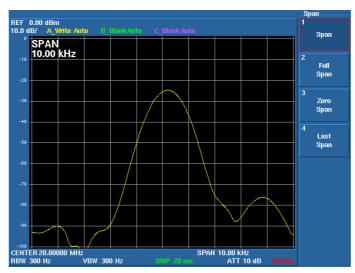


Figure 4-17 Displaying the UNCAL Message

How to cancel the UNCAL message

11. Press **CPL**, *RBW AUTO/MNL*, **1**, and **kHz**. Setting the RBW to 1 kHz cancels the UNCAL message because the sweep time of 20 msec meets the set conditions.

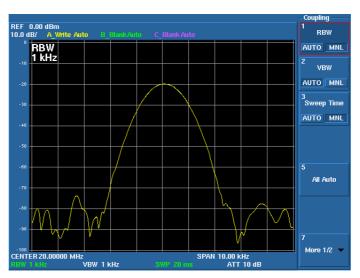


Figure 4-18 Canceling the UNCAL Message

4.3.4 Identifying an Image Signal

4.3.4 Identifying an Image Signal

This function is available only for the U3751, U3771, and U3772.


This instrument may display an image signal depending on the input signal.


If measuring an unknown frequency signal, the real signal and image signal must be identified before starting the measurement.

The Image Suppression and Signal Identification functions can be used to identify the image signal.

Image Suppression function

Detects image signals and automatically deletes them from the display. Press FREQUENCY, *More1/2*, and *Image Suppression ON/OFF*.

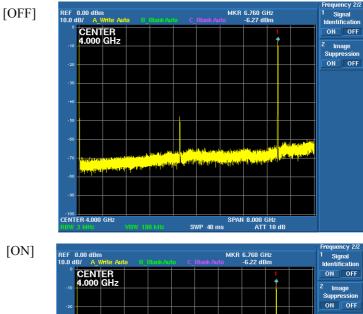

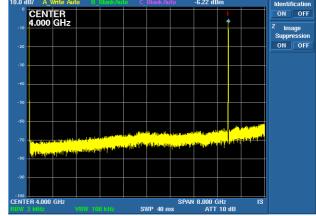

"IS" is displayed at the bottom right of the screen when the Image Suppression function is set to ON.

White font: Indicates that the calculation process of Image Suppression is correctly performed.

Red font: Indicates that the calculation process of Image Suppression is being performed or the calculation results are indefinite.


For example, when the center frequency is changed or the frequency of the input signal changes.

4.3.4 Identifying an Image Signal

Signal Identification function

The frequencies of Image signals are shifted and displayed in each sweep. The displayed frequencies of real signals do not change.

Press FREQUENCY, More1/2, and Signal Identification ON/OFF.

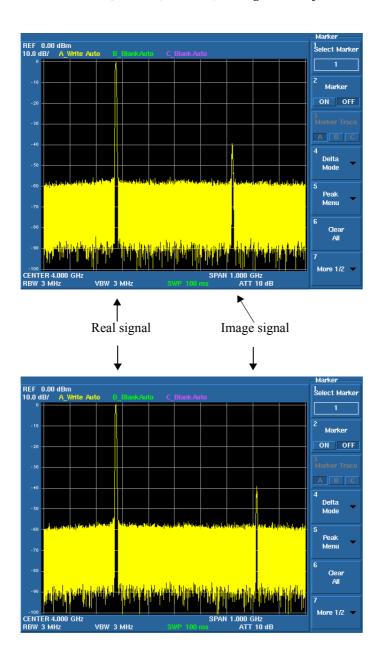

4.3.5 Hard Copy Output

4.3.5.1 Output to a Printer

Printer connection

When using a printer which is used for the first time,

- 1. Turn off the power of the printer and this instrument and connect the printer to the USB connector on the front or rear panels of this instrument.
- 2. Turn on the power of the printer.
- 3. Turn on the power of this instrument.

Anytime after the second time the printer is used, the printer can be connected to this instrument even if the power of this instrument is turned on.

Output to a printer

1. Specify the printer as the output device in COPY Config.

SYSTEM, *More1/2*, *Copy Config*, or

SHIFT, COPY

Select **PRT** (printer) from the **Copy Device** menu.

2. Press the **COPY** key or *Copy* in the Copy menu to start printing.

Printers whose operation has been checked

Manufacturer	Model name
Epson	PM-900C, PM-760C, PM-740C, PM-2200C, PM-G720, PX-V500
НР	HP5650, HP6122, Deskjet5740, Deskjet6840, Photosmart7830
Canon	iP4200

MEMO: The printing time can be reduced by performing the following:


- 1. Start copying during a sweep stop.
- 2. Use White and Black for Color Pattern.

4.3.5 Hard Copy Output

4.3.5.2 File Output to USB Memory

Connecting a USB memory device

- Connect a memory device to a USB port on the front or rear panels of this instrument.
- Press SYSTEM, More1/2, Copy Config, Screen Shot Config, and Media.
 A dialog box is displayed.
 Select a memory device by using the ▼ key and confirm it by using the Hz key.

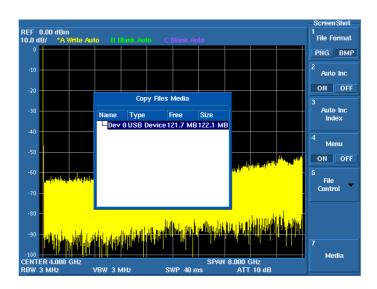

3. Press the **Media** key. The dialog box closes.

File output

1. Selecting a file format

Select the PNG or BMP format by pressing SYSTEM, More1/2, Copy Config, Screen Shot Config, and File Format PNG/BMP.

2. File name

COPYxxx.BMP(PNG) is used as the file name. File number xxx is specified by Auto Inc Index and automatically increments by 1 each time a file is saved when Auto Inc is set to ON. The file name COPY.BMP(PNG) is fixed when Auto Inc is set to OFF.

3. Output

Images on the screen can be saved to the USB memory device by pressing the **COPY** key.

4.3.5 Hard Copy Output

4. Time Stamp

A time stamp (date and time), which uses the same format as the computer, is included in a file. The order in which files are saved can be checked by using this time stamp.

The date and time can be checked and set by panel operations or GPIB commands.

Examples of GPIB commands:

• Command to check the date and time

Date: SETDATE? Time: SETTIME?

• Command to set the date and time

Date: SETDATE yy/mm/dd Time: SETTIME hh/mm/ss

• Example

Set the date to January 1, 2005.

SETDATE 050101

Set the time to 10:10. SETTIME 101000

Table 4-1 USB Memory Devices Whose Operation with this Instrument has Already Checked

Manufacturer	Model name
BUFFALO	RUF-C128ML/U2, RUF2-M128/256/1G, RUF2-E2GL-BL
HAGIWARA	HUD-128PJ *
IO DATA	EasyDisk EDP-128, TB-B128, TB-ST2G/K
LEXAR	JumpDrive 128MB
SanDisk	CruzerMini 128MB, SDCZ4-128-J65 *, SDCZ23-002G-J65N
ADTEC	AD-UMX128MSB *
GREEN HOUSE	GH-UFD128PLZ *
ELECOM	MF-PU2128SV *, MF-AU202GSV
Princeton	PFU-2JU/128/256/512/1G
Transcend	TS2GJF160

^{*} For the 256-MB type, the operation with this instrument has also been checked.

NOTE: The USB memory key with a security function cannot be used.

4.3.6 Measuring by using the TG (OPT76/OPT77)

Measures the characteristics of the bandpass filter, whose pass band is located near the frequency of 1900 MHz.

(Measuring the insertion loss and pass bandwidth of the filter)

Required equipment

This instrument Conversion adaptor: N(m)-BNC(f) ×2 Input cable: BNC(m)-BNC(m)

Turning on the power supply

IMPORTANT: Use this instrument within the specified temperature range to perform accurate measurements.

Perform calibration after allowing a warm up time of 5 minutes or more.

- 1. Verify that the AC power switch on the rear panel is set to OFF.
- 2. Connect the included power cable to the AC power connector on the rear panel.

CAUTION: To prevent damage, do not supply a voltage and frequency, which exceed the specified range, to this instrument.

- 3. Connect the power cable to an electrical outlet.
- 4. Turn on the AC power switch on the rear panel.
 After turning on the AC power switch, wait for three seconds or more.
- 5. Turn on the power switch on the front panel.

MEMO: The display may be different depending on the state of the instrument when the power was last turned off.

Initialization

Initialize the settings of this instrument.

- Press SHIFT and SYSTEM(PRESET). Initial setting conditions are loaded.
- 7. Regarding U3771 and U3772, press SHIFT and (RF1) to select RF INPUT 1.

Connecting the cable

1. Attach the N(m)-BNC(f) adapters to the RF INPUT 1 connector and the TG OUTPUT connector on the front panel and then connect the BNC(m)-BNC(m) cable to both connectors.


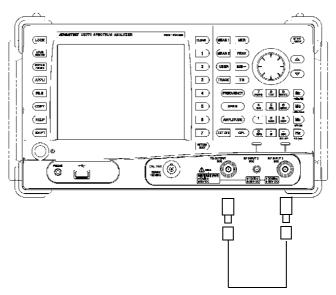


Figure 4-19 Connecting the TG Mesurement

Setting the measurement conditions to allow easier measurement of the input signal

- 2. Press **FREQUENCY**, **1**, **9**, **0**, **0**, and **MHz**. The center frequency is set to 1900 MHz.
- 3. Press **SPAN**, **2**, **0**, **0**, and **MHz**. The frequency span is set to 200 kHz.
- 4. Press **AMPLITUDE**, *dB/div*, and *2dB/div*. The level display scale is set to 2 dB/div.
- 5. Press **TG**, **TG Level**, **5**, and **MHz(-dBm)**. The output level of the tracking generator is set to -5 dBm.
- 6. Press *TG ON/OFF* to turn on the TG output.

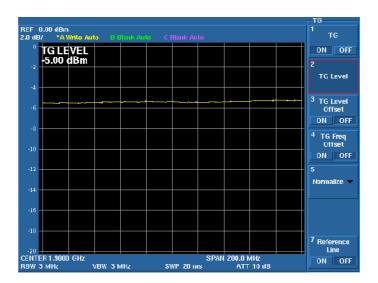

Performing the normalization


MEMO: The frequency response errors of accessories used in the measurement such as cables and adapters can be removed by performing the normalization and the accurate measurement can be performed.

- Press *Normalize*.
 The TG Normz menu is displayed.
- 2. Press *Reference Line ON/OFF*, **5**, and **MHz(-dBm)**. The Reference Line position, at which the normalization is performed, is set to -5 dB.
- 3. Press *Capture Normz Data*.

 The normalization data is acquired based on the set Reference Line position.
- 4. Press *Normalize Correction ON/OFF*. The normalization is performed.

CAUTION: If the settings of the center frequency, frequency span, reference level, or level display scale are changed after the normalization is performed, the normalization subsequent to this change does not perform correctly.

Re-perform the normalization after changing the settings.

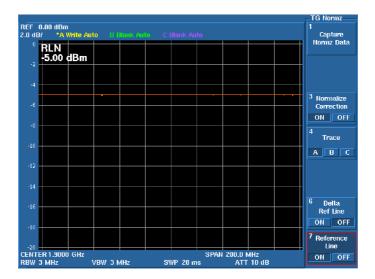

Connecting the unit under test

1. Connect the unit under test to TG OUTPUT and RF INPUT 1 of this instrument as shown in Figure 4-20.


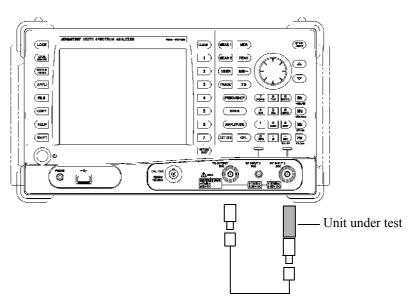


Figure 4-20 Connecting the Unit Under Test

CAUTION:


In the frequency response measurement by using the TG, the level measurement error may be larger even if the UNCAL message is not displayed on the screen. Increase the sweep time until the displayed waveform does not change. The TG response affects the measurement accuracy in the following cases:

- The unit under test has high Q and sharp level change characteristics. (For example, crystal filter)
- The measurement is performed in the wide frequency span.

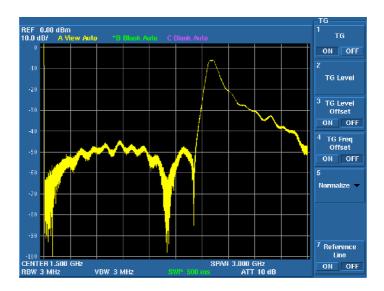

Measuring the insertion loss

- Press *Delta Ref Line ON/OFF*.
 The MKΔ value displays the level difference to the reference line.
- Press PEAK.
 The marker level indicates the insertion loss of the filter.

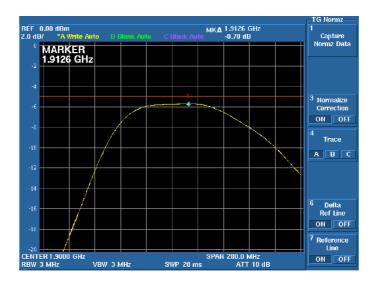


Measuring the 1-dB bandwidth

1. Start from the state of the insertion loss measurement.

Press MEAS2, XdB Down, XdB Level, 1, GHz(+dBm), and Execute XdB Down.

A marker is displayed at the right and left points on the waveform at a level which is $1\ dB$ below the peak.

The marker frequency indicates the 1-dB bandwidth of the filter.

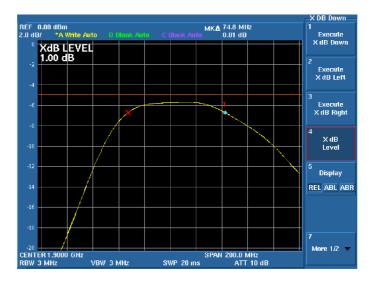

4.3.7 USER Key

4.3.7 USER Key

A soft menu related to operation keys and extended function keys can be set to the USER key menu. The operability is improved by allocating functions, which are frequently-used or are located in a deep multilayer menu, to the USER key menu.

How to set a function menu to the USER menu

- 1. Display a function menu, which is set to the USER menu, in the soft menu display area.
- 2. Press **SHIFT** and then **USER**.
- 3. Press a menu key to be set.

 If canceling the setting, press any other operation key.

If setting an additional function menu to the USER menu, repeat the above procedure.

How to delete a function menu from the USER menu

- 1. Press **USER** to display the USER menu.
- 2. Press **SHIFT** and then **USER**.
- 3. Press a menu key to be deleted.

If deleting an additional soft key, repeat the above procedure.

4.4 Measurement Examples


Descriptions regarding "Turning on the power" and "Initializing this instrument" are omitted from this chapter.

4.4.1 Using the Normalize Function and Level Correction Table

When a signal is measured by using a long measurement cable, the measurement level accuracy can be improved by correcting the cable frequency loss.


Functions used in this measurement

- 1. TG option + Normalize function \rightarrow Cable loss measurement
- 2. Level correction table

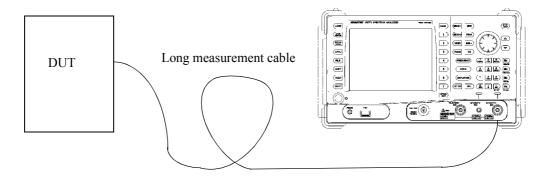


Measuring the cable loss

1. Connect TG OUTPUT and RF INPUT 1 by using the input cable included with this instrument.



2. Press FREQUENCY, 2, 0, MHz, SPAN, 1, MHz, TG, and TG ON/OFF (ON). The center frequency is set to 20 MHz, the frequency span is set to 1 MHz, and the TG (option) is set to ON.


3. Press **EXT CFG**, *Ref/Disp Lines*, and *Reference Line ON/OFF (ON)*. The reference line is displayed on the screen.

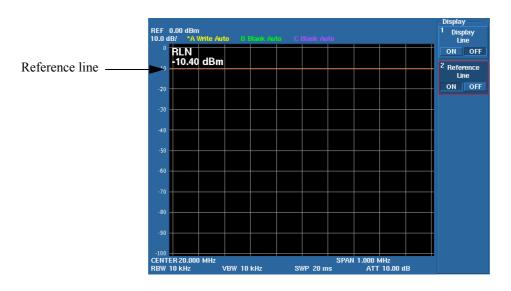


- 4. Turn the knob to adjust the reference line to the TG signal.
- 5. Press FREQUENCY, 1, ., 5, GHz, SPAN, 3, and GHz.

 The center frequency is set to 1.5 GHz and the frequency span is set to 3 GHz.
- 6. Press TG, Normalize, Capture Normz Data, and Normalize Correction ON/OFF (ON).
- 7. Connect TG OUTPUT and RF INPUT 1 by using a cable that is actually used for this measurement.

The frequency characteristic of the cable used in the measurement is displayed.




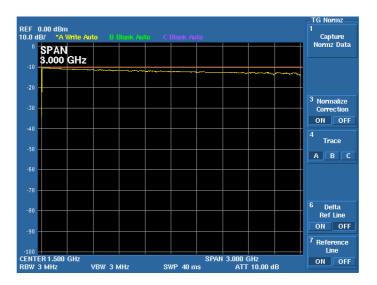

8. Press MKR, Delta Mode, Delta ON/OFF (ON), Ref Object, and Reference Line.

The marker delta mode is set.

The marker value shows a cable loss based on a frequency of 20 MHz.

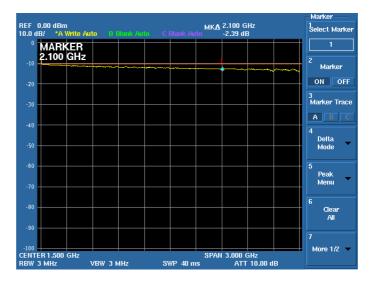

9. Move the marker and read a cable loss for each frequency.
For this measurement, 10 frequency points from 300 MHz to 3 GHz are used.

Creating the correction table

10. Press AMPLITUDE, More 1/2, and Edit Corr Factor.

The Correction Factor Table is displayed.

The cursor is positioned at the frequency setting text field of correction point 1.

11. Press 3, 0, 0, and MHz.

The correction point 1 frequency is set to 300 MHz.


The cursor moves to the level setting text field.

12. Press **0**, **.**, **8**, and **GHz**.

The correction value of correction point 1 is set to 0.8 dB.


The cursor moves to the frequency setting text field of correction point 2.

13. Repeat the above procedure and complete the correction table.

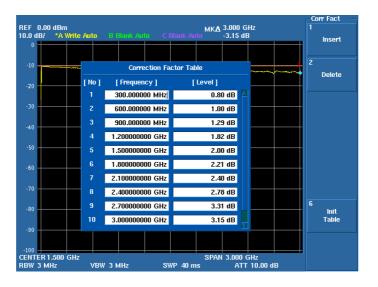

Using the correction table

14. Press **AMPLITUDE**, *More 1/2*, and *Correction Factor ON/OFF (ON)*. The displayed measurement value is corrected based on the correction table.

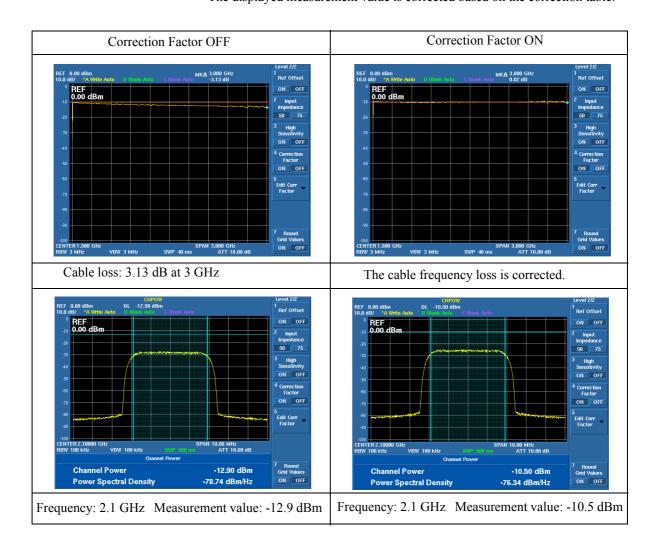


Available range of the correction value

Up to ± 100 dB can be set as the correction value.

The correction value of the first correction point is applied to frequencies from 0 Hz to the first correction point frequency.

Correction values between points where correction values are set are obtained by using a method of linear interpolation.

The correction value of the last correction point is applied to frequencies following to the last correction point frequency.

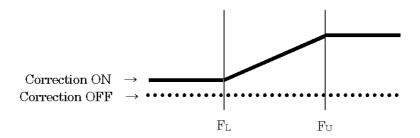

4.4.2 W-CDMA Channel Power Measurement

4.4.2 W-CDMA Channel Power Measurement

This section describes a measurement example of the W-CDMA signal by using the MEAS1 function.

• The maximum input level of this instrument

RF1: +30 dBm ±50 VDC (U3741)


RF1: +30 dBm ±15 VDC (U3751/U3771/U3772)

RF2: +10 dBm ±25 VDC (U3771/U3772)

CAUTION:

- When measuring signal power that exceeds the maximum input level, connect an external attenuator to
 ensure that the input level does not exceed it.
 A band rejection filter may be required depending on the standard.
- 2. When turning the power on, do not connect a DUT to this instrument.
- 3. Before turning the power off, disconnect the DUT from this instrument.

The W-CDMA mobile station signal, whose frequency is 1952.4 MHz and level is +24 dBm, is measured.

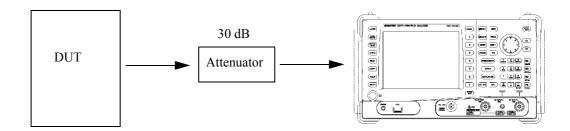


Setting measurement conditions

- 1. Press **FREQUENCY**, **1**, **9**, **5**, **2**, **.**, **4**, and **MHz**. The center frequency is set to 1952.4 MHz.
- Press SPAN, 1, 0, and MHz.
 The frequency span is set to 10 MHz.
- 3. Press **AMPLITUDE**, *More 1/2*, *Ref Offset ON/OFF (ON)*, **3**, **0**, and **GHz**. A value of 30 dB, which is the attenuation of the external attenuator, is added to a level reading value.

4.4.2 W-CDMA Channel Power Measurement

4. Press MEAS1 and Channel Power.

A window that shows the measurement channel width is displayed at the center of the screen.

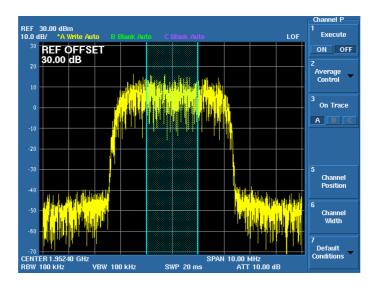

5. Press Channel Width, 3, ., 8, 4, and MHz.


The channel width is set to 3.84 MHz.

Measuring the channel power

6. Press *Execute ON/OFF (ON)*.

The channel power measurement starts.

The detector is automatically set to RMS.

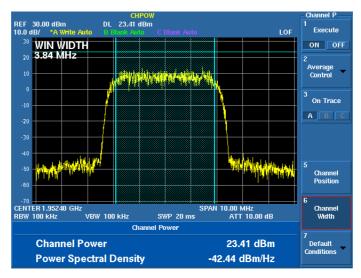


The measurement result is displayed.

A display line that shows the channel power is displayed.


4.4.3 W-CDMA Adjacent Channel Leakage Power (ACP) Measurement

A signal of 2100 MHz output from the W-CDMA transmitter is measured.

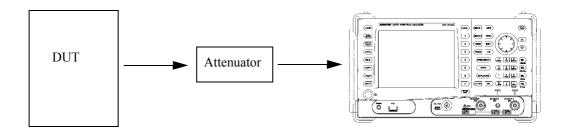

Examples of measurement specifications

Channel space	Specified bandwidth	Specification
5 MHz	3.84 MHz	45 dB
10 MHz	3.84 MHz	50 dB

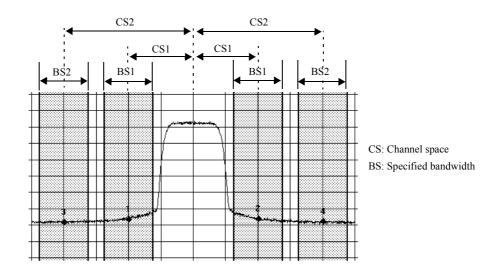

Setting measurement conditions

- 1. Press **FREQUENCY**, **2**, **1**, **0**, **0**, and **MHz**. The center frequency is set to 2100 MHz.
- 2. Press **SPAN**, **2**, **5**, and **MHz**. The frequency span is set to 25 MHz.

4.4.3 W-CDMA Adjacent Channel Leakage Power (ACP) Measurement

CAUTION:

Set the frequency span according to the following conditions.

- For Nyquist Filter OFF: SPAN > 2*CS + BS
- For Nyquist Filter ON:
 SPAN > 2*CS + (1 + Roll Off Factor)*Symbol Rate

3. Press AMPLITUDE, More 1/2, Ref Offset ON/OFF(ON), 3, 0, and GHz.

A value of 30 dB, which is the attenuation of the external attenuator, is added to a level reading value.

4. Press MEAS1 and ACP.

The ACP menu is displayed.

Setting the CS/BS table

5. Press Channel Definition.

The CS/BS table is displayed. The cursor is positioned at the Channel Space 1 setting text field.

6. Press 5 and MHz.

Channel Space 1 is set to 5 MHz. The cursor moves to the Channel Bandwidth 1 setting text field.

7. Press 3, ., 8, 4, and MHz.

Channel Bandwidth 1 is set to 3.84 MHz. The cursor moves to the Channel Space 2 setting text field.

8. Press 1, 0, and MHz.

Channel Space 1 is set to 10 MHz. The cursor moves to the Channel Bandwidth 2 setting text field.

9. Press 3, ., 8, 4, and MHz.

Channel Bandwidth 2 is set to 3.84 MHz.

10. Press **RETURN**.

CS/BS Table			
[Channel Space]	[Channel Bandwidth]		
5.000 MHz	3.840 MHz		
10.000 MHz	3.840 MHz		
	[Channel Space] 5.000 MHz		


4.4.3 W-CDMA Adjacent Channel Leakage Power (ACP) Measurement

Measuring the ACP

11. Press Execute ON/OFF (ON).

The ACP measurement starts.

The detector is automatically set to RMS.

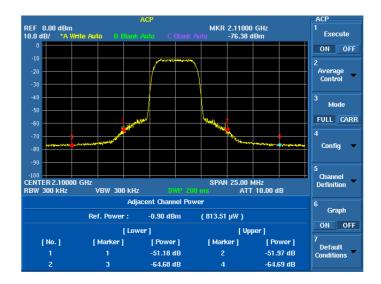

Displaying the channel bandwidth

12. Press Config and Ch Windows ON/OFF (ON).

The set channel bandwidth window is displayed on the screen. The frequency span must be set so that all channels are included in it.


-51.88 dB

-51.15 dB

4.4.4 W-CDMA Spurious Measurement

4.4.4 W-CDMA Spurious Measurement

The spurious response is measured in frequency bands higher than 30 MHz.

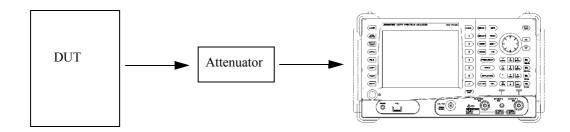

Examples of measurement specifications

Frequency range	RBW	Spurious level
9 kHz ~ 150 kHz	1 kHz	-13 dBm
150 kHz ~ 30 MHz	10 kHz	-13 dBm
30 MHz ~ 1 GHz	100 kHz	-13 dBm
1 GHz ~ 12.75 GHz (*)	1 MHz	-13 dBm

^(*) In a frequency range from 1.8935 GHz to 1.9196 GHz and the 300-kHz RBW, the spurious level is -41 dBm or less.

Setting measurement conditions

1. Press TRACE, Detector, and Posi.

Detector is set to Posi to perform the spurious measurement.

2. Press MEAS1, Spurious, and Bands Definition.

The Spurious Bands table is displayed.

The cursor is positioned at the start frequency setting text field of frequency band 1.

3. Press **3**, **0**, and **MHz**.

The start frequency is set to 30 MHz and the cursor moves to the stop frequency setting text field.

4. Press 1 and GHz.


The stop frequency is set to 1 GHz and the cursor moves to the RBW selection button from Auto and Manual.

If selecting Auto, press Hz.

If selecting Manual, turn the knob clockwise for one click to select the Manual button, and then press ${\bf Hz}$.

5. Select *Manual*, and then press 1, 0, 0, and kHz.

The RBW is set to Manual and 100 kHz.




6. Repeat the above procedure and set the VBW to Manual and 100 kHz, the SWP to Auto, the ATT to Manual and 20 dB, the Ref Level to 0 dBm, and the Preamp to Off.

The cursor moves to the limit value setting text field.

7. Press -, 1, 3, and GHz.

The limit value is set to -13 dBm, and then the cursor moves to the start frequency setting text field of the next frequency band.

8. Repeat the above procedure and complete the Spurious Bands table.



9. Press **RETURN**.

The spurious measurement menu is displayed.

4.4.4 W-CDMA Spurious Measurement


Measuring the spurious response

10. Press Execute ON/OFF (ON).

The spurious response in each frequency band that changes after a sweep is measured according to the measurement conditions set in the Spurious Bands table.


Characters that indicate a frequency band, in which the spurious response is being measured, are displayed in yellow.

If the measured value is equal to the set limit value or less, the judgment is PASS. If the measured value is more than the set limit value, the judgment is FAIL.

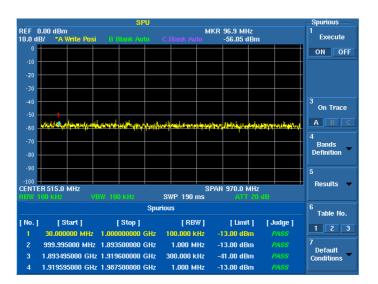


11. Press Results.

Measurement results in each frequency band are displayed.

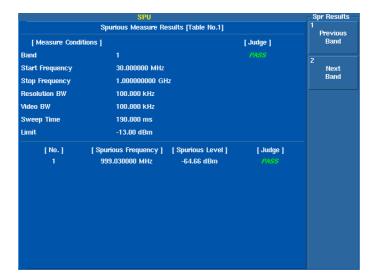

The difference (CN ratio) between a carrier level (C) and noise level (N) in terrestrial digital broadcasting is measured.

When measuring the CN ratio, connect the 75- Ω impedance converter (ZT-130NC) to the RF1 input connector of this instrument. Set the measurement unit to dB μ V.



Setting the measurement unit

- 1. Press **AMPLITUDE**, *Units*, and $dB\mu V$. The measurement unit is set to dB μ V.
- 2. Press **AMPLITUDE**, *More1/2*, and *Input Impedance 50/75 (75)*. The conversion loss of the 75- Ω impedance converter (ZT-130NC) is corrected for the measured value.

Measuring the carrier level (C)

Setting this instrument

Measurement mode: Channel power measurement function

Center frequency: Center frequency in the channel

SPAN 10 MHz
RBW: 30 kHz
VBW: 300 kHz
Measurement bandwidth: 5.6 MHz

(Channel power bandwidth)


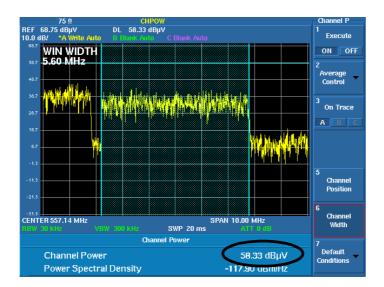


Figure 4-21 Measurement Display for Channel Power

Procedure (Example for 27 channels)


- 1. Press FREQUENCY, 5, 5, 7, ., 1, 4, 2, 8, 5, 7, and MHz. The center frequency is set to 557.142857 MHz.
- 2. Press **SPAN**, **1**, **0**, and **MHz**. The frequency span is set to 10 MHz.

3. Press **AMPLITUDE** and then press ▼ to adjust a signal peak on the third scale from the top.

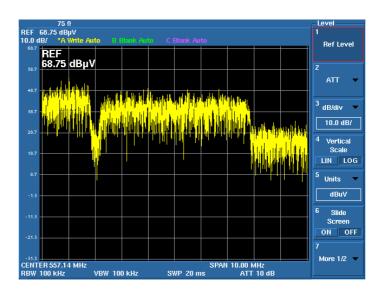

- 4. Press CPL, *RBW AUTO/MNL*, 3, 0, kHz, *VBW AUTO/MNL*, 3, 0, 0, and kHz. The RBW is set to 30 kHz and the VBW is set to 300 kHz.
- 5. Press MEAS1 and Channel Power.

A window that shows the measurement channel width is displayed in the center of the screen.

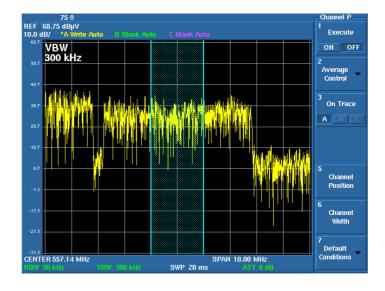

6. Press *Channel Width*, **5**, **.**, **6**, and **MHz**. The channel width is set to 5.6 MHz.

7. Press *Execute ON/OFF (ON)*.

The channel power measurement begins.

8. The measurement result is displayed in the Channel Power window.

 $C = 58.33 \text{ dB}\mu\text{V}$ (Figure 4-21)

Measuring the noise level (N)

Setting this instrument

Measurement mode: Noise/Hz measurement function

Measurement noise area frequency:

Noise that is adjacent to the measurement signal and

not affected by the signal

SPAN: 10 MHz
RBW: 100 kHz
VBW: 1 kHz
Measurement bandwidth: 5.6 MHz

(A value for the Noise/Hz conversion)

Averaging count: 30 times



Figure 4-22 Measurement Display for Noise Power Converted into 5.6 MHz
Bandwidth


Procedure

9. Press *Execute ON/OFF (OFF)*.


The channel power measurement is canceled.

- 10. Press CPL, *RBW AUTO/MNL*, 1, 0, 0, kHz, *VBW AUTO/MNL*, 1, and kHz. The RBW is set to 100 kHz and the VBW is set to 1 kHz.
- 11. Press **MKR** and then press **\(\)** to move the marker into a noise area.
- 12. Press TRACE, Calc, Power Average, Start/Stop (Start), Max Sweep Count, 3, 0, and Hz (Enter).

The Max Sweep Count is set to 30.

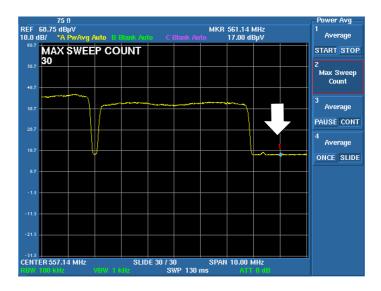

13. Press MEAS 2, Noise/Hz, 5, ., 6, and MHz.

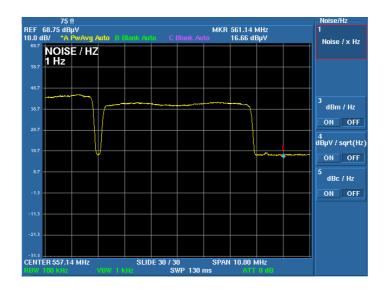

14. Press dB μV/Sqrt (Hz) ON/OFF (ON).

The measurement begins.

15. The measurement result is displayed in the Noise-Marker 1 window. $N=34.26\ dB\mu V\ (Figure\ 4-22)$

Calculating the CN ratio

The CN ratio can be obtained by calculating the values, which are measured from the carrier (C) and noise (N) level measurements. (C: a value in step 8, N: a value in step 15)

CN ratio = C - N = 58.33 - 34.26 = 24.07 dB

4.4.6 Television Signal Measurement

4.4.6 Television Signal Measurement

Japanese television channels are pre-saved to OPT11 and OPT15 (75 Ω input option).

The table can be read using the Recall function and a measurement frequency can be set using the channel number.

Registered files and setting conditions

1_CATV_CH: CATV channel (See A.6.1)

2 VHF&UHF CH: VHF and UHF channels (See A.6.2)

3_BS_IF_CH: BS-IF channel (See A.6.4) 4 CS IF CH: CS-IF channel (See A.6.5)

5_Digital_CH: Terrestrial digital channel (See A.6.3)
6 Digital Noise: Terrestrial digital noise measurement

7 Digital ChPower: Terrestrial digital channel power measurement

Recall the file and refer to the registered channel table. The center frequency can be set using the channel number.

Change SPAN, REF LEVEL, and input attenuator settings according to the operating environment.


NOTE: When the 6_Digital_Noise file is recalled, the input attenuator is set to 0 dB. Be careful of the input signal level.

Example of recalling the 7 Digital ChPower file and measuring the Channel 28 power

Procedure

Press FILE and *Recall*.
 The Recall window is displayed.

2. Turn the knob to select the 7 Digital ChPower.dat file.

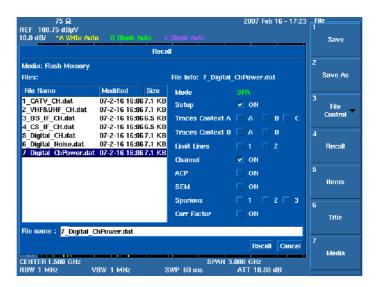

4.4.6 Television Signal Measurement

3. Press \mathbf{Hz} or $\mathbf{\nabla}$.

The 7_Digital_ChPower.dat file is determined as a file to be recalled.

4. Press **Hz** or **▼**.

Select the Recall button.

5. Press **Hz**.

The terrestrial digital broadcasting channel table and measurement conditions are recalled and set.

6. Press FREQUENCY, 2, 8, and Hz.

The center frequency is set to 563.14 MHz, that is for Channel 28.

At the same time, the channel power measurement starts and then the measurement result is displayed.



4.4.7 VSWR Measurement

Reflection characteristics of an antenna and filter are measured by using the SWR bridge.

A return loss and VSWR at a marker point are displayed.

1. Connect the SWR bridge as shown in Figure 4-23 VSWR Measurement.




Figure 4-23 VSWR Measurement

2. Execute normalization without connecting a DUT to the TEST port of the SWR bridge.

Set ČENTER, SPAN, and REF in accordance with the DUT.

Press **TG**, *Reference Line ON/OFF(ON)*, **2**, **0**, and **MHz**. Set the reference line to -20 dBm.

Press TG and TG ON/OFF(ON).

Set the TG output to ON.

Press *Normalize*, *Capture Normz Data*, and *Normalize Correction ON/OFF(ON)*.

Normalization is executed while the TEST port is open.


CAUTION: If a setting condition is changed after normalization is executed, reexecute normalization.

4.4.7 VSWR Measurement



3. Connect the DUT to the TEST port of the SWR bridge. Press *VSWR ON/OFF(ON)*.

A return loss and VSWR at the marker point are displayed.

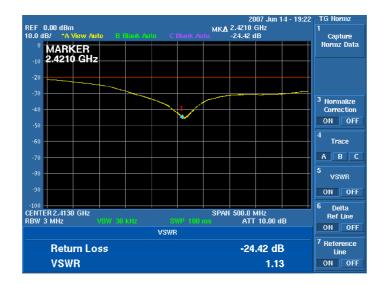

5. MENU MAP, FUNCTIONAL EXPLANATION

This chapter describes the configurations and functions of the soft keys displayed on the touch screen.

Menu Index: This section can be used to refer to the keys in this chapter.

Menu Map: This section shows the menu configurations of the panel keys.

Functional Descriptions: This section describes the functions of the panel keys and soft keys.

Operation Key	Pages	Operation Key	Pages
%AM Meas ON/OFF	. 5-37. 5-40		5-27, 5-28,
%OBW			5-29, 5-30,
0.5 dB/div			5-32, 5-36,
1 dB/div	. 5-62, 5-63		5-38, 5-40,
1/Delta Mkr ON/OFF			5-43, 5-44,
10 dB/div	. 5-62, 5-63		5-45
2 Channel ON/OFF		Average PAUSE/CONT	5-36, 5-38,
2 Channel Preset	. 5-17	C	5-40, 5-43,
2 Channels Viewer			5-44
2 dB/div	. 5-62, 5-63	Average Power	. 5-25, 5-29
5 dB/div	. 5-62, 5-63	Average START/STOP	
A-B→A	. 5-43, 5-46	C	5-39, 5-43,
A-B→B	. 5-43, 5-46		5-44
A-B→C	. 5-43, 5-46	Averaging ON/OFF	5-25, 5-26,
ACP	. 5-25, 5-30		5-27, 5-28,
A-DL→A			5-29, 5-30,
All Auto	. 5-72, 5-73		5-32
AMPLITUDE	. 5-62	B-A→A	5-43, 5-46
Annotations ON/OFF	. 5-7, 5-9	B-A→B	. 5-43, 5-46
APPLI	. 5-17	B-A→C	. 5-43, 5-46
ATT	. 5-62	Bands Definition	5-26, 5-33,
ATT AUTO/MNL	. 5-62		5-34
Attenuation 0 dB	. 5-62	B-DL→B	5-43, 5-46
Auto	. 5-72, 5-73	Black and White	. 5-8, 5-12
Auto Inc Index	. 5-8, 5-13	Blank	. 5-43, 5-44
Auto Inc ON/OFF	. 5-8, 5-13	Calc	. 5-43, 5-44
Auto name Index	. 5-18, 5-20	Calibrate ALL	. 5-7, 5-11
Auto Tune	. 5-61	Calibration	. 5-7, 5-11
Auto-name Radix	. 5-18, 5-20	Calibration Corrections ON/OFF	5-7, 5-11
Average	. 5-43, 5-44,	Calibration F Int Ref	5-7, 5-11
	5-45	Capture Normz Data	. 5-55
Average Control	. 5-25, 5-26,	Carrier Bandwidth	5-26, 5-31,
	5-27, 5-28,		5-32
	5-29, 5-30,	Center	. 5-57
	5-32, 5-36,	Center CH ON/OFF	. 5-57, 5-58
	5-38, 5-39	CF Step Size AUTO/MNL	. 5-57
Average ONCE/SLIDE	. 5-25, 5-26,	Ch Windows ON/OFF	

	5.22	D C 1/ C 1//	5.05.5.06
	5-32	Default Conditions	
Channel Definition	· ·		5-27, 5-28,
Channel Input			5-29, 5-30,
Channel Position	*		5-32, 5-34,
Channel Power	*		5-35, 5-36,
Channel Width		D 1	5-39
Channels Config		Delay	
Clear All		Delete	
Clear Others	, , , , , , , , , , , , , , , , , , ,	Delete Band	
Coarse			5-35
Color Mode Color/Gray		Delete Channel	
Color Pattern	,	Delete Entry	
Color1	ŕ		5-52, 5-65,
Color2			5-69
Command Reference Syntax		Delete Line	,
Config		Delta Mode	
	5-32, 5-47,	Delta ON/OFF	
	5-50	Delta Ref Line ON/OFF	
Config Driver	5-8, 5-15	Delta to CF	5-54
Context A/B	5-66, 5-70,	Delta to CF Step	5-54
	5-71	Delta to Mkr Step	5-54
Context RF2 RF1	5-17, 5-18	Delta to Span	5-54
Continuous Down ON/OFF		Det Avg Mode RMS/Video	5-43, 5-45
Continuous Peak ON/OFF	5-47, 5-50	Detector	5-43, 5-45
Copy	5-8, 5-13	Detector AUTO/MNL	5-43, 5-45
Copy All to Flash	5-18, 5-20	Display Line ON/OFF	5-43, 5-46,
Copy All to USB	5-18, 5-20		5-47, 5-50,
Copy Config	5-8, 5-13		5-51, 5-65,
Copy Device FILE/PRT	5-8, 5-13		5-69
Correction Factor ON/OFF	5-62, 5-64	Display List ON/OFF	5-47, 5-48,
Counter Position	5-36, 5-40		5-50, 5-53
Couple to DL OFF/ABV/BLW	5-47, 5-50,	Display REL/ABL/ABR	5-36, 5-38
	5-51	Each Item	5-7, 5-11
Couple to Line 1 OFF/ABV/BLW	5-47, 5-50,	Edit Channel Formula	5-57, 5-59
•	5-51	Edit Channel Table	5-57, 5-59
Couple to Line 2 OFF/ABV/BLW	5-47, 5-50,	Edit Corr Factor	5-62, 5-64
•	5-51	Edit Date Time	5-8, 5-12
Couple to Win OFF/IN/OUT	5-47, 5-50,	Edit Limit Lines	5-47, 5-50,
•	5-51		5-52
CPL	5-72	EMC	5-72
Date Time		EMC Filter ON/OFF	
dB/div	5-62, 5-63	Execute ON/OFF	5-25, 5-26,
dBc/Hz ON/OFF	*		5-27, 5-28,
dBm			5-29, 5-30,
dBm/Hz ON/OFF			5-32, 5-34,
dBmV			5-36, 5-37,
dBμV	· ·		5-38, 5-39,
dBμV/sqrt(Hz) ON/OFF			5-40, 5-41
dBµVemf		Execute Self Test	
dBpW		Execute X dB Down	
Default		Execute X dB Left	
	- ,, - 11		

Francis V ID Diala	5 26 5 27		5 (2 5 (4
Execute X dB Right		Innert and Output	5-62, 5-64
EXT CFG		Input and Output	
Ext Trigger Level		Innut Innu dana 50/75	7-14
External	*	Input Impedance 50/75	
Factory Init		Insert	,
FILE		Insert Band	
File Control		Insert Channel	
Eile Ferman DINI/VMI	5-18, 5-19	Insert Entry	
File Format BIN/XMLFile Format PNG/BMP			5-52, 5-65, 5-69
	<i>'</i>	Incort Line	
Fine	*	Insert Line	
Fixed Mkr ON/OFF	*	Intermod	
FM Meas	*	ItemsLAN IP Address	
Format Media	*		
Formula 1 ON/OFF		Last Span Level	
Formula 2 ON/OFF		Limit Line 1/2	
Formula 3 ON/OFF	*	Limit Line 1/2	
Free Run	*		5-52, 5-65, 5-69
Freq Input Mode CALC/TABLE		Limit Line Edit	
Freq vs Time		Limit Lines	
Freq vs Time ON/OFF		Limit Setup	
Freq Zoom		Line 1 ABV/BLW	
FREQUENCY		Line 1 ON/OFF	
Frequency Correction ON/OFF		Line 2 ABV/BLW	
Frequency Counter		Line 2 ON/OFF	
Frequency Offset ON/OFF		Link to Marker ON/OFF	
Frequency Pos		Marker ON/OFF	
Frequency Reference		Marker Trace A/B/C	
Frequency Reference INT/EXT/XTL		Math	
Frequency Zoom ON/OFF		Max Hold	
Full Span		Max Hold Continuous	
Fundamental ON/OFF		Max Order	
Gate Delay		Max Sweep Count	
Gate Width		wax sweep count	5-27, 5-28,
Gated Sweep	,		5-29, 5-30,
Gated Sweep ON/OFF			5-32, 5-36,
GPIB Address	,		5-38, 5-39,
Graph ON/OFF			5-43, 5-44
Graphic		MEAS 1	
Graphic Z 1 Screen		MEAS 2	
Graphic Z 2 Screens		Measuring Window	
Graphic Zoom 1 ON/OFF		Media	
Graphic Zoom 2 ON/OFF			5-18, 5-23
Harmonic		Medium	ŕ
Harmonic Max Order		Menu ON/OFF	
High Sensitivity ON/OFF			5-15
IF		Min ATT	5-62
Image Suppression ON/OFF		Min Hold	5-43, 5-44
Init Table		Min Max Peak	5-47, 5-50,
	5-33, 5-35,		5-52

Min Peak	5-47 5-50	Parser AT/SCPI	5-7 5-11
Willia Cuk	5-52	Pass/Fail Config	
MKR		Pass/Fail ON/OFF	
Mkr Step AUTO/MNL		1 455/1 411 51 (/ 511	5-65, 5-68
Mkr to CF		Pause Time	
Mkr to CF Step		PBW	
Mkr to Mkr Step		PEAK	
Mkr to Ref		Peak + X dB Down	
MKR→		Peak Delta Y	
Mod. Freq to Sweep Time ON/OFF		Tear Detta T	5-47, 5-50
Mode FULL/CARR		Peak List Frequency	
Mode Index/Value		Teak List Frequency	5-52
More 1/2		Peak List Level	
WIGIE 1/2	5-7, 5-12, 5-18, 5-20,	reak List Level	5-53
		Peak Menu	
	5-36, 5-38,		
	5-40, 5-43,	Peak to CF	
	5-46, 5-47,		
	5-48, 5-50,	Peak Zoom	
	5-52, 5-54,	PLL BW	,
	5-57, 5-60,	Posi	,
	5-62, 5-63,	Power Average	
N.	5-72, 5-73	Previous Band	
Narrow	*	Print Config	
Nega		Quasi Peak	
Next Band		R3131 Mode ON/OFF	
Next Min Peak		R3162 Mode ON/OFF	
	5-52	Range FULL/WIN	
Next Peak		RBW 1 MHz	
Next Peak Left		RBW 120 kHz	
Next Peak Right		RBW 200 Hz	
Noise/Hz		RBW 9 kHz	. 5-72
Noise/x Hz		RBW Auto	
Normal	5-43, 5-45	RBW AUTO/MNL	
Normalize		RBW CAL	
Normalize Correction ON/OFF		Recall	. 5-18, 5-21
Nyq Roll Off Factor		Ref Freq	. 5-7, 5-9
	5-33	Ref Freq 10 MHz	. 5-7, 5-9
Nyq Symbol Rate	5-26, 5-31,	Ref Level	. 5-62
	5-33	Ref Object	. 5-47, 5-48
Nyquist Filter ON/OFF	5-26, 5-31,	Ref Offset ON/OFF	. 5-62, 5-63
	5-32	Ref Power CHN/PEAK	5-26, 5-32
OBW	5-25, 5-30	Ref/Disp Lines	. 5-65, 5-69
OFF	5-43, 5-46	Reference Line	. 5-47, 5-48
On Trace A/B/C	5-25, 5-26,	Reference Line ON/OFF	5-55, 5-56,
	5-27, 5-28,		5-65, 5-69
	5-29, 5-30,	Reference Marker	. 5-47, 5-48
	5-32, 5-34,	Refresh	. 5-43, 5-44
	5-36, 5-38,	Refresh(Write)	. 5-43, 5-44
	5-40	Remote Control	
Others HIDE/SHOW	5-47, 5-48	Remove File	
Paper Format			5-18, 5-19
•	•		•

5.1 Menu Index

Rename File		Spectrum RF1	
	5-18, 5-19	Spectrum RF2	
Report HIDE/SHOW		Spurious	
Reset Context		Start	
Resolution		Start CH Offset ON/OFF	,
Resolution 1 Hz		Start CH ON/OFF	
Resolution 1 kHz	*	Step ATT CAL	
Resolution 10 Hz	,	Stop	
Resolution 100 Hz	,	Stop CH Offset ON/OFF	
Restore Defaults		Stop CH ON/OFF	
	5-27, 5-28,	Store	
	5-29, 5-30,		5-43, 5-46
	5-32, 5-34,	Subtract	
	5-35, 5-36,	Sweep Mode SGL/CNT	
	5-39	Sweep Time AUTO/MNL	
Results		SYSTEM	
Round Grid Values ON/OFF	,	Table Init	5-47, 5-50,
Sample	5-43, 5-45		5-52, 5-57,
Save	5-18		5-59, 5-65,
Save as	5-18, 5-19		5-69
Save Defaults	5-25, 5-26,	Table No. 1/2/3	5-26, 5-35
	5-27, 5-28,	TG	5-55
	5-29, 5-30,	TG Freq. Offset ON/OFF	5-55
	5-32, 5-34,	TG Level	5-55
	5-35, 5-36,	TG Level Offset ON/OFF	5-55
	5-39	TG ON/OFF	5-55
Screen Shot Config	5-8, 5-13	Time vs Time	5-66, 5-70
Select	5-50	Title	5-18, 5-22
Select Marker	5-47, 5-48,	Total Gain RF Path 1	5-7, 5-11
	5-50	Total Gain RF Path 2	5-7, 5-11
Selecting the Command Set	6-1	Total Power	5-25, 5-28
Self Test	5-8, 5-16	TRACE	5-43
Shift X ON/OFF	5-65, 5-68	Trace A/B/C	5-43, 5-44,
Shift Y ON/OFF	5-65, 5-69		5-45, 5-46,
Show Mask ON/OFF	5-26, 5-32		5-55, 5-56
Show ON/OFF	5-8, 5-13	Trace Points 501/1001	5-7, 5-11
Signal Identification ON/OFF		TRC→A	5-43, 5-46
Signal Track		TRC→B	5-43, 5-46
Signal Track ON/OFF		TRC→C	5-43, 5-46
Slide Screen ON/OFF		Trigger	
Slope NEG/POS	5-65, 5-66,	Units	
•	5-67	User Password	5-8, 5-12
Sound	5-37, 5-41	VBW AUTO/MNL	
Sound AM/FM		VBW/RBW ON/OFF	5-72, 5-73
Source	5-65, 5-66,	Version	
	5-67	Vertical Scale LIN/LOG	
SPAN	5-61	Video	5-65, 5-66
Span		View	
SPAN/RBW ON/OFF		Volts	
Spectrum Analyzer		Volume	
Spectrum Emission		VSWR ON/OFF	
1	-,		,0

5.1 Menu Index

Watts	5-62, 5-63
White and Black	5-8, 5-12
Window	5-25, 5-29
Window HIDE/SHOW	5-65, 5-67
Window Position	5-25, 5-29,
	5-47, 5-50,
	5-51, 5-65,
	5-66, 5-67,
	5-69, 5-70
Window Sweep ON/OFF	5-65, 5-67
Window Width	
	5-47, 5-50,
	5-51, 5-65,
	5-66, 5-67,
	5-69, 5-70
Write	5-43, 5-44
Write Protect ON/OFF	
	5-18, 5-19
X ABS/CF/FA	
X dB Down	
X dB Level	
X-Search Domain	5-47, 5-50
Y ABS/REF/DL	
Y Range ON/OFF	5-47, 5-49
Y- Search Domain	
	5-51
Zero Span	5-61
Zoom and Contexts	
Zoom Position	
Zoom Width	5-66, 5-70

5.2 Functional Descriptions

5.2 Functional Descriptions


This section describes the functions of the panel keys and soft keys.


МЕМО:

- indicates a panel key.
- All other names are soft menus.

5.2.1 SYSTEM


This subsection describes how to configure this instrument.

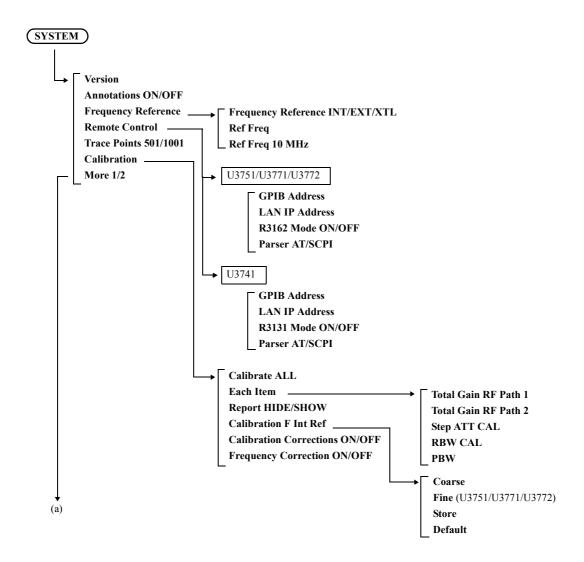

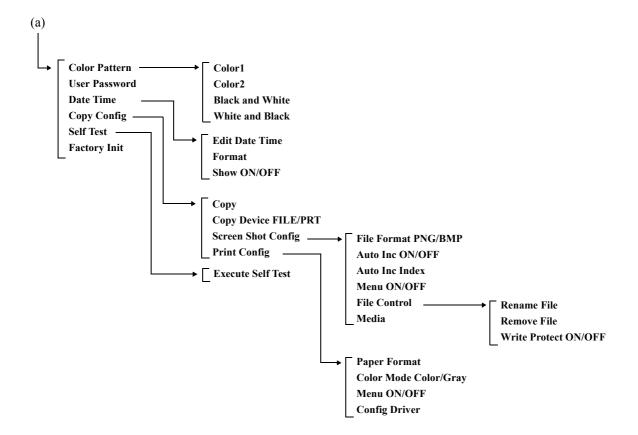

Version

Displays the software version dialog box.



Annotations ON/OFF

ON: Displays set values such as the center frequency on the

top and bottom of the vertical scale.

OFF: Hides set values and zooms into the area in which set

values are displayed.

Frequency Reference

Selects the signal source of the reference frequency.

Frequency Reference INT/EXT/XTL

INT: Selects the internal signal source.

EXT: Uses an external input signal from the EXT. REF

connector.

XTL: Selects an optional crystal oscillator.

Ref Freq The reference frequency can be changed by using the step keys.

The following frequencies can be set as the reference frequency.

1 MHz, 1.544 MHz, 2.048 MHz, 5 MHz

10 MHz, 12.8 MHz, 13 MHz, 13.824 MHz,

14.4 MHz, 15.36 MHz, 15.4 MHz, 16.8 MHz,

19.2 MHz, 19.44 MHz, 19.6608 MHz,

19.68 MHz, 19.8 MHz, 20 MHz, 26 MHz

Ref Freq 10 MHz Sets the reference frequency to 10 MHz.

Remote Control


Displays the Remote Ctrl menu.

GPIB Address

Sets the GPIB address of this instrument.

LAN IP Address

Sets the IP address of this instrument. Displays the Network Setting dialog window.

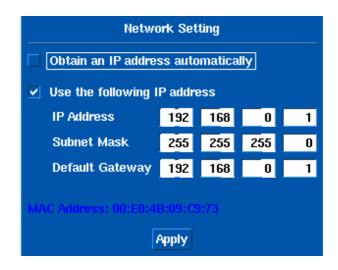

R3162 Mode ON/OFF (U3751/U3771/U3772)

ON:

The following R3162GPIB commands can be used and their operations are the same as those of the R3162. For more information on the commands, refer to the R3162 manual.

Command

MN *

MKD *

PWCH PWTM *

PWTOTAL

PWM

OBW [ON]|OFF OBWEXE

ACPEXE

LIMTYP *

LMTAIN *

LMTADEL

LIMAPOS REL

LIMASFT *

LIMSFT *

AT 0DB

RO*

DL *

OFF: Operates in the U3700 series command system.

R3131 Mode ON/OFF (U3741)

ON: Except for certain R3131/R3131A functions, the same

GPIB commands as those for the R3131/R3131A can be used. For more information on commands, refer to

the R3131 Series Operation Manual.

Unavailable functions:

Trigger (LINE), EMC, Calibration, Hard Copy

OFF: Operates in the U3700 series command system.

Parser AT/SCPI Selects a remote command set to be used.

AT: The AT (Advantest) command set is selected.

SCPI: The SCPI command set is selected.

Trace Points 501/1001 Switches the horizontal axis trace points to 501 or 1001.

501: Sets trace points to 501 points.1001: Sets trace points to 1001 points.

Calibration Displays the Calibration menu.

Calibrate ALL Performs all calibrations.

Each Item Displays the Each Item menu.

Total Gain RF Path 1 Measures the absolute error at 20 MHz based on the CAL signal

that is input to the RF INPUT 1 connector.

Total Gain RF Path 2 Measures the absolute error at 20 MHz based on the CAL signal

that is input to the RF INPUT 2 connector. (U3771, U3772)

Step ATT CAL Measures the error at 20 MHz when switching ATT.

RBW CAL Automatically adjusts IF filters.

PBW Performs the calibration of the noise power bandwidth.

Report HIDE/SHOW Hides or displays the calibration results.

Calibration F Int Ref Calibrates the frequency of the crystal oscillator that is used for

the internal frequency reference.

Coarse Changes the data of the coarse adjustment.

Fine Changes the data of the fine adjustment.

Store Saves the adjusted data.

The saved data is used even if this instrument is preset.

Default Sets the calibration data when this instrument is shipped from the

factory.

Calibration Corrections ON/OFF

Switches the calibration factor ON and OFF.

ON: Uses the CAL factor.

OFF: Does not use the CAL factor.

Frequency Correction ON/OFF

Switches the frequency correction function ON and OFF.

ON: Corrects the frequency characteristics.

OFF: Cancels the frequency correction function.

More 1/2 Displays the System 2/2 menu.

Color Pattern

Color1 Selects the standard color.

Color2 Selects the second set of colors.

Black and White Selects the black and white mode (white traces).

White and Black Selects the white and black mode (black traces).

User Password Sets the password used to lock the panel.

The password is set to [0,0,0,0] when this instrument is shipped

from the factory.

The password can be changed in the dialog box.



A password can be initialized (0,0,0,0) through the GPIB. GPIB AT command: "RPWD"


Date Time

Displays the Date Time menu.

Edit Date Time

Sets a date and time.

They are set or changed in the dialog window.

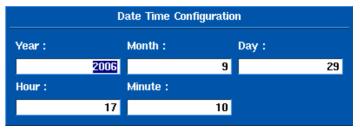

Year: Set a year.

Month: Set a month.

Day: Set a date.

Hour: Set an hour.

Minute: Set a minute.

Format Sets date display formats.

They are set or changed in the dialog window.



Show ON/OFF Switches ON and OFF the date display.

ON: Displays the date.

OFF: Hides the date display.

Copy Config Displays the Copy menu.

Copy Outputs screen data according to Config.

Copy Device FILE/PRT Specifies the copy output device.

FILE: Selects an external USB memory device.

PRT: Selects a printer.

Screen Shot Config Displays the File Config menu.

File Format PNG/BMP

Selects either PNG (portable network graphics) or BMP (bit map)

as the file format.

Auto Inc ON/OFF Sets the automatic incremental function of the file number.

ON: Increments the file number when the screen data is


copied.

OFF: The file COPYxxx.BMP(PNG) is overwritten.

Auto Inc Index Sets the start number to increment automatically.


Menu ON/OFF Hides the soft menu area when a copy is output.

ON: Displays the menu.
OFF: Hides the menu.

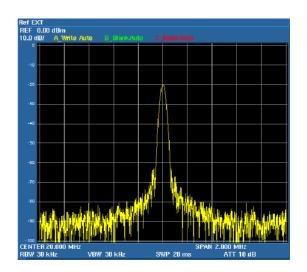

File Control

Displays the Shot File menu. Displays the Files window.

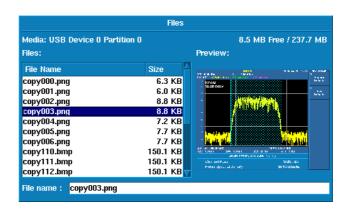

Rename File Changes the selected filename.

Remove File Deletes the selected file.

Write Protect ON/OFF

Write-protects the selected file.

ON: Prevents data from being written to the file.

OFF: Allows data to be written to the file.

Media

Selects the media on which to save data. Selects the external USB memory device in the dialog box.



NOTE: Data cannot be saved in the internal memory.

Print Config

Paper Format Selects the paper size and print direction.

Color Mode Color/Gray

Selects either color or gray scale in the Print Config mode.


Menu ON/OFF Displays or hides the soft menu when a file is printed.

ON: Displays the menu
OFF: Hides the menu.

Config Driver

Selects a printer driver to be used.

The Printer Driver Management window is displayed.



Driver files:

Printer drivers registered in this instrument are listed. Select a driver name to be used by using the knob.

Your choice:

The selected driver name is displayed.

Test driver:

Starts a test printing using the selected driver.

Default: This instrument automatically selects a driver.

Decides to use the selected driver. Use it:

Self Test Displays the Self Test menu.

> Executes the self-test. The self-test is the same as when the power turns on. **Execute Self Test**

> > Test Items


- Supply_Voltage
 Memory
- 3. CPU_Registers

- CPU Registers
 RF_Registers
 RF_PLL_LOCK
 LO_Registers
 LO_PLL_LOCK
 AIF_Registers
 AIF_PLL_LOCK
 TG_Registers
 TG_Registers
 Temperature

Initializes this instrument to the factory settings. Refer to "A.1 Initial Setting List." **Factory Init**

5.2.2 **APPLI**

Displays the APPLI menu.

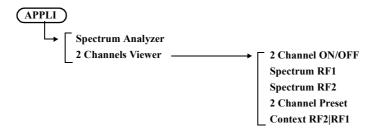

Spectrum Analyzer

2 Channels Viewer

Displays the 2 Channel menu.


Functions only for the U3771 or U3772.

2 Channel ON/OFF

Sets the 2 Channels Viewer mode.

The sweep and measurement are performed only for the active channel.

The active channel screen is enclosed within a red frame.

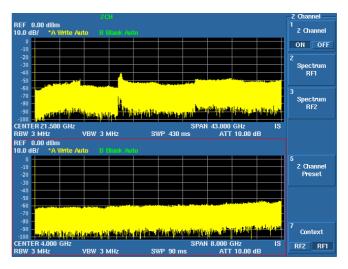

Splits the screen into an upper and lower windows. Upper window: RF INPUT 2 ON:

Lower window: RF INPUT 1

OFF: Cancels the dual-screen display.

The measurement display returns to the active channel

screen.

Spectrum RF1 Cancels the 2 Channel mode and enables RF INPUT 1. Spectrum RF2 Cancels the 2 Channel mode and enables RF INPUT 2. 2 Channel Preset Initializes the RF INPUT 1 and RF INPUT 2 settings.


Context RF2|RF1

Switches the active screen.

RF2: The RF2 (upper window) settings can be changed. RF1: The RF1 (lower window) settings can be changed.

5.2.3 FILE

Displays the File menu.

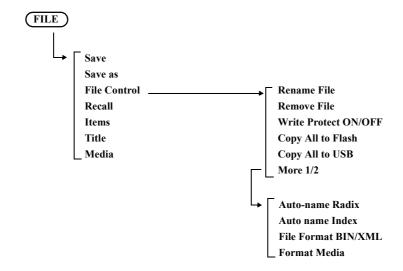

Save

Saves the items specified in Items to the memory device specified in Media.

The format in which to save data can be selected from either binary (.dat) or XML (eXtensible Markup Language) (.xml).

File size (For saving the setting data)

BIN: Approximately 4.8 KB XML: Approximately 16 KB

NOTE: Only binary data can be saved in the internal memory.


Save as

Specifies the filename and saves the file. Displays the Save As window.



File Control

Displays the File Control menu and Files window.

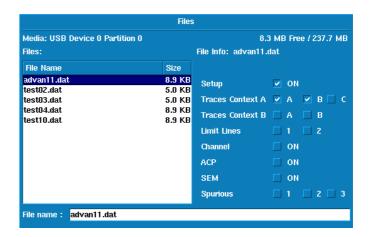

Rename File

Changes the selected filename.

Remove File

Deletes the selected file.

Write Protect ON/OFF

Write-protects the selected file.

ON: Prevents data from being written to the file.

OFF: Allows data to be written to the file.

Copy All to Flash

Copies all files in the USB memory key to the internal memory.

Copy All to USB

Copies all files in the internal memory to the USB memory key.

*:

- The file format that can be copied into the USB memory key is ".dat". The screen image cannot be copied.<-->\adv\dat.
- If the same file name exists in the USB memory key, the file is overwritten.
- Select USB memory from the Media menu.

More 1/2

Displays the File Ctrl menu (2/2).

Auto-name Radix

Defines the common part of the filename under which files are saved.

The file name follows the following format "Radix+Index". When a file is saved, an extension [.dat] is automatically added to the file name which is saved in the format "Radix+Index.dat". Radix can be up to six characters long.

Auto name Index

Specifies the Index part of the filename, under which files are saved.

The Index increments by 1 each time a file is saved. Zero to 99 can be specified in the Index.

File Format BIN/XML

BIN: Saves the data in binary format.

Only binary formats can be saved in the internal memory. The settings of files saved in binary format can be recalled.

XML: Saves the data in XML format.

Files which are saved in XML format can be read easily

but the settings cannot be recalled.

Format Media

Formats external USB memory devices.

Do not remove the memory device while the memory is being formatted.

Recall


Recalls file which was saved in binary format and displays the settings and trace data.

Displays the Recall window.

Execute Recall in the same mode as when the file was saved. Mode is displayed in File Info of the Recall window. The font color is green for a Recall-enabled file and red for a Recall-disabled file.


Green: Recall can be executed.

Red: Recall cannot be executed.

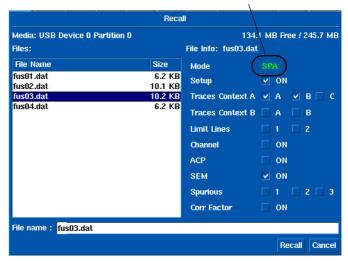

Items

Selects items to be saved. Displays the Items dialog box.



Setup: Saves the setting conditions.

Traces Context A A/B/C:

Saves the trace data.

Even if the Write mode is set, the setting is changed to the View mode while the trace data is recalled.

Traces Context B A/B

Limit Lines:Saves the Limit Line table.

Channel: Saves the Channel Formula table and Channel Table.

ACP: Saves CS/BS Table for the ACP.

SEM: Saves SEM Table.

Spurious 1/2/3:

Saves the Spurious Bands table.

Corr Factor:

Saves Correction Factor Table.

Normalize Context A/B/C:

Saves Normz Data that uses the TG.

Displays the Edit Title dialog box.

Edit Title

Title: abc

How to enter

Pressing a key cycles through a list of characters, which are allocated to that key, and displays them at the cursor position. If the key is not pressed for a few seconds after the previous key entry or another key is pressed, the displayed character is entered.

Table 5-1 Character allocation table

Key	Allocated Characters	
0	0	
	. space , ; :-+_=~#<>! ?	
-	[Back Space]	
1	1	
2	a b c 2	
3	def3	
4	g h i 4	
5	j k 1 5	
6	m n o 6	
7	p q r s 7	
8	tuv8	
9	w x y z 9	


Title

To enter a capital letter, hold down the **SHIFT** key and a key.

- 1. Enter a character by using the keypad.
- 2. Press a unit key such as the Hz key to finish entering the title.
- 3. Press **Title** to close the Edit Title dialog box.

Media

Displays the Media dialog box. Selects either the internal memory or an external USB memory device in the dialog box.



5.2.4 COPY

5.2.4 COPY

Outputs a screen image according to the conditions set by pressing SYSTEM, MORE 1/2, and COPY Config.

The COPY menu can also be displayed by pressing the SHIFT key and COPY key.

File size (For saving the image data)

PNG: Approximately 8 KB
BMP: Approximately 150 KB

5.2.5 HELP

Pressing the **HELP** key displays "HELP?" which indicates the HELP mode.

NOTE: The HELP file is loaded the first time the HELP key is pressed after the power is turned on.

When the HELP mode is set

Press a soft menu key to display the relevant menu description.


Press the soft menu key again to hide the display.


Press the **HELP** key again to cancel the HELP mode.

Procedure

- 1. Select a menu.
- Press the Help key.
- 3. Press a soft menu key.
- 4. Press the **HELP** key to cancel the HELP mode.
- 5. Repeat from step 1 to display the HELP of other menus.

Displays the Meas 1 menu.

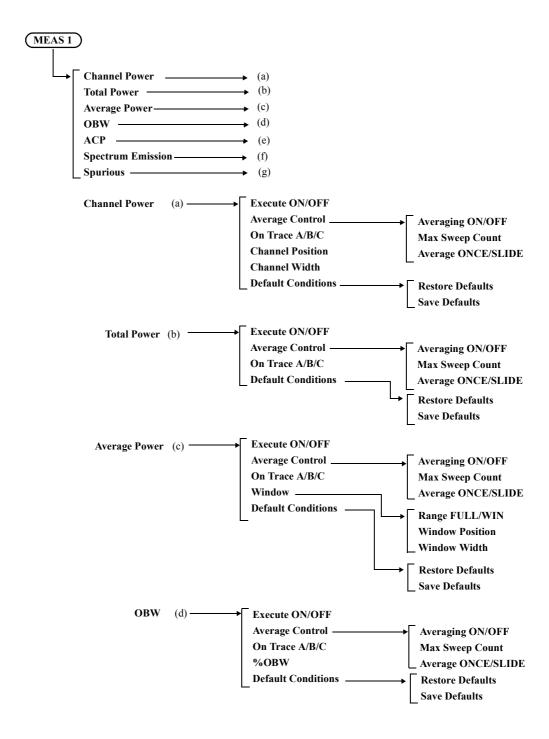

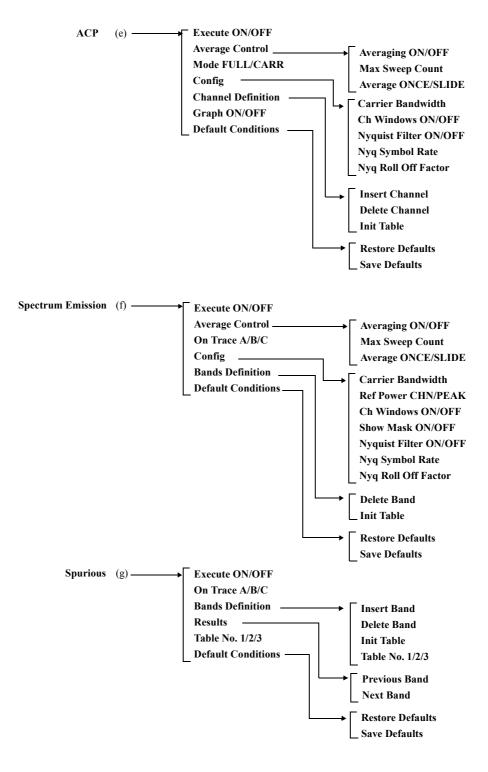

Channel Power

Activates the measuring window and displays the Channel P menu.

The channel power can be obtained by using the following equation.

$$P_{CH} = 10\log \left[\sum_{n=X1} \left(10^{\frac{P(n)}{10}}\right) \times \frac{1}{PBW} \times \frac{SPAN}{(X2-X1)}\right]$$

Pch: Channel power to be obtained

P(n): Displayed data at each trace point (dBm)

SPAN: Channel Width setting value PBW: Noise power bandwidth

X1: Trace point at the window's left edgeX2: Trace point at the window's right edge

Execute ON/OFF

ON: Performs a channel power measurement.

OFF: Cancels the channel power measurement.

Average Control Performs the average settings for the channel power measure-

nent.

Displays the Ch Avg menu.

Averaging ON/OFF Switches the averaging function ON and OFF.

ON: Measures the average channel power.

OFF: Cancels the averaging function.

Max Sweep Count Sets the number of times averaging is performed.

Up to 999 counts can be set.

Average ONCE/SLIDE

ONCE: Performs averaging for the set number of times and

then the process terminates.

SLIDE: Performs averaging for the set number of times and

then calculates the moving average.

On Trace A/B/C Selects a trace in which to execute the channel power measure-

ment.

Channel Position Activates the settings of the measuring window position.

Channel Width Activates the setting of the measuring window width.

Default Conditions Displays the Pow Default menu.

Restore Defaults Recalls the saved setting conditions.

Save Defaults Saves the currently set conditions.

Total Power Measures the total power in the measuring span.

Displays the Toal Pow menu.

The total power can be obtained by using the following equation.

P_T =
$$10\log \left[\sum_{n=X_1}^{X_2} \frac{P(n)}{10}\right] \times \frac{1}{PBW} \times \frac{SPAN}{1001}$$

PT: Total power to be obtained

P(n): Displayed data at each trace point (dBm)

SPAN: Span setting value

PBW: Noise power bandwidth

X1: 1 X2: 1001

Execute ON/OFF

ON: Performs a total power measurement.

OFF: Cancels the total power measurement.

Average Control Performs the average settings for the total power measurement.

Displays the Tot P Avg menu.

Averaging ON/OFF Switches the averaging function ON and OFF.

ON: Measures the average total power.

OFF: Cancels the averaging function.

Max Sweep Count Sets the number of times averaging is performed.

Up to 999 counts can be set.

Average ONCE/SLIDE

ONCE: Performs averaging for the set number of times and

then the process terminates.

SLIDE: Performs averaging for the set number of times and

then calculates the moving average.

On Trace A/B/C Selects a trace in which to perform the total power measurement.

Default Conditions Displays the Pow Default menu.

Restore Defaults Recalls the saved setting conditions.

Save Defaults Saves the currently set conditions.

Average Power

Measures the average power in the measuring range.

Displays the Average P menu.

The average power can be obtained by using the following

Pavg = $10\log \left[\sum_{n=X1} \frac{P(n)}{10}\right] \times \frac{1}{1001}$

PAVG: Average power to be obtained

P(n): Displayed data at each trace point (dBm)

X1. 1

X2: 1001

Execute ON/OFF

ON: Performs an average power measurement.

OFF: Cancels the average power measurement.

Average Control Performs the average settings for the average power measure-

ment.

Displays the Av P Avg menu.

Averaging ON/OFF Switches the averaging function ON and OFF.

> ON: Measures the average power.

OFF: Cancels the averaging function.

Max Sweep Count Sets the number of times averaging is performed.

Up to 999 counts can be set.

Average ONCE/SLIDE

ONCE: Performs averaging for the set number of times and

then the process terminates.

SLIDE: Performs averaging for the set number of times and

then calculates the moving average.

On Trace A/B/C Selects a trace in which to execute the average power measure-

ment.

Window Sets a measuring range in which to execute the average power

measurement.

Displays the Avg P Win menu.

Range FULL/WIN

FULL: Measures the average power in the full measuring span.

WIN: Measures the average power in the measuring window.

Window Position Sets the measuring window position. Window Width Sets the measuring window width.

Default Conditions Displays the Pow Default menu.

> **Restore Defaults** Recalls the saved setting conditions. **Save Defaults** Saves the currently set conditions.

OBW Displays the OBW menu.

Execute ON/OFF

ON: Performs an occupied bandwidth measurement.
OFF: Cancels the occupied bandwidth measurement.

Average Control

Averaging ON/OFF Switches the averaging function ON and OFF.

ON: Measures the occupied bandwidth power.

OFF: Cancels the averaging function.

Max Sweep Count Sets the number of times averaging is performed.

Up to 999 counts can be set.

Average ONCE/SLIDE

ONCE: Performs averaging for the set number of times and

then the process terminates.

SLIDE: Performs averaging for the set number of times and

then calculates the moving average.

On Trace A/B/C Selects a trace in which to execute the occupied bandwidth mea-

surement.

%OBW Sets the ratio of the occupied bandwidth power to the total power

in percentage.

The initial value is 99%.

Default Conditions Displays the OBW Default menu.

Restore Defaults Recalls the saved setting conditions.

Save Defaults Saves the currently set conditions.

ACP Displays the ACP menu.

Execute ON/OFF

ON: Performs the adjacent channel leakage power

measurement.

OFF: Cancels the adjacent channel leakage power

measurement.

Average Control

Averaging ON/OFF Switches the averaging function ON and OFF.

ON: Measures the adjacent channel leakage power.

OFF: Cancels the averaging function.

Max Sweep Count Sets the number of times averaging is performed.

Up to 999 counts can be set.

Average ONCE/SLIDE

ONCE: Performs averaging for the set number of times and

then the process terminates.

MUL: Performs averaging for the set number of times and

then calculates the moving average.

Mode FULL/CARR

FULL: Calculates the adjacent channel leakage power in relation to the reference power, the measurement of

which is taken from the full bandwidth on the screen.

CARR: Calculates the adjacent channel leakage power to the reference power, the measurement of which is taken

from the bandwidth set in Carrier Bandwidth.

Config Displays the ACP Cfg menu.

Carrier Bandwidth Sets the measurement bandwidth of channel power measurement

used as the reference power.

Ch Windows ON/OFF

ON: Displays the ACP channel window.

Nyquist Filter ON/OFF

OFF:

Switches the Nyquist filter function ON and OFF.

Closes the ACP channel window.

ON: Activates a Nyquist filter.

OFF: Cancels the Nyquist filter.

Nyq Symbol Rate Sets a symbol rate.

Nyq Roll Off Factor Sets a roll-off factor.

Channel Definition

Displays the ACP Ch menu.

Displays the CS/BS Table dialog box.

CS/BS Table				
[No]	[Channel Space]	[Channel Bandwidth]		
1	5.000 MHz	3.840 MHz		
2				
3				
4				
5				

[Channel Space]:

Sets the Offset frequency from the carrier frequency that shows the adjacent channel measuring position.

[Channel Bandwidth]:

Sets the measurement bandwidth used in the adjacent channel leakage power measurement.

Insert Channel Inserts a line, on which to set an adjacent channel measurement

condition, at the current cursor position.

The data in the line that existed in the position before insertion is copied to each setting value as new line data.

Delete Channel Deletes the measurement condition at the current cursor position.

Init Table Initializes the contents of the ACP channel table.

Graph ON/OFF

ON: Displays an ACP graph.

OFF: Hides the ACP graph.

Default Conditions Displays the ACP Default menu.

Restore Defaults Recalls the saved setting conditions.

Save Defaults Saves the currently set conditions.

Spectrum Emission Displays the SEM (Spectrum Emission Mask) menu.

Execute ON/OFF

ON: Performs a spectrum emission mask measurement.

OFF: Terminates the spectrum emission mask measurement.

Average Control Displays the SEM Avg menu.

Averaging ON/OFF Switches the averaging function ON and OFF.

ON: Measures the spectrum emission mask.

OFF: Cancels the averaging function.

Max Sweep Count Sets the number of times averaging is performed.

Up to 999 counts can be set.

Average ONCE/SLIDE

ONCE: Performs averaging for the set number of times and

then the process terminates.

SLIDE: Performs averaging for the set number of times and

then calculates the moving average.

On Trace A/B/C Selects a trace in which to execute the spectrum emission mask

measurement.

Config Displays the SEM Cfg menu.

Carrier Bandwidth Sets the power conversion bandwidth for carrier signals.

Ref Power CHN/PEAK

Switches the calculation mode of the reference power between the

Channel mode and the Peak Power mode.

CHN: Calculates the channel power and sets the result as the

reference power for the mask measurement.

PEAK: Sets the Peak power value of the waveform as the

reference power for the mask measurement.

Ch Windows ON/OFF

ON: Displays the SEM window.

OFF: Hides the SEM window.

Show Mask ON/OFF

ON: Displays the Mask line.

OFF: Hides the Mask line.

Nyquist Filter ON/OFF

Switches the Nyquist filter function ON and OFF.

ON: Activates the Nyquist filter.

OFF: Cancels the Nyquist filter.

Nyq Symbol Rate Sets a symbol rate.

Nyq Roll Off Factor Sets a roll-off factor.

Bands Definition Displays the SEM Bands menu and SEM Table window.

Delete Band Deletes a column of measurement conditions from the current

cursor position.

Init Table Initializes all data in the table.

SEM Table					
[No]	1	2	3		
[Start]					
[Stop]					
[IBW]					
[Judge]	Absolute	Absolute	Absolute		
	Relative	Relative	Relative		
	Abs and Rel	Abs and Rel	Abs and Rel		
	Abs or Rel	Abs or Rel	Abs or Rel		
[Lim Abs Start]					
[Lim Abs Stop]					
[Lim Rel Start]					
[Lim Rel Stop]					

[Start] Sets the offset frequency from the center frequency as the start frequency of the emission mask judgment frequency band.

[Stop] Sets the offset frequency from the center frequency as the stop frequency of the emission mask judgment frequency band.

[Integral BW] Sets the power integral bandwidth at each frequency point.

Specifies how to compare the waveform with the set mask values (absolute or relative values) when the mask judgment is performed.

Absolute: Compares the waveform with the mask values set in Limit Abs Start and Limit Abs Stop. If the waveform is equal to or less than the mask values, the result is Pass.

Relative: Compares the waveform with the mask values set in Limit Rel Start and Limit Rel Stop. If the waveform is equal to or less than the mask values, the result is Pass.

Abs and Rel:

[Judge]

Compares the waveform with both the Limit Abs Start, Limit Abs Stop values and the Limit Rel Start, Limit Rel Stop values. If both conditions are satisfied, Pass is displayed.

Abs or Rel:

Compares the waveform with both the Limit Abs Start, Limit Abs Stop values and the Limit Rel Start, Limit Rel Stop values. If either of the conditions is satisfied, Pass is displayed.

[Limit Abs Start] Sets the absolute mask value at the position of the start frequency.

[Limit Abs Stop] Sets the absolute mask value at the position of the stop frequency.

A mask value at a position between the start and stop frequencies is calculated by using the linear interpolation.

[Limit Rel Start] Sets the relative mask value at the position of the start frequency.

The set mask value is used to compare with the offset value from the measured reference power.

[Limit Rel Stop] Sets the relative mask value at the position of the stop frequency. A mask value at a position between the start and stop frequencies is calculated by using the linear interpolation.

Default Conditions Displays the SEM Default menu.

Restore Defaults Recalls the saved setting conditions.

Save Defaults Saves the currently set conditions.

Spurious Displays the Spurious menu.

Execute ON/OFF

ON: Performs the spurious measurement.

OFF: Terminates the spurious measurement.

On Trace A/B/C Selects a trace in which to execute the spurious measurement.

Bands Definition Displays the Spr Config menu.

At the same time, the Spurious Bands setting window is displayed.

The start and stop frequencies of the spurious measurement band, the RBW, VBW, sweep time, attenuator, reference level, preamp ON or OFF, and the judgment level value used in the measurement can be set in the Spurious Bands setting window.



Insert Band Inserts a column, in which spurious measurement conditions can

be set, at the current cursor position.

The data contained in the row that existed in the position before

insertion is copied to each setting value as new row data.

Delete Band Deletes a column of measurement conditions from the current

cursor position.

Init Table Initializes all data in the table currently being edited.

Table No. 1/2/3 Sets the setting sequence table number for the spurious measure-

ment to 1, 2, or 3.

1: Sets table number 1.

2: Sets table number 2.

3: Sets table number 3.

Results Displays the Spr Results menu.

Displays Spurious Measure Results Table.

Previous Band Displays the previous screen.

Next Band Displays the next screen.

Table No. 1/2/3 Sets the setting sequence table number for the spurious measure-

ment to 1, 2, or 3.

1: Sets table number 1.

2: Sets table number 2.


3: Sets table number 3.


Default Conditions Displays the Spr Default menu.

Restore Defaults Recalls the saved setting conditions.

Save Defaults Saves the currently set conditions.

5.2.7 MEAS 2

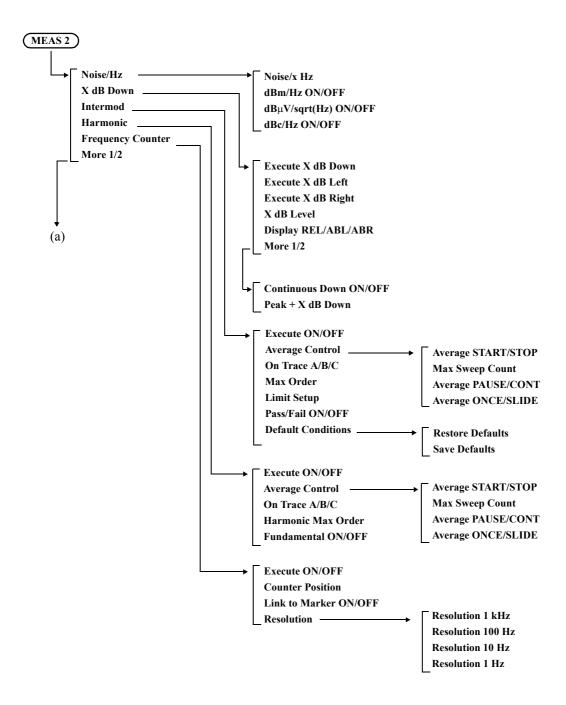

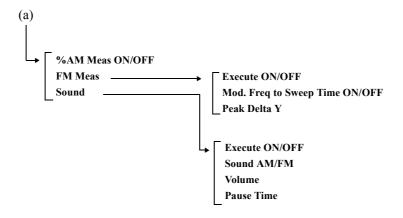

Noise/Hz

Displays the Noise/Hz menu.

Noise/x Hz

Activates settings of the noise measurement bandwidth.

The initial value is 1 Hz.

dBm/Hz ON/OFF

ON:

Displays the marker automatically if the marker is set to

OFF.

Sets the vertical axis unit to dBm and sets the marker

unit to dBm/Hz.

OFF: Terminates the dBm/Hz function.

dBµV/sqrt(Hz) ON/OFF

ON: Displays the marker automatically if the marker is set to

OFF.

Sets the vertical axis unit to dBµV and sets the marker

unit to $dB\mu V/sqrt(Hz)$.

OFF: Terminates the dBµV/sqrt(Hz) function.

dBc/Hz ON/OFF

ON: Automatically sets the marker to the delta marker mode

if the marker is set to OFF.

Sets the delta marker unit to dBc/Hz.

OFF: Terminates the dBc/Hz function.

X dB Down Displays the X dB Down menu.

Displays the marker automatically if the marker is set to OFF. The trace, for which the X dB Down function is executed, is the

active trace.

Set the marker on the active trace.

Execute X dB Down According to the Mode setting, displays a normal marker and a

delta marker X dB lower than the current position.

Execute X dB Left Displays a normal marker to the left of and X dB lower than the

current position.

Execute X dB Right Displays a normal marker to the right of and X dB lower than the

current position.

X dB Level Activates the X dB Level setting.

Display REL/ABL/ABR Sets the display method of the X dB Down marker data.

REL: Sets the marker to the delta marker mode when X dB

Down is executed.

Displays a normal marker on the right and a delta

marker on the left.

ABL: Displays the left marker as an absolute value.

ABR: Displays the right marker as an absolute value.

More 1/2 Displays the XdB 2/2 menu.

Continuous Down ON/OFF Switches the continuous X dB down function ON and OFF.

ON: Repeats Peak X dB down in every sweep.

OFF: Cancels the continuous X dB down function.

Peak + X dB Down Performs the peak search in the search range and then executes X

dB Down.

Intermod Displays the Intermod menu.

Execute ON/OFF

ON: Performs the intermodulation measurement.

OFF: Terminates the intermodulation measurement.

Average Control

Average START/STOP

START: Performs averaging.

STOP: Cancels averaging.

Max Sweep Count Sets the number of times Video averaging is performed.

Up to 999 counts can be set.

Average PAUSE/CONT

PAUSE: Pauses averaging and displays the current number of

times averaging has been performed.

CONT: Restarts averaging from the point at which averaging

was paused.

Average ONCE/SLIDE

ONCE: Performs averaging for the set number of times and

then the process terminates.

SLIDE: Performs averaging for the set number of times and

repeats averaging continuously by using the last data.

On Trace A/B/C Selects a trace in which to execute the inter-modulation measure-

ment.

Max Order Sets the measuring order. The third, fifth, seventh, and ninth

orders can be set.

Limit Setup Displays the Limit Setup dialog box.

[3rd Order Limit]:

Sets the limit value of the third-order distortion signal.

[5th Order Limit]:

Sets the limit value of the fifth-order distortion signal.

[7th Order Limit]:

Sets the limit value of the seventh-order distortion signal.

[9th Order Limit]:

Sets the limit value of the ninth-order distortion signal.

Limit Setup			
3rd Order Limit	0.00 dB		
5th Order Limit	0.00 dB		
7th Order Limit	0.00 dB		
9th Order Limit	0.00 dB		

Pass/Fail ON/OFF

Switches the Pass/Fail judgment due to the comparison with the limit value set in the Limit Setup dialog box ON and OFF.

ON: Performs the Pass/Fail judgment.

If the measurement result is larger than the set limit

value, a Fail judgment is performed.

OFF: Does not perform the Pass/Fail judgment.

Default Conditions Displays the IM Default menu.

Restore Defaults Recalls the saved setting conditions.

Save Defaults Saves the currently set conditions.

Harmonic Displays the Harmonic menu.

Execute ON/OFF

ON: Executes the harmonic measurement function.

OFF: Terminates the harmonic measurement function.

Average Control

Average START/STOP

START: Performs averaging.
STOP: Cancels averaging.

Max Sweep Count

Sets the number of times Video averaging is performed.

Up to 999 counts can be set.

Average PAUSE/CONT

PAUSE: Pauses averaging and displays the current number of

times averaging has been performed.

CONT: Restarts averaging from the point at which averaging

was paused.

Average ONCE/SLIDE

ONCE: Performs averaging for the set number of times and

then the process terminates.

SLIDE: Performs averaging for the set number of times and

repeats averaging continuously by using the last data.

On Trace A/B/C Selects a trace in which to execute the harmonic measurement.

Harmonic Max Order Sets the measuring harmonic order.

The measuring order can be set from 1 to 10.

The default value is 3.

Fundamental ON/OFF

ON: Sets the fundamental frequency.

The measuring span is set in the range that includes the fundamental and set harmonic order frequencies.

OFF: Sets the current center frequency to the fundamental

frequency.

Frequency Counter Displays the Counter menu.

Execute ON/OFF

ON: Sets a frequency counter mode.

OFF: Cancels the frequency counter mode.

Counter Position Adjusts a cursor on the measured signal.

Link to Marker ON/OFF Corresponds the cursor at the counter position with the marker

osition

If the marker position moved, then the counter position also

moved.

OFF: Cancels the function.

Resolution Displays the Cnt Res menu.

Resolution 1 kHz Sets the resolution of the frequency counter to 1 kHz.

Resolution 100 Hz Sets the resolution of the frequency counter to 100 Hz.

Resolution 10 Hz Sets the resolution of the frequency counter to 10 Hz

Resolution 1 Hz Sets the resolution of the frequency counter to 1 Hz.

More 1/2 Displays the Meas 2 2/2 menu.

%AM Meas ON/OFF Switches ON and OFF the %AM modulation factor measurement.

ON: Acquires an AM modulation factor and modulation

frequency by using the peak search function and

displays a calculation result in percentage.

OFF: Cancels the %AM function.

5.2.7 MEAS 2

FM Meas

Displays the FM Meas menu.

Execute ON/OFF

Switches ON and OFF the frequency deviation measurement function.

ON: Measures the frequency deviation of an FM signal.

OFF: Cancels the frequency deviation measurement function

of an FM signal.

A value of Peak Delta Y is used as a condition of performing the peak search.

If setting the Mod. Freq to Sweep Time ON/OFF menu to ON and setting a modulation frequency in advance, a optimum sweep time is automatically set based on the modulation frequency and the number of display points.

If OFF is set for the Mod. Freq to Sweep Time ON/OFF menu, a sufficient sweep time must be set according to the following formula:

 $SWP > PT \times 1 / Fmod$

SWP: Sweep time

PT: The number of display trace points

Fmod: Modulation frequency

(When the FM Meas function is selected, the trace detector is automatically set to the Posi mode.)

Mod. Freq to Sweep Time ON/OFF

Switches ON and OFF a mode, in which a sweep time is determined based on a modulation frequency.

ON: Sets a modulation frequency and then sets a sweep time

based on the modulation frequency.

OFF: Cancels a mode in which a modulation frequency is set.

A value set for SWP Time AUTO/MNL is applied to a sweep time when measurement starts.

Peak Delta Y

Sets a level difference for a signal to be judged as a peak point during the peak search. A level difference set here is used as a threshold level while searching for a peak value.

Sound Displays the Sound menu.

For a signal where the marker is positioned, sound demodulation is performed when a sweep ends.

Execute ON/OFF Switches the sound demodulation function ON and OFF.

ON: Outputs the demodulated sound signal to the PHONE

terminal on the front panel.

OFF: Cancels the sound demodulation function.

Sound AM/FM Switches the demodulation mode between AM and FM.

AM: Selects the AM demodulation.
FM: Selects the FM demodulation.

5-41

5.2.7 MEAS 2

Volume

Sets the demodulated sound volume. The sound volume can be adjusted in 16 levels.

Pause Time


Sets the demodulation time. The setting range is from 100 ms to 1000 s.

Displays the Trace menu and performs the settings related to the trace.

The Trace menu includes the trace selection menu, which corresponds to the menu key 7. The trace is changed each time the key is pressed; $A \rightarrow B \rightarrow C$.

Trace A/B/C

A: Selects trace memory A.B: Selects trace memory B.C: Selects trace memory C.

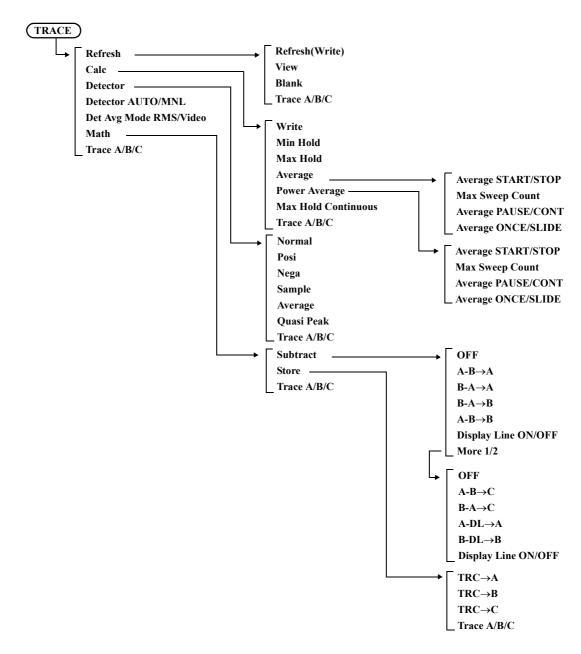

Refresh Displays the Refresh Mode menu.

The selected setting is displayed at the bottom of the menu.

Refresh(Write) Refreshes trace data in each sweep.

View Displays the trace data stored in the memory.

Blank Hides the trace.

Traces A, B, and C cannot be set to Blank at the same time.

Trace A/B/C Selects the applied trace memory.

Calc Displays the Calc Mode menu.

The selected setting is displayed at the bottom of the menu.

Write Displays the waveform data acquired in the default settings.
Min Hold Displays the minimum value of points in each trace sample.
Max Hold Displays the maximum value of points in each trace sample.

Average Displays the Video Average menu.

The Video average performs averaging of the display data.

Average START/STOP

START: Performs averaging.

STOP: Cancels averaging.

Max Sweep Count Sets the number of times Video averaging is performed.

Up to 999 counts can be set.

Average PAUSE/CONT

PAUSE: Pauses averaging and displays the current number of

times averaging has been performed.

CONT: Restarts averaging from the point in which averaging

was paused.

Average ONCE/SLIDE

ONCE: Performs averaging for the set number of times and

then the process terminates.

SLIDE: Performs averaging for the set number of times and

repeats averaging continuously by using the last data.

Power Average Displays the Power Average menu.

Performs averaging of power (W) and draws waveforms.

Average START/STOP

START: Performs averaging.

STOP: Cancels averaging.

Max Sweep Count Sets the number of times Video averaging is performed.

Up to 999 counts can be set.

Average PAUSE/CONT

PAUSE: Pauses averaging and displays the current number of

times averaging has been performed.

CONT: Restarts averaging from the point in which averaging

was paused.

Average ONCE/SLIDE

ONCE: Performs averaging for the set number of times and

then the process terminates.

SLIDE: Performs averaging for the set number of times and

then calculates the moving average.

Max Hold Continuous Displays the maximum value for each trace sample.

The trace is not reset in this function which is different from the

Max Hold function in the Calc menu.

The Max Hold operation starts at a trace point when the key is

pressed

This function can be used when the Detector mode is set to MNL.

Trace A/B/C Selects the applied trace memory.

Detector Displays the Detector menu.

The selected setting is displayed at the bottom of the menu.

Normal Sets the normal detection mode, in which a positive or negative

peak is automatically detected at each trace point.

Posi Sets the positive peak detection mode.

Nega Sets the negative peak detection mode.

Sample Sets the sample detection mode.

Average Sets the average detection mode.

The average detection mode includes RMS (power average) and Video (Trace average), which can be selected in the Det Avg

Mode menu.

Quasi Peak Sets the quasi peak detection mode.(OPT28)

Quasi Peak (QP) can be set when EMC Filter ON (refer to Section

5.2.17, "CPL (Coupled function)") and RBW < 1 MHz.

According to the RBW setting, set an appropriate sweep time

using the following conditions as a guide:

Trace A/B/C Selects the applied trace memory.

Detector AUTO/MNL Switches the detection mode between the auto and manual set-

tings.

AUTO: Automatically sets the optimum detection mode for

measurement based on the trace mode.

MNL: Sets the detection mode manually.

Det Avg Mode RMS/Video

RMS: Selects RMS (power average).

Video: Selects Video (Trace average).

5-45

Math Displays the Math menu.

Subtract Displays the Subtract menu.

The selected setting is displayed at the bottom of the menu.

OFF Does not perform the trace calculation.

 $A-B\rightarrow A$ When trace A is set to the Write mode, the data in memory B is

subtracted from the data acquired in the sweep and the result is

entered into memory A.

B-A→**A** When trace A is set to the Write mode, the data acquired in the

sweep is subtracted from the data in memory B and the result is

entered into memory A.

 $B-A \rightarrow B$ When trace B is set to the Write mode, the data in memory A is

subtracted from the data acquired in the sweep and the result is

entered into memory B.

A-B→B When trace A is set to the Write mode, the data acquired in the

sweep is subtracted from the data in memory A and the result is

entered into memory B.

Display Line ON/OFF

ON: Displays and activates the display line.

OFF: Cancels the display line.

More 1/2 Displays the Subtract 2/2 menu.

OFF Does not perform the trace calculation.

 $A-B \rightarrow C$ When trace A is set to the Write mode, the data in memory B is

subtracted from the data acquired in the sweep and the result is

entered into memory C.

B-A→C When trace A is set to the Write mode, the data acquired in the

sweep is subtracted from the data in memory B and the result is

entered into memory C.

 $A-DL\rightarrow A$ When trace A is set to the Write mode, the data on the display line

is subtracted from the data acquired in the sweep and the result is

entered into memory A.

 $B-DL \rightarrow B$ When trace B is set to the Write mode, the data on the display line

is subtracted from the data acquired in the sweep and the result is

entered into memory B.

Display Line ON/OFF

ON: Displays and activates the display line.

OFF: Cancels the display line.

Store Displays the Store menu.

Copies the active trace data and sets to the View mode.

TRC→A Saves the active trace data to trace memory A.

TRC→B Saves the active trace data to trace memory B.

TRC→C Saves active trace data to trace memory C.


Trace A/B/C Selects the applied trace memory.


Trace A/B/C Selects the applied trace memory.

Trace A/B/C Selects the applied trace memory.

5.2.9 MKR

Displays the Marker menu and an active marker by pressing the **MKR** key. The frequency and level on the marker are displayed in the marker area.

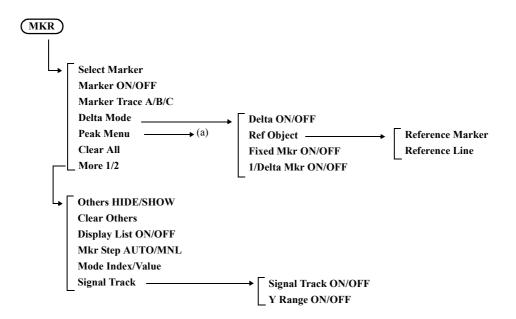

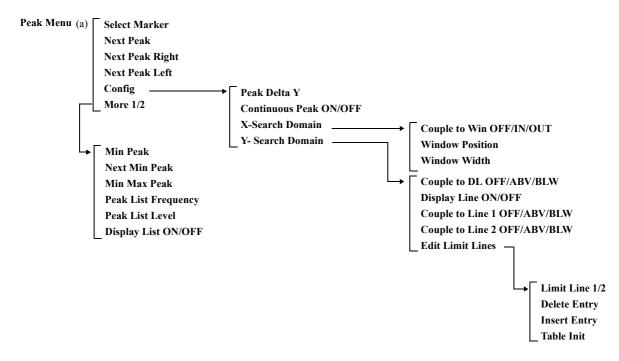

5.2.9 MKR

Select Marker Selects the active marker and sets its position.

The marker number increases by one each time the key is pressed.

The marker number cycles from 1 to 10:

1-2-3-4-5-6-7-8-9-10-1-

The marker number decreases by one if SHIFT is pressed and

then **Select Marker** is pressed.

Marker ON/OFF Activates the marker selected by Select Marker.

Marker Trace A/B/C Moves the active marker to the selected trace.

Delta Mode Displays the Delta Marker menu.

Delta ON/OFF Switches the delta marker display function ON and OFF.

ON: Displays a delta marker at the same position as a normal

marker.

The relative values of frequency and level to the normal

marker are displayed in the marker area.

OFF: Hides the delta marker.

Ref Object Sets the reference in the delta marker mode.

Reference Marker Selects the reference marker. **Reference Line** Selects the reference line.

Fixed Mkr ON/OFF Switches the fixed marker function ON and OFF.

ON: Maintains the frequency and level of the delta marker.

OFF: Cancels the fixed marker function.

1/Delta Mkr ON/OFF Switches the inverse number display function for the delta marker

value ON and OFF.

ON: Displays a frequency value on the time axis and a time

value on the frequency axis.

OFF: Cancels the inverse number display function.

Peak Menu Displays the Peak menu.

Does not move the marker. Refer to "5.2.10 PEAK".

Clears all markers.

The marker display position is set at the center of the screen

(default value).

More 1/2 Displays the Marker 2/2 menu.

Others HIDE/SHOW Hides all markers except for the active marker.

Clear Others Clears all markers except for the active marker.

Display List ON/OFF Switches the list display of enabled markers ON and OFF.

ON: Displays a list of frequencies and levels in order of

marker number.

OFF: Hides the display of marker list.

Mkr Step AUTO/MNL Switches the step size between auto and manual settings when the

marker is moved by the step key.

AUTO: Sets the marker step size to 1/10 of the frequency span.

MNL: Sets the step size manually.

5.2.9 MKR

Mode Index/Value Selects either Index or Value as the marker position setting.

Index: Maintains the marker position at the point on the screen.

If the center frequency is changed, the marker does not move and remains at the same position on the screen.

Value: The marker position retains the frequency information.

If the center frequency is changed, the marker position

moves according to the frequency.

Signal Track Displays the Sig Track menu.

Signal Track ON/OFF Switches the signal truck function ON and OFF.

ON: Performs the peak search for the same peak in each

sweep, and sets the marker frequency to the center

frequency.

OFF: Cancels the signal truck function.


Y Range ON/OFF Sets the margin when the signal track function detects the peak.

5.2.10 PEAK

5.2.10 PEAK

Displays the Peak menu.

Displays the marker at the maximum level of the trace in the search range and displays the frequency and level of the marker. However, the frequency of the feed-through (zero carrier) is excluded.

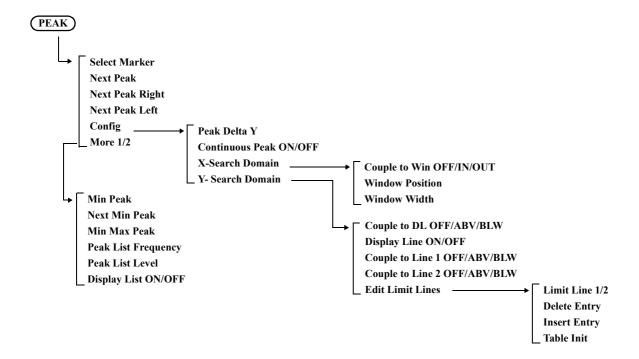

Select Marker Selects the active marker.

The marker number increases by one each time the key is pressed. The marker number decreases by one if **SHIFT** is pressed and

then **Select Marker** is pressed.

Next Peak Moves the marker to the next highest peak from the current

marker position in the search range.

Next Peak Right Moves the marker to the next peak on the right (higher frequency

than the current marker position) in the search range.

Next Peak Left Moves the marker to the next peak on the left (lower frequency

than the current marker position) in the search range.

Config Displays the Peak Cfg menu.

Peak Delta Y Sets the level difference from the peak, in which a signal is recog-

nized as a peak point during the peak search.

This level difference is used as the threshold level for the peak

point search.

Continuous Peak ON/OFF Switches the continuous peak search function ON and OFF.

ON: Repeats the peak search in each sweep.

OFF: Cancels the continuous peak search function.

X-Search Domain Displays the X PK Area menu.

Couple to Win OFF/IN/OUT

Sets a peak search range on the horizontal axis.

OFF: Sets the full range on the screen as the search range.

IN: Sets the inside of the displayed window as the search

range.

OUT: Sets the outside of the displayed window as the search

range.

Window Position Sets the center position of the window defined by Couple to Win.

Window Width Sets the window width defined by Couple to Win.

Y- Search Domain Displays the Y PK Area menu.

Couple to DL OFF/ABV/BLW

Sets a peak search range on the vertical axis.

OFF: Sets the full range as the search range.

ABV: Sets the range above the display line as the search

range.

BLW: Sets the range below the display line as the search

range.

Display Line ON/OFF

ON: Displays the display line.

Sets the position of the display line.

OFF: Hides the display line.

Couple to Line 1 OFF/ABV/BLW

Specifies the search range for limit line 1.

OFF: Does not specify the search range related to limit line 1.

ABV: Specifies the range above limit line 1 as the search

range.

BLW: Specifies the range below limit line 1 as the search

range.

Couple to Line 2 OFF/ABV/BLW

Specifies the search range for limit line 2.

OFF: Does not specify the search range related to limit line 2.

ABV: Specifies the range above limit line 2 as the search

range.

BLW: Specifies the range below limit line 2 as the search

range.

5.2.10 PEAK

Edit Limit Lines Displays the Limit Line menu and Limit Line table.

Limit Line				
[No]	[Frequency]	[Level]		
1				
2				
3				
4				
5				

Limit Line 1/2

1: Edits limit line 1.

2: Edits limit line 2.

Delete Entry Deletes a line on which the cursor is positioned in the limit line

table

Insert Entry Inserts a line in the limit line table.

Table Init Clears all settings in the limit line table.

More 1/2 Displays the Peak 2/2 menu.

Min Peak Moves the active marker to the minimum value of the trace in the

search range.

Next Min Peak Moves the marker to the next lowest peak from the current marker


position in the search range.

Min Max Peak Automatically sets the delta marker mode, moves the reference

marker to the maximum value, and moves active marker to the

minimum value.

Peak List Frequency Lists peak levels and peak frequencies in order of frequency.

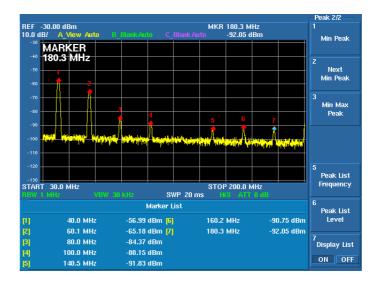

5.2.10 PEAK

Peak List Level
Display List ON/OFF

Lists peak levels and peak frequencies in order of peak level.

Switches the peak list display.

ON: Displays the list.
OFF: Hides the list.


5.2.11 MKR→

5.2.11 MKR→

If the MKR

key is pressed, active marker data such as the frequency and level can be used as the data of other function

Displays the Mkr to menu.



Mkr to CF Sets the frequency of the active marker to the center frequency.

Mkr to Ref Sets the level of the active marker to the reference level.

Peak to CF Displays the marker at the highest peak in the search range and

sets the center frequency to the frequency of the marker.

Peak to Ref Displays the marker at the highest peak in the search range and

sets the reference level to the level of the marker.

Delta to Span Sets the frequency span to the difference between the frequencies

of the delta marker and the normal marker.

Delta to CF Sets the center frequency to the difference between the frequen-

cies of the delta marker and the normal marker.

More 1/2 Displays the Mkr to 2/2 menu.

Mkr to CF Step Sets the step size of the center frequency to the frequency of the

marker as.

Delta to CF Step Sets the step size of the center frequency to the difference between

the frequencies delta marker and the normal marker as.

Mkr to Mkr Step Sets the step size of the marker to the frequency of the marker.


Delta to Mkr Step Sets the step size of the marker to the difference between the fre-

quencies of the delta marker and the normal marker.

5.2.12 TG (Option)

5.2.12 TG (Option)

Displays the TG menu.

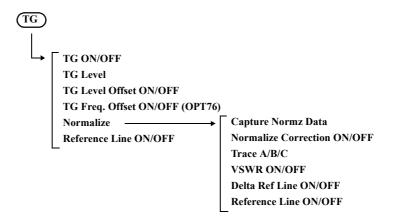

TG ON/OFF

ON: Turns on a tracking generator.

OFF: Turns off the tracking generator.

TG Level Sets the output level of the tracking generator.

Setting range

0 dBm to -30 dBm (OPT77) 0 dBm to -60 dBm (OPT76)

TG Level Offset ON/OFF

Switches the TG level offset function ON and OFF.

ON: The offset level can be set in the range of 0 ± 100.0 dB. The relationship between the displayed TG level, set

TG level, and offset is as follows:

Displayed TG level = Set TG level + Offset

OFF: Cancels the offset function.

TG Freq. Offset ON/OFF

Adds the offset frequency to the TG output frequency. It functions with OPT76.

ON: The offset frequency can be set in the range of 0 Hz to

+1 GHz and the resolution of approx. 1 kHz.

The output frequency is up to 3 GHz even if adding the

offset frequency.

OFF: Cancels the offset function.

Normalize Displays the TG Normz menu.

Capture Normz Data Acquires the normalization data at the position of the reference

line

Normalize Correction ON/OFF

ON: Normalizes the measurement data by using the

normalization data.

Only trace A can be normalized.

OFF: Cancels the normalization function.

5.2.12 TG (Option)

Selects the trace memory in which the data to be normalized is acquired and the normalization function is performed. Trace A/B/C

VSWR ON/OFF Displays a return loss and VSWR as marker values.

When performing a measurement, advance normalization with the SWR bridge must be executed.

Refer to Section 4.4.7, "VSWR Measurement".

Displays Return Loss and VSWR. R.L = $20 \log \rho$ VSWR = $(1+\rho)/(1-\rho)$

OFF: Cancels the Return Loss and VSWR displays.

Delta Ref Line ON/OFF

ON: Sets the marker to ON and displays the level difference

to the reference line. (MK Δ)


OFF: Hides the MK Δ display.

Reference Line ON/OFF

Displays the reference line and sets its display position. ON:

OFF: Hides the reference line.

Displays the Frequency menu.

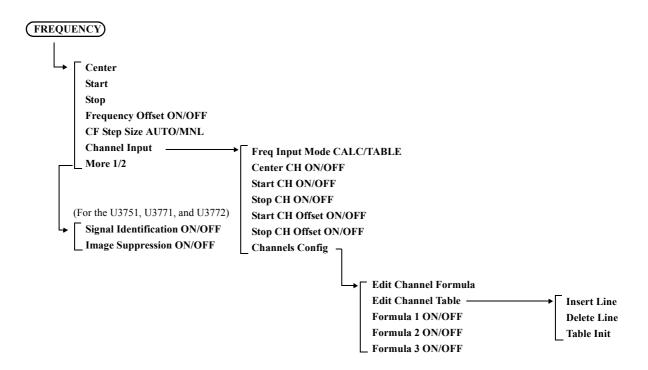

Center Sets the center frequency.

The frequency range is displayed by the center frequency and fre-

quency span.

Start Sets the start frequency.

The frequency range is displayed by the start frequency and stop

frequency.

Stop Sets the stop frequency.

CF Step Size AUTO/MNL

The frequency range is displayed by the start frequency and stop

frequency.

Frequency Offset ON/OFF Switches the frequency offset function ON and OFF.

ON: Sets the offset value and changes only the display of the

frequency by the offset value.

(Displayed value of frequency = Set value + Offset

value)

OFF: Cancels the offset function.

Switches the step size between auto and manual settings when the center frequency is changed by the step key.

AUTO: Automatically sets the step size to 1/10 of the span

width.

MNL: Sets the step size manually.

Channel Input Displays the Channel menu.

Uses the channel code instead of the frequency for the frequency

setting.

Freq Input Mode CALC/TABLE

Selects the channel input format.

CALC: Acquires a frequency from a channel number by using

the mathematical formula.

TABLE: Acquires a frequency from a look-up table, which

corresponds to a channel number.

Center CH ON/OFF Sets the center frequency input mode to the channel.

ON: Sets the channel code input mode.

OFF: Sets the frequency input mode.

Start CH ON/OFF Sets the start frequency input mode to the channel.

ON: Sets the channel code input mode.

OFF: Sets the frequency input mode.

Stop CH ON/OFF Sets the stop frequency input mode to the channel.

ON: Sets the channel code input mode.
OFF: Sets the frequency input mode.

Start CH Offset ON/OFF Switches the start frequency offset function ON and OFF when

the channel input mode is set.

ON: Sets the offset value.

Start frequency = Carrier frequency (Start channel) -

start offset frequency

OFF: Cancels the offset function.

Stop CH Offset ON/OFF Switches the stop frequency offset function ON and OFF when

the channel input mode is set.

ON: Sets the offset value.

Stop frequency = Carrier frequency (Stop channel) +


stop offset frequency

OFF: Cancels the offset function.

Channels Config Displays the Channels Config menu.

Edit Channel Formula Displays the dialog box in which the mathematical formula to acquire the channel set frequency is defined.

The set frequency is as follows: Carrier frequency = Origin + CH spacing * (CH No. - CH offset)

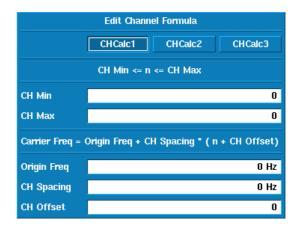

Edit Channel Table Displays the dialog box used to set the channel table.

Channel Table				
[No]	[Channel Number]	[Carrier Frequency]		
1				
2				
3				
4				
5				
6				
7				
8				
9				
10				

Insert Line Inserts a line in the channel table.

Delete Line Deletes the line where the cursor is positioned.

Table Init Initializes the channel table. Clears all settings.

Formula 1 ON/OFF Formula 2 ON/OFF Formula 3 ON/OFF

Sets the mathematical formula used in the channel input mode. This function is enabled when Freq Input Mode is set to CALC.

More 1/2 Displays the Frequency 2/2 menu.

Signal Identification ON/OFF (U3751/U3771/U3772)

ON: Turns on the Signal Identification function.

Image signals shift on the screen but the signals do not

move in each sweep.

OFF: Cancels the Signal Identification function.

Image Suppression ON/OFF (U3751/U3771/U3772)

ON: Turns on the Image Suppression function.

Detects image signals and deletes them from the

display.

OFF: Cancels the Image Suppression function.

5.2.14 SPAN

SPAN

Span

Full Span

Zero Span

Last Span

Peak Zoom

Auto Tune

Span Sets the frequency span.

The frequency range is displayed by the center frequency and fre-

quency span.

Full Span Sets the frequency span to full span. (SPAN - 8 GHz)

Zero Span Sets the zero span mode at the center frequency.

Last Span Returns the frequency span to the previous value.

Peak Zoom Displays the marker at the highest peak in the targeted search range and sets the frequency of the marker to the center frequency.

At this time, the frequency span is changed to 1/10 of the currently

set value.

Auto Tune Searches the maximum signal level in the full band and captures

the signal, then finally sets the frequency span to a value before

AUTŎ TÚNE starts.


The reference level is set to the peak level of the searched signal.

ON: Starts AUTO TUNE.
OFF: Stops AUTO TUNE.

5.2.15 AMPLITUDE

5.2.15 AMPLITUDE

Displays the Level menu and enables the settings related to the amplitude display.

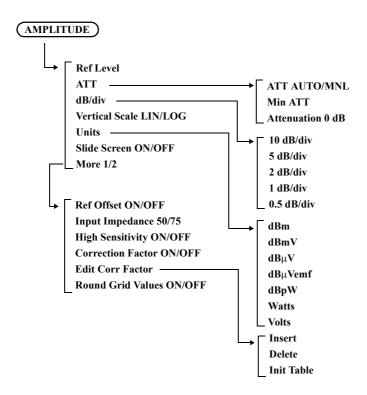

Ref Level Sets the reference level. ATT Displays the Attenuation menu. ATT AUTO/MNL Switches the attenuator function between auto and manual settings. AUTO: Automatically sets the attenuator value according to the reference level. Sets the attenuator value manually. MNL: Min ATT Sets the minimum value of the attenuator. This setting is enabled only when the attenuator is set manually. Attenuation 0 dB Sets the attenuator to 0 dB. Displays the confirmation window before setting. This setting can be set by selecting OK with step keys and press-

ing the unit key (ENTER).

5.2.15 AMPLITUDE

dB/div

10 dB/div Sets the LOG scale to 10 dB/div 5 dB/div Sets the LOG scale to 5 dB/div. Sets the LOG scale to 2 dB/div. 2 dB/div 1 dB/div Sets the LOG scale to 1 dB/div. 0.5 dB/div Sets the LOG scale to 0.5 dB/div.

Vertical Scale LIN/LOG

LIN: Displays waveform data on a linear scale. LOG: Displays waveform data on a log scale.

Units

dBm Sets the display unit to dBm. dBmV Sets the display unit to dBmV. $dB\mu V$ Sets the display unit to dBµV. **dB**µVemf Sets the display unit to dBµVemf. dBpW Sets the display unit to dBpW. Watts Sets the display unit to Watts. Volts Sets the display unit to Volts.

Slide Screen ON/OFF Scrolls the screen display up and down up to $\pm 100\%$.

> Enables the function. Enter the amount of the display ON:

scrolls by using the knob, step keys or keypad.

OFF: Cancels the slide function.

More 1/2 Displays the Level 2/2 menu.

Ref Offset ON/OFF Switches the reference level offset function ON and OFF.

> ON: The offset level can be set in the range of 0 to ± 100.0 dB. The relationship among the displayed reference level, set reference level, and offset is as follows:

Displayed reference level = Set reference level + Offset

OFF: Cancels the offset.

Input Impedance 50/75

50: Converts the power assuming that the input impedance is 50 Ω . This setting is the standard value that is 50.

75: Converts the power assuming that the input impedance is 75 Ω . The 6 dB conversion loss of the ZT-130NC 75/ 50 Ω impedance converter is added automatically.

NOTE: For OPT11 and OPT15 (75 Ω option), Input Impedance is fixed at 75 Ω This impedance cannot be changed to 50 Ω

5.2.15 AMPLITUDE

High Sensitivity ON/OFF Switches the high-sensitivity input function ON and OFF.

> Turns on the built-in preamp. The preamp gain is corrected at each frequency and it does not need to be ON:

considered in level measurements.

OFF: Turns off the built-in preamp.

Correction Factor ON/OFF

ON: Corrects the display level according to the correction

table.

OFF: Cancels the correction based on the correction data.

Edit Corr Factor Displays the Corr Factor menu and the correction table.

A frequency of up to 400 GHz and a level of ± 100 dB can be set.

Insert Inserts a line in the correction table.

Delete Deletes a line on which the cursor is positioned in the correction

table.

Init Table Clears all settings in the correction table.


Round Grid Values ON/OFF


ON: Displays the vertical scale by rounding off the Ref

Level setting value to integers.

OFF: Displays the vertical scale according to the Ref Level

setting value.

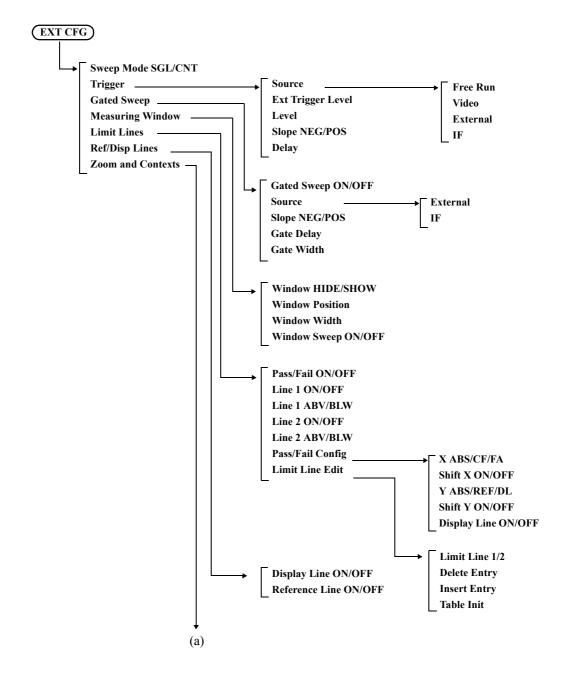

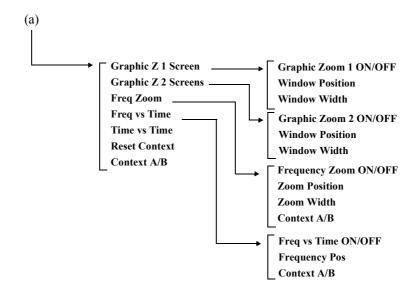

Sweep Mode SGL/CNT Sets the sweep mode.

SGL: Sets the SINGLE mode.

The sweep starts by pressing the START/STOP key

and stops.

CNT: Sets the CONTINUOUS mode.

Repeats the sweep automatically by the next trigger

signal after the sweep stops.

Trigger Displays the Trigger menu.

Source Displays the Trig Source menu.

Free Run Repeats the sweep automatically.

Video Synchronizes the sweep with the video signal and then starts the

sweep.

External Synchronizes the sweep with the external trigger signal (EXT ter-

minal) and then starts the sweep.

IF Synchronizes the sweep with the IF signal and then starts the

sweep.

Ext Trigger Level Sets the trigger signal for the external trigger signal.

Level Sets the trigger level for the Video or IF trigger.

Slope NEG/POS Switches the trigger slope polarity.

This setting is enabled only when the video trigger, external trig-

ger or IF trigger is used.

NEG: Starts the sweep at the falling edge of a trigger.

POS: Starts the sweep at the rising edge of a trigger.

Delay Sets the delay time from a trigger point.

Gated Sweep Displays the Gated Sweep menu.

Gated Sweep ON/OFF Switches the gated sweep ON and OFF.

ON: Sweep is executed according to the currently set gate

conditions (gate position and width).

OFF: Turns the gated sweep mode off.

Source Displays the Gate Source menu.

External: Performs sweep synchronizing with the external trigger

signal.

IF: Performs sweep synchronizing with the IF signal.

Slope NEG/POS Switches the trigger slope polarity.

NEG: The sweep starts at the falling edge of a trigger signal.


POS: The sweep starts at the rising edge of a trigger signal.

Gate Delay Sets the delay time from a trigger point.

Setting range: 0 sec to 1 sec

Gate Width Sets the gate time width.

Setting range: 50 µsec to 1 sec

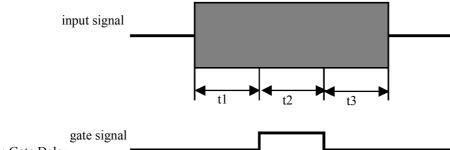

t1: Gate Delayt2: Gate Width

Measuring Window Displays the Window menu.

Window HIDE/SHOW

HIDE: Hides the measuring window.

SHOW: Displays the measuring window.

Window Position Sets the center position of the window.

Window Width Sets the window width.

Window Sweep ON/OFF

ON: Performs the sweep only in the range set in the

measuring window.

OFF: Performs the sweep in the range of the set span width.

Limit Lines Displays the Pass/Fail menu.

Pass/Fail ON/OFF Switches the Pass/Fail judgment due to the comparison with the

limit value ON and OFF.

ON: Performs the Pass/Fail judgment.

Performs the Judgment in each sweep.

If the limit line is not defined, this setting cannot be

used.

OFF: Does not perform the Pass/Fail judgment.

Line 1 ON/OFF Switches limit line 1 ON and OFF.

ON: Displays limit line 1.

OFF: Hides limit line 1.

Line 1 ABV/BLW Sets the judgment condition for limit line 1.

ABV: Sets the range above limit line 1 as the PASS condition.

BLW: Sets the range below limit line 1 as the PASS condition.

Line 2 ON/OFF Switches limit line 2 ON and OFF.

ON: Displays limit line 2.

OFF: Hides limit line 2.

Line 2 ABV/BLW Sets the judgment condition for limit line 2.

ABV: Sets the range above limit line 2 as the PASS condition.

BLW: Sets the range below limit line 2 as the PASS condition.

Pass/Fail Config Displays the PF Config menu.

X ABS/CF/FA Sets the attributes of the horizontal axis data of the limit line.

ABS: Sets the horizontal axis position according to the absolute value of the limit line set in Limit Line Edit.

The horizontal axis position of the limit line moves according to changes in the frequency span and center

frequency setting.

CF: Sets the reference position to the center of the

horizontal axis.

FA: Sets the reference position to the leftmost point on the

horizontal axis.

Shift X ON/OFF

ON: Sets the offset frequency from the reference position.

The limit line display is shifted by the frequency offset.

OFF: Cancels the shift of the limit line.

Y ABS/REF/DL Sets the attributes of the vertical axis (level) data of the limit line.

ABS: Sets the vertical axis position according to the absolute

value of the limit line set in Limit Line Edit.

The vertical axis position of the limit line moves

according to the change of the level setting.

REF: Sets the reference level as the reference position.

DL: Sets the display line as the reference position.

Shift Y ON/OFF

ON: Sets the offset (dB) of the vertical axis from the limit

line.

The limit line display is shifted by the level offset.

Display Line ON/OFF

ON: Displays the display line.

Sets the position of the display line.

OFF: Hides the display line.

Limit Line Edit Displays the Limit Line menu.

Limit Line 1/2

Edits limit line 1.
 Edits limit line 2.

Delete Entry Deletes a line on which the cursor is positioned in the limit line

table

Insert Entry Inserts a line in the limit line table.

Table Init Clears all settings in the limit line table.

Ref/Disp Lines Displays the Display menu.

Display Line ON/OFF Switches the display of the display line, which is used as the ref-

erence line when trace levels are compared, between ON and

OFF.

ON: Displays the display line.
OFF: Hides the display line.

Reference Line ON/OFF Switches the display of the reference line, which is used as the ref-

erence to display level data in relative value, between ON and

OFF.

ON: Displays the reference line.

The reference line position can be changed.

OFF: Hides the reference line.

Zoom and Contexts Displays the Zoom Contexts menu.

Graphic Z 1 Screen Displays the G Zoom 1 Screen menu.

Graphic Zoom 1 ON/OFF

ON: Zooms in the area selected by the window.

OFF: Cancels the zoom-in display.

Window Position Sets the center position of the window.

Window Width Sets the window width.

Graphic Z 2 Screens

Displays the G Zoom 2 Screen menu.

Graphic Zoom 2 ON/OFF

ON: Splits the screen into an upper and lower display.

The upper screen displays the original waveform. The lower screen zooms in on the area selected by the

window.

OFF: Cancels the zoom-in display.

Window Position Sets the center position of the window.

Window Width Sets the window width.

Freq Zoom Displays the Freq Zoom menu.

Frequency Zoom ON/OFF

ON: Splits the screen into an upper and lower display.

The upper screen displays the original waveform. The lower screen zooms in on the frequency range selected by the window, in which the sweep is

performed.

OFF: Cancels the dual-screen display.

Zoom Position Sets the center position of the window.

Zoom Width Sets the window width.

Context A/B Switches the active screen between A (upper screen) and B (lower

screen).

A: The upper screen settings can be changed.

B: The lower screen settings can be changed.

Freq vs Time Displays the Freq vs Time menu.

Freq vs Time ON/OFF

ON: Splits the screen into an upper and lower display.

The horizontal axis in the upper screen represents frequency, and the lower screen represents the time

(zero span) at the zoomed position.

OFF: Cancels the dual-screen display.

Frequency Pos Sets the frequency where the zero span is performed.

Context A/B Switches the active screen between A (upper screen) and B (lower

screen).

A: The upper screen settings can be changed.

B: The lower screen settings can be changed.

Time vs Time Sets the dual-screen display and displays the horizontal axis in

time for both the upper and lower screens.

The display of the horizontal axis in time is retained even if the

dual-screen has been canceled by using Reset Context. Re-set SPAN to display the horizontal axis in frequency.

Reset Context Context A/B

Cancels the dual-screen display.

Switches the active screen between A (upper screen) and B (lower screen).


A: The upper screen settings can be changed.

B: The lower screen settings can be changed.

5.2.17 CPL (Coupled function)

5.2.17 CPL (Coupled function)

Sets the resolution bandwidth (RBW), video bandwidth (VBW), and sweep time.

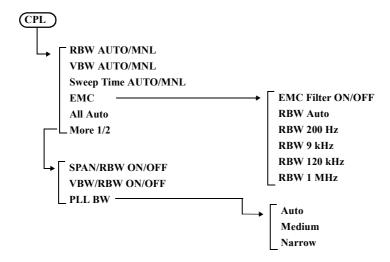

RBW AUTO/MNL Switches the RBW between auto and manual settings.

AUTO: Automatically sets the optimum RBW according to the

frequency span setting.

MNL: The RBW can be set arbitrarily.

VBW AUTO/MNL Switches the VBW between auto and manual settings.

AUTO: Automatically sets the optimum VBW according to the

RBW setting.

MNL: The VBW can be set arbitrarily.

Sweep Time AUTO/MNL Switches the sweep time between auto and manual settings.

AUTO: Automatically sets the optimum sweep time according

to the frequency span, RBW, and VBW settings.

MNL: The sweep time can be set arbitrarily.

EMC Displays the EMC menu. (OPT28)

EMC Filter ON/OFF ON: Uses the EMC filter.

OFF: Cancels the EMC filter mode.

RBW Auto Sets the resolution bandwidth automatically according to the mea-

surement frequency band.

RBW 200 Hz

Sets the resolution bandwidth to 200 Hz.

RBW 9 kHz

Sets the resolution bandwidth to 9 kHz.

RBW 120 kHz

Sets the resolution bandwidth to 120 kHz.

RBW 1 MHz

Sets the resolution bandwidth to 1 MHz.

5.2.17 CPL (Coupled function)

All Auto Automatically sets the optimum RBW, VBW, and sweep time

according to the frequency span setting.

More 1/2 Displays the Coupling 2/2 menu.

SPAN/RBW ON/OFF Switches the RBW vs frequency span function between the auto

and manual settings.

This setting is enabled only when the RBW is set to AUTO.

ON: The frequency vs RBW span ratio can be changed.

OFF: The frequency/RBW span value is fixed to 100.

VBW/RBW ON/OFF Switches the VBW vs RBW function between the auto and man-

ual settings.

This setting is enabled only when the VBW is set to AUTO.

ON: The VBW vs RBW ratio can be changed.

OFF: The VBW/RBW value is fixed to 1.

PLL BW Displays the PLL Band Width menu. (OPT 70)

Sets the band-pass filter width in the PLL circuit.

Auto Sets the filter width automatically so that the optimum phase

noise characteristics corresponding to the frequency span can be

obtained.

Medium Sets the filter width to Medium.

Narrow Sets the filter width to Narrow.

The phase noise around 300 kHz to 2 MHz away from the carrier

is improved.

CAUTION: When PLL Band Width is set to Medium or Narrow,

the phase noise may deteriorate depending on the set

frequency span.

In such a case, set to AUTO.

6. OVERVIEW OF REMOTE CONTROL

This chapter describes the overview of the remote control system.

6.1 Remote Control

6.1.1 Types of Systems

The following two types of remote control systems can be configured, depending on the interface:

Interface	Overview		
GPIB (Talker/Listener mode)	The external controller controls the U3700 Series and other devices, which are connected with each other through the GPIB, in this system. For more information, refer to "6.2 GPIB Remote Control System" (on page 6-2).		
LAN	The external controller controls the U3700 Series and other devices, which are connected with each other through LAN, in this system. For more information, refer to "6.3 LAN Remote Control System" (on page 6-6).		

6.1.2 Selecting the Command Set

Either the AT (Advantest) command set or SCPI command set is selected as a command set used for programming in this instrument.

Both command sets cannot be used together.

Press SYSTEM, Remote Control, and Parser AT/SCPI.

6.2 GPIB Remote Control System

6.2 GPIB Remote Control System

The GPIB (General Purpose Interface Bus) that is compliant with IEEE standards 488.1-1978 and 488.2-1987 comes standard with this instrument so that remote control can be performed from the external controller.

The following describes how to control this instrument by using the GPIB remote control function.

6.2.1 What is the GPIB?

The GPIB (General Purpose Interface Bus) is a high performance bus that integrates computers and measuring instruments.

The GPIB operations are defined by IEEE standard 488.1-1978. Since the GPIB is a bus structure interface, the specific device can be identified by assigning a unique device address to each device. Up to 15 devices can be connected to a bus in parallel. A GPIB device includes at least one of the following functions:

Talker

A device that is specified to send data to the bus is called a "talker". Only one device operates as an active talker on a GPIB bus.

Listener

A device that is specified to receive data from the bus is called a "listener". Two or more active listener devices exist on a GPIB bus.

Controller

A device that specifies talkers and listeners is called a "controller". On a GPIB bus, only one device operates as an active controller. Of these controllers, a device that can control IFC and REN messages is called the "system controller".

Only one system controller is permitted on a GPIB bus. If there are two or more controllers on a bus, the system controller becomes the active controller at the time of system startup and the other devices with controller capability act as addressable devices.

To set another controller as the active controller, use Take Control (TCT) interface messages. At this time, this controller becomes a non-active controller.

The controller controls the entire system by sending interface or device messages to each measuring instrument. The roles of these messages are shown below.

- Interface message: Controls the GPIB bus.
- Device message: Controls the measuring instruments.

6.2.2 Setting up the GPIB

1. GPIB connection

The standard GPIB connection is shown below. Secure the GPIB connector with two screws.

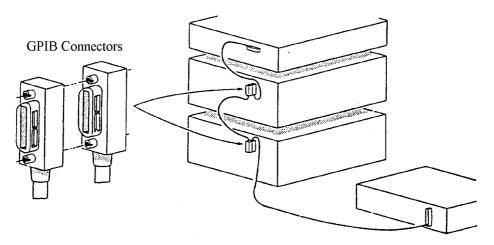


Figure 6-1 GPIB Connection

Note the following when using the GPIB interface:

- Connect the GPIB cable to the GP-IB 1 connector on the rear panel of this instrument.
- The total cable length of the GPIB cable used in one bus system should not be longer than 2 m × {the number of connected devices (the GPIB controller is counted as one device)}. The total cable length should be 20 m or less.
- Up to 15 devices can be connected to one bus system.
- There is no restriction in how cables are connected. However, no more than three GPIB connectors should be stacked on one device. If four or more GPIB connectors are stacked, the joints of the connectors may break because excessive force is applied to them.

For example, a system consisting of five devices can use cables of up to 10 m (2 m/device \times 5 devices = 10 m) length. Cable lengths can be allocated freely unless the total cable length exceeds the permitted maximum length. If 10 or more devices are connected, however, some devices should be connected with cables less than 2 m so that the total cable length does not exceed 20 m.

- Ensure that all devices on the bus are turned on. If any device on the bus is not turned on, the system may not operate correctly.
- Turn off all devices on the bus before connecting or disconnecting GPIB cables.

2. GPIB address setting

GPIB addresses should be set by pressing the **System** key and selecting *GPIB Address*.

6.2.3 GPIB Bus Functions

6.2.3 GPIB Bus Functions

6.2.3.1 GPIB Interface Functions

Table 6-1 GPIB Interface Functions

Code	Description
SH1	Source handshake function
AH1	Accepter handshake function
Т6	Basic talker function, serial polling function, listener-specified talker cancel function
TE0	No extended talker function
L4	Basic listener function, talker-specified listener cancel function
LE0	No extended listener function
SR1	Service request function
RL1	Remote function, local function, local lockout function
PP0	No parallel polling function
DC1	Device clear function
DT1	Device trigger function
DT0	No device trigger function
C0	No system controller function
E1	Using the open-collector bus driver

6.2.3.2 Responses to Interface Messages

The responses of this instrument to interface messages described in this section are defined in IEEE standards 488.1-1978 and 488.2-1987.

For more information on how to send interface messages to this instrument, refer to the operation manual of the controller used.

1. Interface clear (IFC)

This message is directly sent to this instrument through a signal line.

This instrument stops the operation of the GPIB bus by using this message. Though all input/output is stopped, the I/O buffer is not cleared (it is cleared by DCL).

2. Remote enable (REN)

This message is directly sent to this instrument through a signal line.

If this instrument is specified as a listener when this message is TRUE, it enters the remote state.

This instrument remains in this state until it receives a GTL command, REN changes to FALSE, or the LOCAL key is pressed.

This instrument ignores all received data when it is in the local state.

When it is in the remote state, this instrument ignores all key entry except the LOCAL key.

When it is in the local lockout state (referred to as "Local lockout (LLO)"), this instrument ignores all key entry.

3. Serial poll enable (SPE)

When receiving this message from a controller, this instrument enters the serial polling mode.

When this instrument specified as a talker in this mode, it sends status bytes instead of ordinary messages. This mode continues until this instrument receives a serial polling disable (SPD) message or an IFC message.

When this instrument is sending a service request (SRQ) message to the controller, bit6 (RQS bit) of response data is set to 1 (TRUE). After transmission is completed, RQS bit is set to 0 (FALSE). Service request (SRQ) messages are directly sent through a signal line.

4. Device clear (DCL)

When receiving DCL, this instrument performs the following operations:

- Clearing the input and output buffers
- Resetting the syntax analysis, execution control, and response data generation units
- Canceling all the commands that impede the remote command to be executed next
- Canceling any commands that are waiting for other parameters

The following operations are not executed:

- Changing data that is set or stored in this instrument
- Interrupting front panel operations
- Affecting or interrupting the operations of this instrument in mid-execution
- Changing status byte excluding MAV (MAV is set to 0 as a result of clearing the output buffer)

5. Selected device clear (SDC)

Performs the same operation as DCL. However, SDC is executed only when this instrument is a listener.

In other cases, it is ignored.

6. Go to local (GTL)

This message sets this instrument to the local state. In the local state, all front panel operations are enabled.

7. Local lockout (LLO)

This message sets this instrument to the local lockout state. When this instrument enters the remote state from this state, all front panel operations are disabled (In the ordinary remote state, front panel operation can be performed by pressing the LOCAL key).

In this case, this instrument can be set to the local state by any of the following two methods:

- Setting the REN message to FALSE (The local lockout state is also canceled)
- Turning off and turning on the power

6.3 LAN Remote Control System

6.3 LAN Remote Control System

The LAN (Local Area Network) interface that is compliant with IEEE standard 802.3 is included as standard with this instrument so that this instrument can be controlled remotely through socket communication by the external controller.

The controlling method using the LAN remote control function is described below.

6.3.1 Setting up the LAN

1. LAN connection

The standard LAN setup is shown below. To allow communication through the LAN between an external controller and this instrument or other devices, connect them with 10BASE-T LAN cable and RJ45 connectors. To directly connect this instrument and an external controller with a LAN cable, use a LAN cable (cross over cable) and connect as shown in Table 6-2. To connect this instrument and other devices (excluding an external controller) with a LAN, use an external device designed to connect devices that has two or more LAN interfaces such as an Ethernet hub. The LAN cable used in this case is connected as shown in Table 6-3.

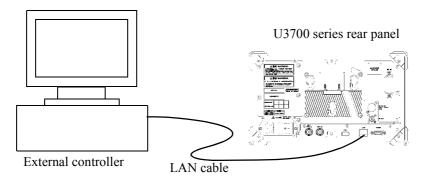


Figure 6-2 LAN Setup

Conne	ctor A	Connector B	
Signal name	RJ45 Pin number	RJ45 Pin number	Signal name
RX+	1	3	TX+
RX-	2	6	TX-
TX+	3	1	RX+
TX-	6	2	RX-
Not Used	4	4	Not Used
	5	5	
	6	6	
	7	7	
	8	8	

Table 6-2 Connection of 10BASE-T Cross-over Cables

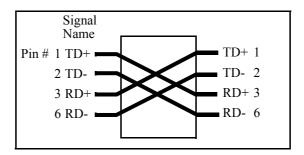


Figure 6-3 Connection of Cross-over Cables

1able 6-3	Connection of	TOBASE-T	Straight Car	nes

Signal name	RJ45 Pin number	Line color	Pair number
RX+	1	White/Orange	2
RX-	2	Orange	2
TX+	3	White/Green	3
TX-	6	Green	3
Not Used	4	Blue	1
	5	White/Blue	1
	7	White/Brown	4
	8	Brown	4


6.3.2 Setting the IP Address

6.3.2 Setting the IP Address

Press SYSTEM, Remote Control, and LAN IP Address.


Setting the IP Address Manually
 Enter a check mark into the "Use the following IP address" check box.

IP Address
Subnet Mask
Default Gateway
Set the above items.

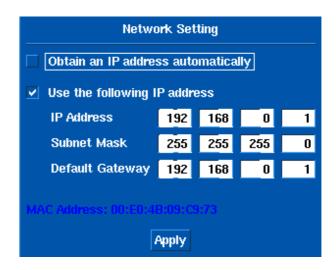

Click the *Apply* button and press Hz.


2. Obtaining the IP Address Automatically
Enter a check mark into the "Obtain an IP address automatically" check box.

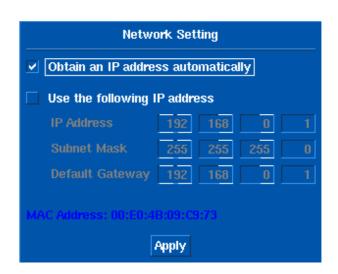

Click the *Apply* button and press Hz.

6.3.3 Control from a Controller

After an IP address is obtained, the IP address is displayed in the window.

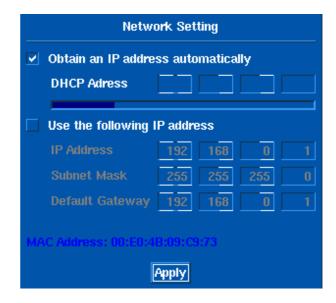

6.3.3 Control from a Controller

To control this instrument from an external controller, a port number for socket communication is required. The port number "5025" is assigned for socket communication in the remote state in this instrument. To write a program for socket communication, a library for network connection with the TCP/IP protocol is required. The library differs depending on the environment, such as the OS of the external controller. In the Windows OS environment, for example, WinSock is provided.

After completing the network connection with this instrument, send the "REN" command to this instrument to enable the remote control.

(At this time, the remote lamp on the front panel of this instrument is on.)

After that, this instrument can be remotely controlled by sending the same commands as the GPIB.

Some of the functions available in the GPIB remote control system are specific to the GPIB bus, such as service requests, and cannot be used in the LAN remote control system.

6.4 Message Exchanging Protocol

6.4 Message Exchanging Protocol

This instrument receives program messages from the controller or other devices through the GPIB bus or LAN and generates a response. Program messages include commands, queries (which are commands that ask for a response) and data.

6.4.1 Buffers

This instrument has two buffers.

1. Input buffer

This buffer temporarily stores data to analyze commands.

(1024-byte length)

The input buffer can be cleared by the following two methods:

- Turning the power on
- Executing a DCL or SDC
- 2. Output buffer

This buffer stores data until the data is read by the controller.

(1024-byte length)

The output buffer can be cleared by the following two methods:

- Turning the power on
- Executing a DCL or SDC

6.4.2 Message Exchange

When other controllers or devices receive messages from this instrument, the following items must be observed:

- Generating a response in reply to a query (Refer to "Parser").
- Generating responses in the order queries are executed (Refer to "Generating response data").

Parser

The parser receives command messages from the input buffer in the order queries are received, executes syntax analysis, and determines what operations are to be executed by the commands received.

Generating response data


• When the parser executes a query, this instrument generates data on the output buffer as its response (that is, a query must be sent immediately before outputting data).

6.5 Command Syntax

This chapter describes the command syntax.

6.5.1 Command Syntax

The command syntax is defined in the following format:



1. Header

Two types of header are available: the common command header and the simple header. The common command header starts with an asterisk (*). The simple header is a functionally independent command that has no hierarchical structure.

If a question mark (?) is attached immediately after a header, it becomes a query command.

2. Spaces

Spaces may be used to separate headers from data to ease readability.

3. Data

When the command requires more than one data item, list these data items by delimiting them with commas (,). A space may be inserted before or after the comma (,). For more information on data types, refer to Section 6.5.2 "Data Formats."

4. Writing more than one command

You can write multiple commands by delimiting them with semicolons (;) in one line.

6.5.2 Data Formats


6.5.2 Data Formats

This instrument uses the following data formats for the input and output data.


1. Numeric data

There are three formats for numeric data as shown below. When entering numeric values for this instrument, any format may be used. Depending on the command, a unit may be attached to the entered numeric value.


• Integer type: NR1 format



• Fixed-point type: NR2 format



• Floating-point type: NR3 format



2. Unit

Available units are listed below:


Unit	Exponential	Description
GZ	10 ⁹	Frequency
MZ	10 ⁶	Frequency
KZ	10^{3}	Frequency
HZ	100	Frequency
VOLT	100	Voltage
MV	10-3	Voltage
UV	10 ⁻⁶	Voltage
NV	10-9	Voltage
MW	10-3	Power
DB	10 ⁰	dB description
MA	10-3	Current
SC	100	Second
MS	10-3	Second
US	10 ⁻⁶	Second
PER	100	Percentage
%	10 ⁰	Percentage

6.5.3 Status Byte

This instrument has a layered status register structure that is compliant with IEEE standard 488.2-1987, and can send various statuses of this instrument to the controller. This section describes the behavioral model of status bytes and allocation of events.

1. Status Register

This instrument adopts the model of the status registers defined in IEEE standard 488.2-1987. The status registers consist of the condition register, event register, and enable register.

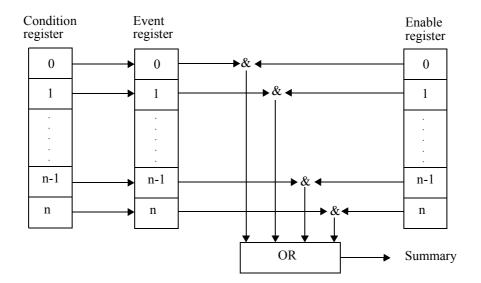

a. Condition Register

The condition register is always monitoring the status of this instrument. That is, this register always retains the latest status of this instrument. However, data cannot be both written into and read from the condition register because the condition register retains data as internal information.

b. Event Register

The event register latches and retains statuses from the condition register (or retains changes). Once this register is set, the setting value is kept until it is read by a query or cleared by *CLS. Data cannot be written into the event register.

c. Enable Register

The enable register specifies which bit in the event register is set as an effective status to generate a summary. The enable register is ANDed with the event register and the OR of the result is generated as a summary. The summary is written into the status byte register.

Data can be written into the enable register.

This instrument uses the following three types of status registers:

- Status byte register
- Standard event register
- Standard operation status register

The arrangement of the status register in this instrument is shown in Figure 6-4.

The details of the status register are shown in Figure 6-5.

6.5.3 Status Byte

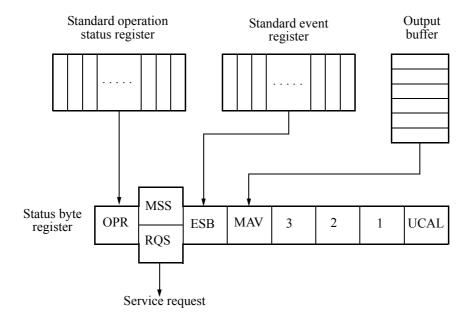


Figure 6-4 Status Register Arrangement

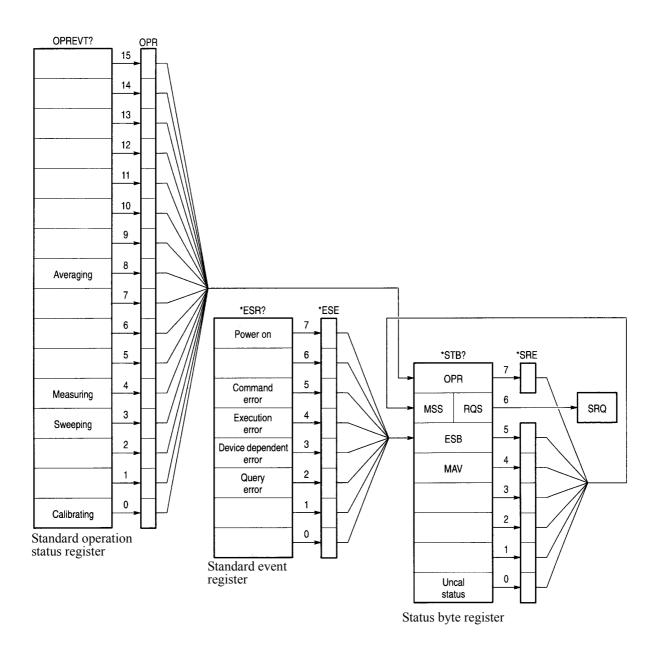


Figure 6-5 Details of Status Register

2. Event Enable Register

Each event register has an enable register to determine which bit is available. The enable register sets the corresponding bit in decimal value.

- Service request enable register setting: *SRE
- Standard event status enable register setting: *ESE
- Operation status enable register setting: OPR

6.5.3 Status Byte

3. Standard Operation Status Register

Assignment in the standard operation status register is listed below:

Bit	Functional definition	Description
15 to 9		Always 0
8	Averaging	Set to 1 when averaging is complete.
7 to 5		Always 0
4	Measuring	Set to 1 when sequence measuring is complete.
3	Sweeping	Set to 1 when sweeping is complete
2 to 1		Always 0
0	Calibrating	Set to 1 when correction data acquisition is completed.

4. Status Byte Register

The status byte register summarizes the information from the status register. A summary of this status byte register is sent to the controller as a service request. Therefore, the status byte register operates slightly differently than the status register structure. This section describes the status byte register.

The structure of the status byte register is shown in Figure 6-6.

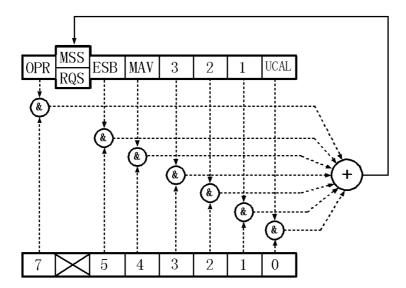


Figure 6-6 Structure of the Status Byte Register

This status byte register follows the status register except for the following three points:

- The summary of the status byte register is written to bit6 of the status byte register.
- Bit6 of the enable register is always valid and cannot be changed.
- Bit6 (MSS) of the status byte register writes the RQS of the service request.

This register responds to the serial polling from the controller. When the register responds to the serial polling, bit0 to bit5, bit7, and the RQS of the status byte register are read, and then the RQS is reset to 0. No other bits are cleared until each factor is set to 0.

The status byte register, RQS, and MSS can be cleared by executing "CLS" and "S2". Consequently, the SRQ line is set to FALSE.

The meaning of each bit in the status byte register is shown below:

Bit	Functional definition	Description
7	OPR	A summary of the standard operation status register.
6	MSS	The summary bit of the entire status data structure. RQS is set to TRUE when MSS is set to 1 in the status byte register. MSS cannot be read during serial polling but it is 1 when RQS is 1. To read the MSS, use the common command *STB?. MSS, bit0 to bit5, and bit7 of the status byte register are read by *STB?. In this case, the status byte register and MSS are not cleared. MSS is not set to 0 until all the unmasked factors in the status register structure are cleared.
5	ESB	A summary of the standard event register.
4	MAV	The summary bit of the output buffer. Not uses in this instrument.
3 to 1		Always 0
0	UCAL	Set to 1 if a signal level error occurs because the sweep is too fast.

6.5.3 Status Byte

5. Standard Event Register

Assignments in the standard event register are listed below:

Bit	Functional definition	Description
7	Power on	Set to 1 when the power is turned on.
6		Always 0
5	Command Error	Set to 1 if the parser detects a syntax error.
4	Execution Error	Set to 1 if an instruction that was received as a GPIB command fails to execute for some reason (e.g., the parameter is out of range).
3	Device Dependent Error	Set to 1 if any errors except for Command Error, Execution Error, and Query Error occur.
2	Query Error	Set to 1 if no data exists or if data is lost when the controller tries to read data from this instrument.
1	Request Control	Not uses in this instrument.
0	Operation Complete	Not uses in this instrument.

6.6 GPIB Remote Programming

This section shows the AT commands in each function:

- Command code
 - An asterisk "*" indicates a function that numeric or character strings data follows after the code. Numeric data and "ON" can be omitted from [].
- Output format
 - A comma "," indicates that two or more data are output.
 - ON or OFF indicates that 1 or 0 is output.
 - Frequency is output in Hz and time is output in sec.
 - Level data is output in the currently set display unit.

AT Command	Pages	AT Command	Pages
<n>AVG* <n>GR</n></n>	6-31	ABC	6-31
<n>AVG* <n>GS</n></n>	6-31	ACP	6-44
<n>B</n>		ACPCBW	6-44
<n>G</n>	6-30	ACPLOAD	6-44
<n>GC</n>	6-31	ACPNQST	6-44
<n>GCNT</n>	6-31	ACPREF	6-44
<n>GP</n>	6-31	ACPSAVE	6-44
<n>GSGL</n>	6-31	ACPSCR	6-44
<n>MAX</n>	6-30	ACPTM	6-44
<n>MIN</n>	6-30	ADG	6-44
<n>NORM</n>	6-53	ADLA	6-31
<n>PAVG</n>	6-31	AL	6-28
<n>PGC</n>	6-31	AMMF	6-41
<n>PGCNT</n>	6-31	AMMOD	6-41
<n>PGP</n>	6-31	ANNOT	6-51
<n>PGSGL</n>	6-31	AR	6-53
<n>V</n>	6-30	AS	6-29
<n>W</n>	6-30	AT	6-27
% PER	6-54	ATMIN	6-27
*CLS	6-51	AUNITS	6-27
*ESE	6-51	BA	6-28
*ESR	6-51	BAA	6-31
*IDN	6-52	BAB	6-31
*OPT	6-52	BAC	6-31
*SRE	6-51	BDLB	6-31
*STB	6-51	BMP	6-50
*TST	6-52	CA	6-25
AA	6-27	CALCA	6-30
ABA	6-31	CALCB	
ABB	6-31	CALCC	6-30

CARNID	(52	DDM	(5 1
CAPPOS		DBM	
CARRBS	-	DBMV	
CC		DBPW	
CDB		DBUV	
CF		DC0	
CFCH		DC1	
CFCHON		DC2	
CHCALC1		DD	
CHCALC2		DEL	
CHCALC3		DET	
CHCON1		DETA <n></n>	
CHCON2		DETAVG	
CHCON3		DETB	
CHTDEL	6-26	DETC	6-32
CHTIN	6-26	DLIM0	6-51
CLALL	6-47	DLIM1	6-51
CLATT	6-48	DLIM2	6-51
CLCREF	6-48	DLIM5	6-51
CLDREF	6-48	DLN	6-34
CLFREF	6-48	DLN OFF	6-34
CLGAIN	6-47	DLN ON	6-34
CLPBW	6-47	DS MTSP	6-37
CLRBW	6-47	DUALCH	6-35
CLSREF	6-48	DUALCHINIT	6-35
CN	6-42	DY	6-38
CN0		E	
CN1		EMCON EMCDET	
CN2		FA	
CN3		FACH	
CNPOS		FACHO	
CNPOSA		FACHON	
CNRES		FACHOON	
CORS		FB	
CORS OFF		FBCH	
CORS ON		FBCHO	
COUNT		FBCHON	
COVR		FBCHOON	
COVR OFF	-	FC	
COVR ON		FILEFORMAT	
CP		FILEMEDIA	
CR CR CFF		FINPMD	
CR OFF		FMMEAS	
CR ON		FMMODF	
CRDEL		FMMODFY	
CRIN		FO	
CS		FOON OFF	
CSBSDEL		FORM1	
CSBSIN		FORM2	
CTXTSEL		FORM3	
DB		FORM4	
DBEMF	6-54	FS	6-25

FTPOS	6-34	LMTAINF	6-33
FX	6-36	LMTAINT	6-33
GDATA	6-50	LMTB	6-33
GIMAG	6-50	LMTBDELF	6-34
GTL	6-51	LMTBDELT	6-34
GTPOS	6-29	LMTBINF	6-33
GTSLP	6-29	LMTBINT	6-34
GTSRC	6-29	LOF	6-50
GTSWP	6-29	LON	6-50
GTWID	6-29	LTSP LS	6-25
GZ	6-54	M0 MKCS	6-37
HARM	6-40	M1 MTCS	6-37
HARMNUM	6-40	M2 MKMKS	6-37
HCDEV	6-50	M3 MTMKS	
HCOPY	6-50	MC MKCF	
HRMFND	6-40	MDF2	
HRMFND OFF	6-40	MDL2	6-36
HRMFND ON	6-40	MF <n></n>	6-35
HS	6-27	MFL	6-35
HZ	6-54	MFL <n></n>	6-35
ID		MFLC	
IMGSP		MFLC <n></n>	
IMLOAD		MFR	
IMLS3		MIS	
IMLS5		MK	
IMLS7		MKBW	
IMLS9		MKD	
IMM		MKLST	
IMMDF		MKMODE	
IMMREF		MKROBJ	
IMMRES		MKROJB	
IMODR		MKRSEL	
IMPFC		MKSPOS	
IMSAVE		MKSWID	
INSTR		MKSX	
IP *RST		MKSYDL	
KZ		MKSYLA	
LARNG		MKSYLB	
LBRNG		MKTRACE	
LIMAPOS		ML	
LIMAS		ML <n></n>	
LIMASFT		MLN	
LIMPOS		MLN <n></n>	
LIMS		MLR	
LIMSF		MLSFL	
LIMST		MLTOFF	
LL1		MLTSCR	
LLO		MMS	
LMTA		MNRF	
LMTADELF		MO MKOFF	
LMTADELT	6-33	·	6-36
1/171 1 / 31/1 / 1 / 1	V .1.1	1711 / 3	(,-,,()

MPM	6-36	PMEASAVG	
MR MKRL	6-37	PMEASAVGONCE	6-43
MS MSEC	6-54	PMEASMODE	6-43
MTCF	6-37	PMEASOFF	6-43
MV	6-54	PMEASTM	6-43
MW	6-54	PMEASTRACE	6-43
MZ	6-54	PNG	6-50
NI	6-39	PPM	6-54
NIC	6-39	PS	6-38
NIF		PSXDB	
NIM		PU	
NION		PWAVG	
NIRES		PWAVGLOAD	
NIU		PWAVGON	
NORM		PWAVGRANGE	
NSEC		PWAVGSAVE	
NV		PWAVGTM	
NXL		PWCH	
NXM		PWCHLOAD	
NXP		PWCHON	
NXR		PWCHPSD	
OBW		PWCHSAVE	
OBWLOAD		PWCHTM	
OBWON		PWTOTAL	
OBWPER		PWTOTALON	
OBWSAVE		PWTOTALPSD	
OBWTM	6-44	PWTOTALTM	
OHM	6-27	PWTOTLOAD	6-43
OPR	6-51	PWTOTSAVE	6-43
OPREVT	6-51	QP0	6-47
OPT10	6-52	QP1	6-47
OPT11	6-52	QP2	6-47
OPT15	6-52	QP3	6-47
OPT20		QPAUTO QA	6-47
OPT28		RB	
OPT50		RC	
OPT53		REDLT	
OPT54		REN	
OPT74	6-52	RENAME	6-48
OPT75		RF	
OPT76		RFACT	
OPT77		RFC	
PARSER		RFE	
PFC		RFI	
PFJ? OPF?		RFX	
PKCF		RL	
PKRL		RLN	
PKZOOM		RLN OFF	
PLLBW		RLN ON	
PLS FREQ		RO	
PLS LEVEL	6-38	RO ON OFF	6-27

RPWD	6-52	SVSPR1	6-49
RX	6-53	SVSPR2	6-49
S0		SVSPR3	
S1		SVTRC1A	
S2		SVTRC1B	
SAM		SVTRC1C	
SC		SVTRC2A	
SCRF		SVTRC2B	
SDV		SW ST	
SEM		SWM	
SEMCBW		SWPCNT	
SEMLOAD		SYMRT	
SEMNQST		SYNCTO	
SEMON		T <n></n>	
SEMRFCALC		TAA	
SEMRFPOW		TAB	
SEMSAVE		TAC	
SEMTDEL		TBA	
SEMTIN		TBB	
SEMTM		TBC	
SETDATE		TG	
SETTIME		TGDLTRLN	
SFM		TGF	
SG		TGL	
SGY		TGLO	
SGY OFF		TGLO ON OFF	
SGY ON		TGO	
SI SNGLS		TGO ON OFF	
SIGID		TN	
SN CONTS		TPL TP	
SOF		TPS TP	
SON		TRACESEL	
SP		TRGDLY	
SPRFDEL		TRGLVL	6-29
SPRIN SPRFIN		TRGSLP	
SPRTBL		TRGSRC	
SPURI		TRGTTLLVL	
SR		TRSUB	
STORE		TS	
SUPIP		US USEC	
SV		UV	
SVACP	6-49	V VOLT	6-54
SVANT		VA	
SVCH		VB	6-28
SVLIM1		VS	
SVLIM2		VSWR	
SVNRM1A		VSWRLOSS	
SVNRM1B		VSWRON	
SVNRM1C		W WATT	
SVSEM		WDOSWP	
SVSET	6-48		6-34

U3700 Series User's Guide

WLX	6-34
WP	6-48
XDB	6-39
XDL	6-39
XDR	6-39
ZAT	6-27
ZMPOS	6-34
ZMWID	6-34
7 S	6-25

6.8 AT Command List

6.8.1 Frequency

Function	Comm	nand (EXE, SET)	Que	ery (GET)
Function	Code	Argument Format	Code	Output Format
Center Frequency	CF*	Frequency	CF?	Frequency
CF Step Size	CS*	Frequency	CS?	Frequency
CF Step Auto	CA [*]	[ON] OFF	CA?	0 = OFF (manual) 1 = ON (auto)
Frequency Offset	FO [ON,]* FO ON OFF	Frequency	FO? FOON?	Frequency 0 = OFF 1 = ON
Start Frequency	FA*	Frequency	FA?	Frequency
Stop Frequency	FB*	Frequency	FB?	Frequency
Frequency Span	SP*	Frequency	SP?	Frequency
Full Span	FS			
Zero Span	ZS			
Last Span	LTSP LS			
Frequency Setting Mode	FINPMD*	CALC TBL	FINPMD?	0 = CALC 1 = TBL
Set Start Channel Offset	FACHO*	Frequency	FACHO?	Frequency
Set Stop Channel Offset	FBCHO*	Frequency	FBCHO?	Frequency
Start Channel Offset	FACHOON*	ON OFF	FACHOON?	0 = OFF 1 = ON
Stop Channel Offset	FBCHOON*	ON OFF	FBCHOON?	0 = OFF 1 = ON
Set Center Channel Set- ting	CFCH*	Integer	CFCH?	Integer (Channel Number)
Set Start Channel Setting	FACH*	Integer	FACH?	Integer (Channel Number)
Set Stop Channel Setting	FBCH*	Integer	FBCH?	Integer (Channel Number)
Center Channel Setting	CFCHON*	ON OFF	CFCHON?	0 = OFF 1 = ON
Start Channel Setting	FACHON*	ON OFF	FACHON?	0 = OFF 1 = ON

6.8.1 Frequency

Function	Command (EXE, SET)		Query (GET)	
Tunction	Code	Argument Format	Code	Output Format
Stop Channel Setting	FBCHON*	ON OFF	FBCHON?	0 = OFF 1 = ON
Channel Type 1 Input3 Formulas :	CHCALC1 *,*,*,*,* CHCALC2 *,*,*,* CHCALC3 *,*,*,*	Integer, Integer, Frequency, Frequency, Integer		
Formula 1 for Type 1	CHCON1*	ON OFF	CHCON1?	0 = OFF 1 = ON
Formula 2 for Type 1	CHCON2*	ON OFF	CHCON2?	0 = OFF 1 = ON
Formula 3 for Type 1	CHCON3*	ON OFF	CHCON3?	0 = OFF 1 = ON
Channel Type 2 Input	CHTIN*,*	Integer, Frequency		
Channel Type 2 Deletion	CHTDEL			
Signal Ident	SIGID*	ON OFF	SIGID?	0 = OFF 1 = ON
Image Suppress	IMGSP*	ON OFF	IMGSP?	0 = OFF 1 = ON
Auto Tune	TN			
Peak Zoom	PKZOOM			

6.8.2 Level

Function	Comman	d (EXE, SET)	Quer	y (GET)
Tunction	Code	Argument Format	Code	Output Format
Reference Level	RL*	Level	RL?	Level
Attenuation	AT*	DB (Integer)	AT?	DB (Integer)
Min Attenuation	ATMIN*	DB (Integer)	ATMIN?	DB (Integer)
Zero Attenuation	ZAT			
Attenuation Auto	AA[*]	[ON] OFF	AA?	0 = OFF (manual) 1 = ON (auto)
XdB/Div	DD*	DB (Discr. Val.: 10, 5, 2, 1, 0.5 dB)	DD? DDB?	0 = 10 dB 1 = 5 dB 2 = 2 dB 3 = 1 dB 4 = 0.5 dB -1 = others
Linear × 1	LL1			
Vertical Scale	VS*	LIN LOG	VS?	0 = LOG 1 = LIN
Level Offset	RO*	DB	RO?	DB
	RO ON OFF		ROON?	0 = OFF 1 = ON
Hi Sens	HS[*]	[ON] OFF	HS?	0 = OFF 1 = ON
Input	OHM*	Integer (Discr. Val.: 50, 75)	OHM?	Integer
Display Unit (Level Unit)	AUNITS*	DBM DBMV DBUV DBEMF DBPW W[ATT] V[OLT]	AUNITS?	0 = DBM 1 = DBMV 2 = DBUV 3 = DBEMF 4 = DBPW 5 = WATT 6 = VOLT
Correction Factor ON OFF	CR ON CR OFF		CRON?	0 = OFF 1 = ON
Table Input	CRIN*,*	Frequency, Level (DB)		
Table Delete	CRDEL			

6.8.3 Bandwidth

6.8.3 Bandwidth

Function	Comm	Command (EXE, SET)		ery (GET)
runction	Code	Argument Format	Code	Output Format
RBW	RB*	Frequency	RB?	Frequency
RBW Auto	BA[*]	[ON] OFF	BA?	0 = OFF 1 = ON
VBW	VB*	Frequency	VB?	Frequency
VBW Auto	VA[*]	[ON] OFF	VA?	0 = OFF (manual) 1 = ON (auto)
Couple All Auto	AL[*]	[ON] OFF	AL?	0 = OFF 1 = ON (all auto)
RBW : Span	CORS*	Ratio (float)	CORS?	Ratio (float)
	CORS ON[*] CORS OFF		CORSON?	0 = OFF 1 = ON
VBW : RBW	COVR*	Ratio (float)	COVR?	Ratio (float)
	COVR ON[*] COVR OFF		COVRON?	0 = OFF 1 = ON
PLL Band Width	PLLBW*	AUTO MID NARW	PLLBW*	0 = Auto 1 = Narrow 2 = Medium

6.8.4 Sweep

Function	Comm	Command (EXE, SET)		Query (GET)	
runction	Code	Argument Format	Code	Output Format	
Sweep Time	SW ST*	Time	SW? ST?	Time	
Sweep Auto	AS[*]	[ON] OFF	AS?	0 = OFF (manual) 1 = ON (auto)	
Sweep Mode			SWM?	0 = Single 1 = Normal	
Sweep Mode Normal	SN CONTS				
Sweep Mode Single	SI SNGLS				
Take Sweep	TS				
Sweep Start / Stop	SR				
Gated Sweep Mode	GTSWP*	ON OFF	GTSWP?	0 = OFF 1 = ON	
Gate Source	GTSRC*	EXT IF	GTSRC?	2 = EXT 3 = IF	
Gate Slope	GTSLP*	(FALL NEG -) (RISE POS +)	GTSLP?	0= RISE POS + 1= FALL NEG -	
Gate Delay	GTPOS	Time	GTPOS?	Time	
Gate Width	GTWID*	Time	GTWID?	Time	

6.8.5 Trigger

Function	Command (EXE, SET)		Query (GET)	
1 unction	Code	Argument Format	Code	Output Format
Trigger Mode	TRGSRC*	FREE IF EXT VIDEO	TRGSRC?	0 = FREE 1 = TRG_VIDEO 2 = TRG_EXT 3 = TRG_IF
Video or IF Trigger Level	TRGLVL*	Level	TRGLVL?	Level
External Trigger Level	TRGTTLLVL*	Voltage	TRGTTLLVL?	Voltage
Trigger Slope	TRGSLP*	(FALL NEG -) (RISE POS +)	TRGSLP?	0 = RISE POS +1 = FALL NEG -
Trigger Delay	TRGDLY*	Time	TRGDLY?	Time

6.8.6 Trace

6.8.6 Trace

NOTE: Three Traces are available A, B and C. In the Command List below, just replace <n> by the letter for the selected trace ie <n> = $A \mid B \mid C$

Function	Comm	Command (EXE, SET)		Query (GET)	
runcuon	Code	Argument Format	Code	Output Format	
Trace Mode			T <n>?</n>	0 = WRITE 1 = VIEW 2 = BLANK	
Write	<n>W</n>				
View	<n>V</n>				
Blank	<n>B</n>				
Calc Mode Trace A	CALCA*	WRITE MIN MAX AVG PAVG MAXCONT	CALCA?	0 = WRITE 1 = MIN HOLD 2 = MAX HOLD 3 = AVERAGE 4 = POWER AVG 5 = MAX HOLD CONT	
Calc Mode Trace B	CALCB*	WRITE MIN MAX AVG PAVG MAXCONT	CALCB?	0 = WRITE 1 = MIN HOLD 2 = MAX HOLD 3 = AVERAGE 4 = POWER AVG 5 = MAX HOLD CONT	
Calc Mode Trace C	CALCC*	WRITE MIN MAX AVG PAVG MAXCONT	CALCC?	0 = WRITE 1 = MIN HOLD 2 = MAX HOLD 3 = AVERAGE 4 = POWER AVG 5 = MAX HOLD CONT	
Calc Mode : Max Hold	<n>MAX*</n>	ON OFF	<n>MAX?</n>	0 = OFF 1 = ON	
Calc Mode : Min Hold	<n>MIN*</n>	ON OFF	<n>MIN?</n>	0 = OFF 1 = ON	
Averaging and Power Averaging Times	<n>G*</n>	Integer	<n>G?</n>	Integer	

Francisco.	Comman	d (EXE, SET)	Que	Query (GET)	
Function	Code	Argument Format	Code	Output Format	
Averaging and Power Averaging Times Active Trace	SWPCNT*	Integer	SWPCNT?	Integer	
Average Start	<n>AVG* <n>GR</n></n>	ON	<n>AVG?</n>	0 = OFF	
Average Stop	<n>AVG* <n>GS</n></n>	OFF	7	1 = ON	
Average : Pause	<n>GP</n>		<n>GP?</n>	0 = Continue	
Average : Continue	<n>GC</n>		7	1 = Pause	
Average: 1 Time	<n>GSGL</n>		<n>GSGL?</n>	0 = sliding	
Average : Continuous	<n>GCNT</n>		7	1 = once	
Power Average Start	<n>PAVG*</n>	ON	<n>PAVG?</n>	0 = OFF	
Power Average Stop	<n>PAVG*</n>	OFF		1 = ON	
Power Average : Pause	<n>PGP</n>		<n>PGP?</n>	0 = Continue	
Power Average : Continue	<n>PGC</n>		7	1 = Pause	
Power Average : 1 Time	<n>PGSGL</n>		<n>PGSGL?</n>	0 = sliding	
Power Average : Continuous	<n>PGCNT</n>			1 = once	
Math : A-B→A	ABA				
Math : B-A→A	BAA				
Math : A-DL→A	ADLA				
Math : B-A→B	BAB				
Math : A-B→B	ABB				
Math : B-DL→B	BDLB				
Math : A-B→C	ABC				
Math : B-A→C	BAC				
Math: Trace Subtraction	TRSUB*	OFF ABA BAA ADLA BAB ABB BDLB ABC BAC	TRSUB?	0 = OFF 1 = ABA 2 = BAA 3 = ADLA 4 = BAB 5 = ABB 6 = BDLB 7 = ABC 8 = BAC	
Math: Trace Store (Current trace → trace n)	STORE*	TRA TRB TRC			
Number of Trace Points	TPS TP*	501	TP?	0 = 501	
	TPL TP*	1001		1 = 1001	

6.8.6 Trace

Frantisa	Comm	and (EXE, SET)	Que	ery (GET)
Function	Code	Argument Format	Code	Output Format
Detector Mode Trace A	DET*	NRM POS NEG SMP AVG QP	DET?	0 = NRM 1 = POS 2 = NEG 3 = SMP 4 = AVG 5 = QP
Detector Mode Trace B	DETB*	NRM POS NEG SMP AVG QP	DETB?	0 = NRM 1 = POS 2 = NEG 3 = SMP 4 = AVG 5 = QP
Detector Mode Trace C	DETC*	NRM POS NEG SMP AVG QP	DETC?	0 = NRM 1 = POS 2 = NEG 3 = SMP 4 = AVG 5 = QP
Detector Mode Auto	DETA <n>*</n>	ON OFF	DETA <n>?</n>	0 = OFF 1 = ON
Detector Average Mode	DETAVG*	RMS VIDEO	DETAVG?	0 = VIDEO 1 = RMS
Select Active Trace	TRACESEL*	TRA TRB TRC	TRACESEL?	0 = TRA 1 = TRB 2 = TRC
Trace A I/O ASCII	TAA	DDDDDSDLM>× TRP (*1)	TAA?	DDDDD <dlm>× TRP (*1)</dlm>
Trace A I/O Binary	TBA	2Bytes*TRP	TBA?	2Bytes×TRP
Trace B I/O ASCII	TAB	DDDDD <dlm>x TRP (*1)</dlm>	TAB?	DDDDD <dlm>× TRP (*1)</dlm>
Trace B I/O Binary	TBB	2Bytes×TRP	TBB?	2Bytes×TRP
Trace C I/O ASCII	TAC	DDDDD <dlm>x TRP (*1)</dlm>	TAC?	DDDDD <dlm>× TRP (*1)</dlm>
Trace C I/O Binary	TBC	2Bytes×TRP	TBC?	2Bytes×TRP
Trace Output Fornat				
16bits Integer	FORM1			
16bits Integer	FORM2			
IEEE 32bits Float	FORM3			
IEEE 32bits Float	FORM4			

6.8.7 Pass/Fail

Function	Comm	and (EXE, SET)	Qu	ery (GET)
Function	Code	Argument Format	Code	Output Format
Pass/Fail Judgement	PFC*	ON OFF	PFC?	0 = OFF 1 = ON
Judgement Result			PFJ? OPF?	0 = Pass 4 = Error 1 = Fail Limit 1 2 = Fail Limit 2 3 = Fail Limit 1&2
X Position Mode	LIMPOS*	ABS LFT CENT	LIMPOS?	0 = ABS 1 = CENT (center freq) 2 = LFT (start freq)
Y Position Mode	LIMAPOS*	ABS REF DL	LIMAPOS?	0 = ABS 1 = REF 2 = DL
X Offset Activate	LIMS*	ON OFF	LIMS?	0 = OFF 1 = ON
X Offset Frequency Domain	LIMSF*	Frequency	LIMSF?	Frequency
X Offset Time Domain	LIMST*	Time	LIMST?	Time
Y Offset Activate	LIMAS*	ON OFF	LIMAS?	0 = OFF 1 = ON
Y Offset	LIMASFT*	DB	LIMASFT?	DB
Limit Line 1	LMTA*	ON OFF	LMTA?	0 = OFF 1 = ON
Limit Line 1 Frequency Domain Data Input	LMTAINF*,*	Frequency, Level		
Limit Line 1 Time Domain Data Input	LMTAINT*,*	Time, Level		
Limit Line 1 Frequency Domain Data Erase	LMTADELF			
Limit Line 1 Time Domain Data Erase	LMTADELT			
Limit Line 2	LMTB*	ON OFF	LMTB?	0 = OFF 1 = ON
Limit Line 2 Frequency Domain Data Input	LMTBINF*,*	Frequency, Level		

6.8.8 Display

Function	Command (EXE, SET)		Query (GET)	
	Code	Argument Format	Code	Output Format
Limit Line 2 Time Domain Data Input	LMTBINT*,*	Time, Level		
Limit Line 2 Frequency Domain Data Erase	LMTBDELF			
Limit Line 2 Time Domain Data Erase	LMTBDELT			
Limit Line 1 Pass Range	LARNG*	ABOVE BELOW	LARNG?	0 = ABOVE 1 = BELOW
Limit Line 2 Pass Range	LBRNG*	ABOVE BELOW	LBRNG?	0 = ABOVE 1 = BELOW

6.8.8 Display

Function	Command (EXE, SET)		Query (GET)	
	Code	Argument Format	Code	Output Format
Display Line Level	DLN	Level	DLN?	Level
	DLN ON[,*] DLN OFF		DLNON?	0 = OFF 1 = ON
Reference Line Level	RLN*	Level	RLN?	Level
	RLN ON[,*] RLN OFF		RLNON?	0 = OFF 1 = ON
Window Center Position	WLX*	Frequency Time	WLX?	Frequency Time
Window Width	WDX*	Frequency Time	WDX?	Frequency Time
Window Sweep	WDOSWP*	ON OFF	WDOSWP?	0 = OFF 1 = ON
Zoom	MLTSCR*	ZM FT TT OFF	MLTSCR?	0 = OFF 1 = ZM 2 = FT 3 = TT 4 = DUAL VIEWER
Zoom Position	ZMPOS*	Frequency Time	ZMPOS?	Frequency Time
Zoom Width	ZMWID*	Frequency Time	ZMWID?	Frequency Time
Frequency Pos	FTPOS*	Frequency	FTPOS?	Frequency
Select Active Context	CTXTSEL*	Integer (0 1)	SCRSEL?	0 = CTXT A 1 = CTXT B

Function	Command (EXE, SET)		Query (GET)	
	Code	Argument Format	Code	Output Format
2 Channels Viewer	DUALCH[*]	[ON] OFF	DUALCH?	0 = OFF 1 = ON
2 Channel Preset	DUALCHINIT			

6.8.9 Marker

< n > = 0 | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10

NOTE: Marker 0 is the reference marker.

Function	Command (EXE, SET)		Query (GET)	
	Code	Argument Format	Code	Output Format
All Markers Off	MO MKOFF			
All Markers Off Except Active Marker	MLTOFF			
Select Active Marker	MKRSEL*	<n></n>	MKRSEL?	<n>></n>
Active Marker ON / OFF	MLN*	ON OFF	MLN?	0 = OFF 1 = ON
Marker ON / OFF	MLN <n>*</n>	[ON] OFF	MLN <n>?</n>	0 = OFF 1 = ON
Active Marker Frequency	MK*	Frequency Time	MK? MF?	Frequency Time
Marker Frequency	MF <n>*</n>	Frequency Time	MF <n>?</n>	Frequency Time
Active Marker Level			ML?	Level
Marker Level			ML <n>?</n>	Level
Active Marker Freq + Lev			MFL?	Frequency Time, Level
Marker Freq + Lev			MFL <n>?</n>	Frequency Time, Level
Active Marker Num + Stauts + Freq + Lev			MFLC?	Marker Number, Status (1=ON 0=OFF), Frequency Time, Level

6.8.9 Marker

Function	Command (EXE, SET)		Query (GET)	
	Code	Argument Format	Code	Output Format
MarkerNum + Stauts + Freq + Lev			MFLC <n>?</n>	Marker Number, Status (1=ON 0=OFF), Frequency Time, Level
Reference Marker Frequency Absolute Value			MDF2? MFR?	Frequency Time
Reference Marker Level Absolute Value			MDL2? MLR?	Level
Delta Mode	MKD*	[ON] OFF		
Reference Object	MKROBJ*	MARK RLIN	MKROBJ?	0 = MARK 1 = RLIN
Fixed ΔMarker	FX*	ON OFF	FX?	0 = OFF 1 = ON
Inverse \(\Delta Marker \)	REDLT*	ON OFF	REDLT?	0 = OFF 1 = ON
Delta Mode Reference	MKROJB*	MARK RLIN DLIN LLINU LLINL	MKROBJ?	MARK RLIN DLIN LLINU LLINL
Marker Step Size	MPM*	Frequency Time	MPM?	Frequency Time
Marker Step Auto	MPA[*]	[ON] OFF	MPA?	0 = OFF 1 = ON
Signal Track	SG[*]	[ON] OFF	SG?	0 = OFF 1 = ON
Signal Track Y Range	SGY[ON,]*	Level	SGY?	Level
	SGY ON SGY OFF		SGYON?	0 = OFF 1 = ON
Active Marker Trace	MKTRACE*	TRA TRB TRC	MKTRACE?	0 = TRA 1 = TRB 2 = TRC
Marker Mode	MKMODE*	INDEX VAL	MKMODE?	0 = INDEX 1 = VAL
Display Marker List	MKLST	ON OFF	MKLST?	0 = OFF 1 = ON
Get Marker List			MLSFL?	Num Marker, Active (1=ON 0=OFF), Frequency Time, Level (,)

6.8.10 Peak and Marker Move

6.8.10 Peak and Marker Move

Function	Command (EXE, SET)		Query (GET)	
	Code	Argument Format	Code	Output Format
$MKR \rightarrow CF$	MC MKCF			
$MKR\Delta \rightarrow CF$	MTCF			
$MKR \rightarrow REF$	MR MKRL			
$PEAK \rightarrow CF$	PKCF			
$PEAK \rightarrow REF$	PKRL			
$MKR\Delta \rightarrow SPAN$	DS MTSP			
$MKR \rightarrow CF Step$	M0 MKCS			
$MKR\Delta \rightarrow CF$ Step	M1 MTCS			
MKR → MKR Step	M2 MKMKS			
$MKR\Delta \rightarrow MKR$ Step	M3 MTMKS			

6.8.11 Peak

6.8.11 Peak

Function	Command (EXE, SET)		Query (GET)	
	Code	Argument Format	Code	Output Format
Peak Search	PS			
Next Peak	NXP			
Next Peak Left	NXL			
Next Peak Right	NXR			
Min Search	MIS			
Next Min Peak	NXM			
Min Max Peak	MMS			
Continuous Peak	CP*	ON OFF	CP?	0 = OFF 1 = ON
Peak ΔY Div	DY*	Level Div	DY?	Level Div
Peak List Frequency Level	PLS FREQ PLS LEVEL			
X Peak Area Couple to Window	MKSX	OFF IN OUT	MKSX?	0 = OFF 1 = IN 2 = OUT
X Peak Area Position	MKSPOS*	Frequency Time	MKSPOS?	Frequency Time
X Peak Area Width	MKSWID*	Frequency Time	MKSWID?	Frequency Time
Y Peak Area Couple to Display Line	MKSYDL	OFF ABOVE BELOW	MKSYDL?	2 = OFF 0 = ABOVE 1 = BELOW
Y Peak Area Couple to Limit Line 1	MKSYLA	OFF ABOVE BELOW	MKSYLA?	2 = OFF 0 = ABOVE 1 = BELOW
Y Peak Area Couple to Limit Line 2	MKSYLB	OFF ABOVE BELOW	MKSYLB?	2 = OFF 0 = ABOVE 1 = BELOW

6.8.12 Measurement

Emption	Comn	nand (EXE, SET)	Qu	iery (GET)
Function	Code	Argument Format	Code	Output Format
Noise	NI*	Frequency	NI?	Frequency
Noise ON + dBm/Hz	NIM			
Noise ON + $dB\mu V/\sqrt{Hz}$	NIU			
Noise ON + dBc/Hz	NIC			
Noise OFF	NIF			
Noise Mode Query			NION?	$0 = OFF$ $1 = dBm/Hz$ $2 = dB\mu V/\sqrt{Hz}$ $3 = dBc/Hz$
Noise Value			NIRES?	Level
X dB Down Level	MKBW*	DB	MKBW?	DB
X dB Down	XDB			
X dB Down Left	XDL			
X dB Down Right	XDR			
X dB Relative X dB Absolute Left X dB Absolute Right	DC0 DC1 DC2	 	DC?	0 = Relative 1 = Absolute Left 2 = Absolute Right
Continuous dB Down	CDB[*]	[ON] OFF	CDB?	0 = OFF 1 = ON
Peak + X dB Down	PSXDB			
IM Measurement Mode	IMM[*]	[ON] OFF	IMM?	0 = OFF 1 = ON
IM Reference Frequency			IMMREF?	Frequency, Level
IM Delta Frequency			IMMDF?	Delta Frequency
IM Distortion Signal Data Readout			IMMRES?	n <dlm>LL1, LJ1, UL1, UJ1<dlm> (*1)</dlm></dlm>
IM Order Setting	IMODR*	Integer (3 5 7 9)	IMODR?	Integer (3 5 7 9)
IM Criteria Input 3rd Order	IMLS3*	DB	IMLS3?	DB
IM Criteria Input 5th Order	IMLS5*	DB	IMLS5?	DB

6.8.12 Measurement

Function	Command	d (EXE, SET)	Query	y (GET)
	Code	Argument Format	Code	Output Format
IM Criteria Input 7th Order	IMLS7*	DB	IMLS7?	DB
IM Criteria Input 9th Order	IMLS9*	DB	IMLS9?	DB
IM Pass/Fail Judgement	IMPFC*	ON OFF	IMPFC?	0 = OFF 1 = ON
IM Save Setup	IMSAVE			
IM Restore Setup	IMLOAD			
Harmonics Measurement	HARM[*]	[ON] OFF	HARMON?	0 = OFF 1 = ON
Harmonics Results			HARM?	n <dlm>Freq1, Level1, DeltaLevel1 <dlm>(*2)</dlm></dlm>
Harmonics Max Order	HARMNUM*	Integer	HARMNUM?	Integer
Harmonics Fundamental	HRMFND [ON,] *	Frequency	HRMFND?	Frequency
	HRMFND ON HRMFND OFF		HRMFND ON?	0 = OFF 1 = ON

(*1)

n: Result set number corresponding to the order LLn: Level difference in the lower frequency signal LJn: Pass/Fail judgment in the lower frequency signal

0: Pass 1: Fail

-1: Judgment off

ULn: Level difference in the upper frequency signal UJn: Pass/Fail judgment in the upper frequency signal

<DLM>: Delimiter

(*2)

n: Result set number. Freqn: Harmonic frequency. Leveln: Harmonic level.

DeltaLeveln: Harmonic level difference with fundamental frequency.

<DLM>: Delimiter

Function	Command (EXE, SET)		Quer	Query (GET)	
	Code	Argument Format	Code	Output Format	
AM Modulation Measurement	AMMOD*	ON OFF	AMMODON?	0=OFF 1=ON	
AM Modulation Depth			AMMOD?	Real %	
AM Modulation			AMMF?	Frequency	
FM Measurement	FMMEAS*	ON OFF	FMMEASON?	0=OFF 1=ON	
FM Frequency Deviation			FMMEAS?	Frequency	
Modulation Frequency to Sweep time	FMMODF[ON,]* (*3)	Frequency	FMMODF?	Frequency	
	FMMODFY* (*4)	Frequency	FMMODFY?	Frequency	
	FMMODF*	ON OFF	FMMODFON?	0=OFF 1=ON	
Sound Mode					
:ON	SON		SD?	0 = OFF	
:ON (AM)	SAM			1 = ON (AM) $2 = ON (FM)$	
:ON (FM)	SFM			2 - ON (1:WI)	
:OFF	SOF				
Sound Volume	SDV*	Integer	SDV?	Integer	
Demodulation Time	PU*	Time	PU?	Time	

^(*3) Sets the Modulation Frequency to Sweep Time mode to ON and then sets an FM frequency deviation value.

^(*4) Sets an FM frequency deviation value without setting the Modulation Frequency to Sweep Time mode to ON.

6.8.13 Counter

6.8.13 Counter

Function	Command	l (EXE, SET)	Query	y (GET)
	Code	Argument Format	Code	Output Format
Resolution 1 kHz	CN0			
Resolution 100 Hz	CN1			
Resolution 10 Hz	CN2			
Resolution 1 Hz	CN3			
Resolution Query			CN?	0 = 1 kHz 1 = 100 Hz 2 = 10 Hz 3 = 1 Hz
Counter Position	CNPOS*	Frequency	CNPOS?	Frequency
Counter Position Auto (Position Linked to Marker)	CNPOSA[*]	[ON] OFF	CNPOSA?	0 = OFF 1 = ON
Counter	COUNT*	ON OFF	COUNT?	0 = OFF 1 = ON
Counter Value			CNRES?	Frequency

6.8.14 Power

Function	Command	(EXE, SET)	Query (GET)	
	Code	Argument Format	Code	Output Format
Measure Mode			PMEASMODE?	0 = OFF 1 = CHPOW 2 = TOTPOW 3 = AVGPOW 4 = OBW 5 = ACP 6 = SEM 7 = SPU
Measure OFF	PMEASOFF			
Measure Averaging	PMEASAVG*	ON OFF	PMEASAVG?	0 = OFF 1 = ON
	PMEASAVGONCE *	ONCE MULT	PMEASAVGON CE?	0 = ONCE 1 = MULT
Measure Averaging Times			PMEASTM?	Integer
Measure Trace	PMEASTRACE*	TRA TRB TRC	PMEASTRACE ?	0 = TRA 1 = TRB 2 = TRC
Channel Power ON/OFF	PWCHON[*]	[ON] OFF	PWCHON?	0 = OFF 1 = ON
Channel Power Average Times	PWCHTM*	Integer	PWCHTM?	Integer
Channel Power			PWCH?	Level
Channel Power Spectral Density			PWCHPSD?	dB
Power Measure Save	PWCHSAVE			
Power Measure Restore	PWCHLOAD			
Total Power ON/OFF	PWTOTALON[*]	[ON] OFF	PWTOTALON?	0 = OFF 1 = ON
Total Power Average Times	PWTOTALTM*	Integer	PWTOTALTM?	Integer
Total Power			PWTOTAL?	Level
Total Power Spectral Density			PWTOTALPSD ?	dB
Power Measure Save	PWTOTSAVE			
Power Measure Restore	PWTOTLOAD			

6.8.14 Power

Function	Comman	d (EXE, SET)	Query (GET)	
	Code	Argument Format	Code	Output Format
Average Power ON/OFF	PWAVGON[*]	[ON] OFF	PWAVGON?	0 = OFF 1 = ON
Average Power Average Times	PWAVGTM*	Integer	PWAVGTM?	Integer
Average Power Range	PWAVGRANGE*	FULL WIN	PWAVGRANGE ?	0 = FULL 1 = WIN
Average Power			PWAVG?	Level
Power Measure Save	PWAVGSAVE			
Power Measure Restore	PWAVGLOAD			
OBW Execution	OBWON[*]	[ON] OFF	OBWON?	0 = OFF 1 = ON
OBW Measurement Value			OBW?	Frequency (Fc), Frequency (OBW)
OBW %	OBWPER*	Real%	OBWPER?	Real%
OBW Average Times	OBWTM*	Integer	OBWTM?	Integer
OBW save setup	OBWSAVE			
OBW restore setup	OBWLOAD			
ACP Execution	ACP[*]	[ON] OFF	ACPON?	0 = OFF 1 = ON
ACP Measurement Value			ACP?	n <dlm>f1L,11L, f1H, l1H<dlm>(*1)</dlm></dlm>
ACP Average Times	ACPTM*	Integer	ACPTM?	Integer
ACP Reference Power Value			ACPREF?	Level
ACP Screen	ACPSCR*	FULL CARR	ACPSCR?	0 = FULL 1 = CARR
ACP Carrier Bandwidth	CARRBS* ACPCBW*	Frequency	CARRBS? ACPCBW	Frequency
CS/BS Table Input	CSBSIN*,*	Frequency (CS), Frequency (BS)		
CS/BS Table Deletion	CSBSDEL			
ACP Graphics Mode	ADG[*]	[ON] OFF	ADG?	0 = OFF 1 = ON
ACP save setup	ACPSAVE			
ACP restore setup	ACPLOAD			
ACP Nyquist Filter	ACPNQST*	ON OFF	ACPNQST?	0 = OFF 1 = ON

Function	Comma	nd (EXE, SET)	Quer	Query (GET)	
i unction	Code	Argument Format	Code	Output Format	
Nyquist Symbol Rate	SYMRT*	Frequency	SYMRT?	Frequency	
Nyquist Roll Off Factor	RFACT*	Real	RFACT?	Real	
Spectrum Emission Mask Execution	SEMON[*]	[ON] OFF	SEMON?	0 = OFF 1 = ON	
SEM Average Times	SEMTM*	Integer	SEMTM?	Integer	
SEM Carrier Bandwidth	SEMCBW*	Frequency	SEMCBW?	Frequency	
SEM Ref Power	SEMRFCALC*	CHN PEAK	SEMRFCALC?	0 = Channel 1 = Peak	
SEM Nyquist Filter	SEMNQST*	ON OFF	SEMNQST?	0 = OFF 1 = ON	
SEM save setup	SEMSAVE				
SEM restore setup	SEMLOAD				
SEM Band Table Input	SEMTIN ********	Frequency, (start) Frequency, (stop) Frequency, (ibw) dB, (limit abs start) dB, (limit abs stop) dB, (limit rel start) dB, (limit rel stop) ABS REL A_AND_R A_OR_R (judge)			
SEM Band Table Delete	SEMTDEL				
SEM Reference Power			SEMRFPOW?	dBm	
SEM Measurement Value			SEM?	Channel Number, Start Frequency, Stop Frequency, Frequency, Absolute Power, Relative Power, Judge (,)	
Spurious Measurement Execution	SPURI*	[ON FREQ] OFF	SPURION?	0 = OFF 1 = ON	

6.8.14 Power

Function	Command	(EXE, SET)	Query (GET)	
Tunction	Code	Argument Format	Code	Output Format
SPU Measurement Result			SPURI?	n <dlm>m1<dl M>f1, 11, j1<dlm> fm1, lm1, jm1<dlm>m2<d LM>f1, 11, j1<dlm> fm2, lm2, jm2<dlm>mn <dlm>f1, 11, j1<dlm> fmn, lmn, jmn<dlm>(*2)</dlm></dlm></dlm></dlm></dlm></d </dlm></dlm></dl </dlm>
SPU Table Selection	SPRTBL*	Integer (0 1 2)	SPRTBL?	Integer (0 1 2)
SPU Table Input Freq	SPRIN SPRFIN *,*,*,*,*	Freq, (start) Freq, (stop) AUTO Freq, (rbw) AUTO Time, (swp) Level, (ref level) AUTO Level, (att) ON OFF, (preamp) Level (Limit)		
SPU Freq Table Deletion	SPRFDEL			

(*1)

n: Number of points (0 thru 5)

fnL: nth frequency Low nth level Low fnH: nth frequency High nth level High <DLM>: Delimiter

(*2)

n: Number of measurement points (0 thru 15) m: Number of spurious signal (0 thru 10)

f: Spurious frequency l: Spurious level

j: Spurious judgment result (0:Pass, 1:Fail)

<DLM>: Delimiter

6.8.15 EMC

Function	Command (EXE, SET)		Query (GET)	
Function	Code	Argument Format	Code	Output Format
Correction Factor	CR[*]	[ON] OFF	CRON?	0 = OFF 1 = ON
Correction Factor Table Input	CRIN*,*	Frequency, Level(DB)		
Correction Factor Table Deletion	CRDEL			
EMC Trace Detection OFF ON	EMCON EMCDET	NRM OFF PEAK ON	EMCON? EMCDET?	0 = OFF 3 = ON
EMC BW Auto 200 Hz 9 kHz 120 kHz 1 MHz	QPAUTO QA QP0 QP1 QP2 QP3		QPAUTO? QA?	0 = Auto 1 = 200 Hz 2 = 9 kHz 3 = 120 kHz 4 = 1 MHz

6.8.16 Calibration

Function	Command (EXE, SET)		Query (GET)	
runction	Code	Argument Format	Code	Output Format
Calibration All	CLALL			
Total Gain Calibration	CLGAIN[*]	[RFC1] RFC2	CLGAIN [RFC1] RFC2?	Integer 0 = OK >0 = Warning <0 = Error
RBW Calibration	CLRBW		CLRBW?	Integer 0 = OK >0 = Warning <0 = Error
PBW Calibration	CLPBW		CLPBW?	Integer 0 = OK >0 = Warning <0 = Error

6.8.17 Save/Recall

Function	Command (EXE, SET)		Query (GET)	
runction	Code	Argument Format	Code	Output Format
ATT step Calibration	CLATT		CLATT?	Integer 0 = OK >0 = Warning <0 = Error
CAL 10 M Reference Coarse	CLCREF*	Integer	CLCREF?	Integer
CAL 10 M Reference Fine	CLFREF*	Integer	CLFREF?	Integer
CAL 10 M Reference Default	CLDREF			
CAL 10 M Reference Store	CLSREF			
F-Correction	FC*	ON OFF	FC?	0 = OFF 1 = ON
CAL-Correction	CC*	ON OFF	CC?	0 = OFF 1 = ON

6.8.17 Save/Recall

Function	Comman	d (EXE, SET)	Query	y (GET)
	Code	Argument Format	Code	Output Format
Save (File or File Number)	SV[*]	:String Integer		
Delete (File)	DEL*	:String		
Recall (File)	RC*	:String		
Rename (File, New Name)	RENAME*,*	:String, :String		
Write Protect (File)	WP*,*	:String, ON OFF		
File Format	FILEFORMAT*	BIN XML	FILEFORMAT?	0 = BIN 1 = XML
Media	FILEMEDIA*	FLASH USB	FILEMEDIA?	0 = FLASH 1 = USB
Save Setup	SVSET*	ON OFF	SVSET?	0 = OFF 1 = ON
Save Trace A Context 1	SVTRC1A*	ON OFF	SVTRC1A?	0 = OFF 1 = ON

6.8.17 Save/Recall

Function	Comm	and (EXE, SET)	Que	ery (GET)
runction	Code	Argument Format	Code	Output Format
Save Trace B Context 1	SVTRC1B*	ON OFF	SVTRC1B?	0 = OFF 1 = ON
Save Trace C Context 1	SVTRC1C*	ON OFF	SVTRC1C?	0 = OFF 1 = ON
Save Trace A Context 2	SVTRC2A*	ON OFF	SVTRC2A?	0 = OFF 1 = ON
Save Trace B Context 2	SVTRC2B*	ON OFF	SVTRC2B?	0 = OFF 1 = ON
Save Limit Line 1	SVLIM1*	ON OFF	SVLIM1?	0 = OFF 1 = ON
Save Limit Line 2	SVLIM2*	ON OFF	SVLIM2?	0 = OFF 1 = ON
Save Spurious Table 1	SVSPR1*	ON OFF	SVSPR1?	0 = OFF 1 = ON
Save Spurious Table 2	SVSPR2*	ON OFF	SVSPR2?	0 = OFF 1 = ON
Save Spurious Table 3	SVSPR3*	ON OFF	SVSPR3?	0 = OFF 1 = ON
Save Channel	SVCH*	ON OFF	SVCH?	0 = OFF 1 = ON
Save Spectrum Emission Mask Table	SVSEM*	ON OFF	SVSEM?	0 = OFF 1 = ON
Save ACP	SVACP*	ON OFF	SVACP?	0 = OFF 1 = ON
Save Correction Factor	SVANT*	ON OFF	SVANT?	0 = OFF 1 = ON
Save Normalize Context A Trace A	SVNRM1A	ON OFF	SVNRM1A?	0 = OFF 1 = ON
Save Normalize Context A Trace B	SVNRM1B	ON OFF	SVNRM1B?	0 = OFF 1 = ON
Save Normalize Context A Trace C	SVNRM1C	ON OFF	SVNRM1C?	0 = OFF 1 = ON
Syncronize All Files : USB to Flash : Flash to USB	SYNCTO	FLASH USB		

6.8.18 File Management

6.8.18 File Management

Function	Command (EXE, SET)		Query (GET)	
1 unction	Code	Argument Format	Code	Output Format
Reading Bitmap File			BMP?	Binary data <eoi></eoi>
Reading Portable Network Graphics File			PNG?	Binary data <eoi></eoi>
Reading Image File			GIMAG :String	Binary data <eoi></eoi>
Reading Data File			GDATA :String	Binary data <eoi></eoi>

6.8.19 Config

Function	Command (EXE, SET)		Query (GET)	
Tunction	Code	Argument Format	Code	Output Format
Title	LON*	/*String*/	LB?	String
Erase Title	LOF			
10 MHz Internal Reference Signal Source	RFI		FREF?	0 = INT 1 = EXT
10 MHz External Reference Signal Source	RFE			2 = XTL
Xtal	RFX			
Reference Signal Source	RF*	Frequency	RF?	Frequency
Input RF Connector	RFC	RFC1 RFC2	RFC?	1 = RFC1 2 = RFC2
Device Select Printer USB	HCDEV	PRT USB	HCDEV?	0 = Printer 1 = USB
Screen Copy	НСОРҮ			

6.8.20 Preset

Function	Command (EXE, SET)		Query (GET)	
1 unction	Code	Argument Format	Code	Output Format
Preset	IP *RST			
Factory Init	SUPIP			

6.8.21 **GPIB**

Function	Comm	nand (EXE, SET)	Qı	uery (GET)
Tunction	Code	Argument Format	Code	Output Format
Status Byte Clear	*CLS			
STB Read			*STB?	Integer
SRE Read/Write	*SRE0*	Integer	*SRE?	Integer
ESR Read			*ESR?	Integer
ESE Read/Write	*ESE	Integer	*ESE?	Integer
OSR Read			OPREVT?	Integer
OSER Read	OPR*	Integer	OPR?	Integer
SRQ Interrupt ON	S0			
SRQ Interrupt OFF	S1			
SRQ status clear	S2			
Delimiter CR LF EOI	DLIM0			
Delimiter LF	DLIM1			
Delimiter EOI	DLIM2			
Delimiter;	DLIM5			
Local Lockout	LLO			
Remote Control	REN			
Local Control	GTL			
R3162 Mode	INSTR*	FUS SA2	INSTR?	0 = FUS
				1 = SA2
Refresh Screen in Remote	SCRF[*]	[ON] OFF	SCRF?	ON OFF
Control				
Open Menus in Remote Control	MNRF[*]	[ON] OFF	MNRF?	ON OFF
Annotations	ANNOT[*]	[ON] OFF	ANNOT?	ON OFF
Parser Mode	PARSER*	ATSET SCPISET	PARSER?	0 = AT 1 = SCPI

TRP: Number of trace points <DLM>: Delimiter (*1)

6.8.22 Others

6.8.22 Others

Function	Comman	d (EXE, SET)	Query (GET)		
Function	Code	Argument Format	Code	Output Format	
Device ID Output			*IDN? ID?	Maker Name, Device Name, Serial No., Revision	
Date Setting	SETDATE*	Date (YYMMDD)	SETDATE?	Date	
Time Setting	SETTIME*	Time (HHMMSS)	SETTIME?	Time	
Reset user password (for front panel lock)	RPWD				
Option List			*OPT?	Opt1,Opt2,, Optn <dlm></dlm>	
Option					
: 2CH Input			OPT10?	1 = Installed	
: 2CH Input 75 Ohm			OPT11?	0 = Not installed	
:75 Ohm Input			OPT15?		
: High Stability			OPT20?		
: EMC Filter			OPT28?		
: 3GPP Demod			OPT50?		
: Time Domain			OPT53?		
: Time Domain 2CH			OPT54?		
: TG -30 dBm			OPT74?		
: TG -60 dBm 75 Ohm			OPT75?		
: TG -60 dBm			OPT76?		
: TG High Freq.			OPT77?		
Execute Self Test			*TST?	Supply_Voltage, judge <dlm> (*1) Memory, judge<dlm> CPU_Registers, judge<dlm> RF_Registers, judge<dlm> RF_PLL_Lock, judge<dlm> LO_Registers, judge<dlm> LO_PLL_Lock, judge<dlm> AIF_Registers, judge<dlm> AIF_Registers, judge<dlm> TG_Registers, judge<dlm> (*2) Temperature, judge<dlm> (*1)</dlm></dlm></dlm></dlm></dlm></dlm></dlm></dlm></dlm></dlm></dlm>	

^(*1) CH1 @ 2ch option (*2) CH1 @2ch option & TG Option

6.8.23 TG

Function	Comma	nd (EXE, SET)	Que	Query (GET)	
i unction	Code	Argument Format	Code	Output Format	
TG ON	TG		TG?	0 = OFF 1 = ON	
TG OFF	TGF				
TG Level	TGL*	Level	TGL?	Level	
TG Frequency Offset	TGO[ON,]* TGO ON OFF	Frequency	TGO? TGOON?	Frequency 0 = OFF 1 = ON	
TG Level Offset	TGLO[ON,]* TGLO ON OFF	DB	TGLO? TGLOON?	DB 0 = OFF 1 = ON	
Capture Normalize Data Active Trace	CAPND				
Normalize Correction Active Trace	NORM*	ON OFF	NORM?	0 = OFF 1 = ON	
Capture Normalize Data Trace (n = $A B C$)	<n>RX</n>				
Normalize Correction Trace (n = $A B C$)	<n>NORM*</n>	ON OFF	<n>NORM?</n>	0 = OFF 1 = ON	
Normalize Execute Active Trace	AR				
Delta Reference Line	TGDLTRLN*	ON OFF	TGDLTRLN?	0 = OFF 1 = ON	
VSWR ON/OFF	VSWRON [*]	[ON] OFF	VSWRON?	0 = OFF 1 = ON	
VSWR Measurement Value			VSWR?	Real	
VSWR Return Loss Value			VSWRLOSS?	DB (Real)	

6.8.24 Units

6.8.24 Units

Function	Code
Exponent	E (see IEEE Std 488.2-1992 page 89)
GHz	GZ
MHz	MZ
KHz	KZ
Hz	HZ
DB	DB
DBM	DBM
DBMV	DBMV
DBUV	DBUV
DBEMF	DBEMF
DBPW	DBPW
Watt	W WATT
mW	MW
Volt	V VOLT
Millivolt	MV
Microvolt	UV
Nanovolt	NV
Second	SC
Millisecond	MS MSEC
Microsecond	US USEC
Nanosecond	NSEC
%	% PER
ppm	PPM

6.9 Example of Remote Control Programs

6.9 Example of Remote Control Programs

This chapter describes examples of programs which control the instrument by remote.

The example programs in this chapter use the Microsoft Corp. Visual Basic language. If programming in another language, the example programs must be described in that language.

The explanation of the programs here assumes that the GPIB board provided by the National Instruments Corp. (hereafter referred to as the NI Corp.) is used as a GPIB controller.

6.9.1 Basic Steps for GPIB Bus Control

This section describes the step-by-step procedures in which the GPIB bus is controlled by the Visual Basic programs. For operations such as initializing variables and defining function routines, which depend on Visual Basic, the notational rules for the Visual Basic program must be applied.

6.9.1.1 Reading the GPIB Control Library for Visual Basic

To control the GPIB board provided by NI Corp. by using the program described in the Visual Basic language, the two files must be built into the Visual Basic Project. Those two files are the VBIB-32.BAS file, in which the GPIB communication interface for the Visual Basic language provided by the NI Corp. is described, and the NIGLOBAL.BAS file, in which errors and timeout values are defined.

6.9.1.2 Program Examples Using VB

Example 1 Setting the center frequency after resetting this instrument.

```
Call ibdev(0,8,T10S,1,0,SPA) 'Initialize 'Performs a Device Clear.

Call ibwrt(spa, "IP") 'preset 'Sets the center frequency to 30 MHz.
```

Example 2 Setting the start frequency to 300 kHz, setting the stop frequency to 800 kHz and adding 50 kHz to the frequency offset.

```
Call ibclr(spa) ' Performs a Device Clear.

Call ibwrt(spa, "FA 300KZ") ' Sets the start frequency to 300 kHz.

Call ibwrt(spa, "FB 800KZ") ' Sets the stop frequency to 800 kHz.

Call ibwrt(spa, "FO 50KZ") ' Adds 50 kHz to the frequency offset.
```

Example 3 Setting the reference level to 87 dBµV (in 5 dB/div) and the RBW to 100 kHz

```
Call ibclr(spa) ' Performs a Device Clear.

Call ibwrt(spa, "AUNITS DBUV") ' Sets the level unit to dB\muV.

Call ibwrt(spa, "RL 87DB") ' Sets the reference level to 87 dB (\muV).

Call ibwrt(spa, "DD 5DB") ' Sets the vertical scale to 5 dB/div.

Call ibwrt(spa, "RB 100KZ") ' Sets the RBW to 100 kHz.
```

Example 4 Setting the instrument using variables

Example 5 Saving set values in Register 5 and recalling them from Register 5

```
Dim LabelBuff As String
                                 ^{\prime} Defines the character string buffer for the
LabelBuff = "SPECTRUM Analyzer"' Sets the label.
Call ibclr(spa)
                                 ' Performs a Device Clear.
Call ibwrt(spa, "CF 30MZ")
Call ibwrt(spa, "SP 1MZ")
                                 ' Sets the parameter.
Call ibwrt(spa, "DET POS")
Call ibwrt(spa, "LON " & LabelBuff)
                                 ' Sets the label.
Call ibwrt(spa, "SV 5")
                                 ' Saves the data to Register 5.
Call ibwrt(spa, "CF 1GZ")
                                 ' Changes the set parameters.
Call ibwrt(spa, "SP 200MZ")
Call ibwrt(spa, "RC 5") ' Recalls the data from Register 5.
```

Example 6 Enter Limit line1 in the table and turn Limit line 1 on

```
Call ibclr(spa)
                                         ' Performs a device clear.
Call ibwrt(spa, "LMTADEL")
                                       ' Clears the table used for Limit Line 1.
Call ibwrt(spa, "AUNITS DBUV") ' Sets the level unit to \text{dB}\mu\text{V}.
Call ibwrt(spa, "LMTAIN 25MZ, 49.5DB")
                                        ' Enters data used by Limit Line 1.
Call ibwrt(spa, "LMTAINF 35MZ, 49.5DB")
Call ibwrt(spa, "LMTAINF 35MZ, 51.5DB")
Call ibwrt(spa, "LMTAINF 55MZ, 51.5DB")
Call ibwrt(spa, "LMTAINF 55MZ, 54.3DB")
Call ibwrt(spa, "LMTAINF 65MZ, 54.3DB")
Call ibwrt(spa, "LMTAINF 65MZ, 57.0DB")
Call ibwrt(spa, "LMTAINF 68MZ, 57.0DB")
Call ibwrt(spa, "LMTAINF 68MZ, 60.0DB")
Call ibwrt(spa, "LMTAINF 75MZ, 60.0DB")
Call ibwrt(spa, "LMTAINF 75MZ, 62.5DB")
Call ibwrt(spa, "LMTAINF 82MZ, 62.5DB")
Call ibwrt(spa, "LMTAINF 82MZ, 64.7DB")
Call ibwrt(spa, "FA OMZ")
                                        ' Sets the start frequency to 0 MHz.
Call ibwrt(spa, "FA OMZ )

Call ibwrt(spa, "FB 100MZ") 

Call ibwrt(spa, "LMTA ON") 

' Sets the stop frequency to 100 MHz.

Turns Limit line 1 on.
```

6.9.1.3 Sample Programs for Reading Data

In order to output measurement data or settings, use the "xx?" command. This ensures that the data is read when this instrument is in the talker mode. Available output formats are listed in the table below. The delimiter positioned at the end of data can be specified from 5 types (refer to "Others" in the GPIB code list). Once set, "xx?" command continues to operate until it is changed.

	Output Format				
Frequency	$\begin{array}{c ccccccccccccccccccccccccccccccccccc$				
Level	$\begin{array}{c ccccccccccccccccccccccccccccccccccc$				
Time	$\begin{array}{cccccccccccccccccccccccccccccccccccc$				
Constant	DDDD CR LF ↑ ↑ 2 4 The maximum size of the data in bytes corresponds to the maximum size of the output data ExampleThe ON/OFF status or Averaging count is output				

<Supplement>1 = Sign (a space for plus sign; "-" for minus sign)

- 2 = Mantissa of data
- 3 = Exponent of data
- 4 = Delimiter (CR/LF in initial setting can be changed with "DLn" code.)

Example 1 Reading and displaying the marker level

```
Dim sep As Integer
Call ibclr(spa)
                                  ' Performs a device clear.
Call ibwrt(spa, "CF 30MZ")
                                  ' Sets the parameter.
Call ibwrt(spa, "SP 1MZ")
Call ibwrt(spa, "MLN ON")
                                  ' Marker ON
Call ibwrt(spa, "MK 30MZ")
Call ibwrt(spa, "TS")
                                 ^{\prime} Sets the marker to 30 MHz.
Call ibwrt(spa, "ML?")
                                  ' Requests the value of the marker level.
Rdbuff = Space(30)
                                  ' Allocates 30 bytes to the buffer area.
                                 ^{\prime} Reads the data (30 bytes Max.).
Call ibrd(spa, Rdbuff)
sep = InStr(1, Rdbuff, vbCrLf, 0)
                                 ^{\prime} Checks the number of character up to the
                                 ^{\prime} delimiter.
RichTextBox1.Text = "MarkerLevel = " & Left(Rdbuff, sep - 1)
                                 ' Displays the data on the screen.
An example display:
MarkerLevel = -88.1875
```

Example 2 Reading and displaying the center frequency

```
Dim sep As Integer
Call ibclr(spa)
                               ' Performs a Device Clear.
Call ibwrt(spa, "CF?")
                               ' Query command for the center frequency.
                               ' Allocates 30 bytes to the buffer memory.
Rdbuff = Space(30)
                              ' Reads the data (30 bytes Max.)
Call ibrd(spa, Rdbuff)
sep = InStr(1, Rdbuff, vbCrLf, 0)
                               ' Checks the number of character to the
                               ' delimiter.
RichTextBox1.Text = "CenterFreq = " & Left(Rdbuff, sep - 1)
                               ' Displays the data on the screen.
An example display:
CenterFreq = +3000000.0000
```

Example 3 Reading the level and display unit and displaying them

```
Dim sep As Integer
Call ibclr(spa)
                                ' Performs a Device Clear.
Call ibwrt(spa, "RL?")
                                ' Query command for the reference level.
Rdbuff = Space(30)
                                ' Allocates 30 bytes to the buffer memory.
                                ^{\prime} Reads the data from the spectrum analyzer.
Call ibrd(spa, Rdbuff)
sep = InStr(1, Rdbuff, vbCrLf, 0)
                                ' Checks the number of characters to the
                                ' delimiter.
RichTextBox1.Text = "RefLevel = " & Left(Rdbuff, sep - 1)
                                ' Display the data on the screen.
Call ibwrt(spa, "AUNITS?")
                                ' Requests the level unit.
Rdbuff = Space(3)
Call ibrd(spa, Rdbuff)
sep = InStr(1, Rdbuff, vbCrLf, 0)
                                ^{\prime} Checks the number of characters to the
                                ' delimiter.
RichTextBox1.Text = RichTextBox1.Text & vbCrLf & "UNIT = " & Left(Rdbuff, sep
                                  1)
                                ^{\prime} Displays the previous result, followed by a
                                ' return mark and the most recent result.
An example display:
RefLevel = +0.0000
UNIT = 0
```

Example 4 Executing the 6 dB-down operation, reading the frequency and level and displaying them

```
Dim sep As Integer
Call ibclr(spa)
                              ' Performs a Device Clear.
Call ibwrt(spa, "CF 30MZ")
                              ' Sets the parameter.
Call ibwrt(spa, "SP 20MZ")
Call ibwrt(spa, "MKBW 6DB")
                             ' Sets a 6 dB down measurement.
Call ibwrt(spa, "PS")
Call ibwrt(spa, "XDB")
                             ' Executes the peak search.
                             ^{\prime} Performs the 6 dB down measurement.
Call ibwrt(spa, "MFL?")
                             ' Requests the value of the marker level and
                              ' frequency.
Rdbuff = Space(50)
                              ' Allocates the buffer memory space to 50
                              ' bytes.
                              ' Reads the data (50 bytes Max.) from the
Call ibrd(spa, Rdbuff)
                              ' spectrum analyzer.
sep = InStr(1, Rdbuff, vbCrLf, 0)
                              ' Checks the number of characters to the
                              ' delimiter.
RichTextBox1.Text = "Marker Freq & Level = " & Left(Rdbuff, sep - 1)
                              ' Displays the data on the screen.
An example display:
```

Example 5 Measuring OBW and displaying it

```
Dim LENG1 As Integer, LENG2 As Integer
Dim OBW As String
Dim FC As String
Dim searchchar As String
                                ' Performs a device clear.
Call ibclr(spa)
Call ibwrt(spa, "CF 30MZ")
                                ' Sends the command already set.
Call ibwrt(spa, "SP 1MZ")
Call ibwrt(spa, "MLN ON")
                                ' Marker ON
Call ibwrt(spa, "MK 30MZ")
Call ibwrt(spa, "OBWON ON")
Call ibwrt(spa, "TS")
Call ibwrt(spa, "OBW?")
                                ^{\prime} Sends the query command.
Rdbuff = Space(60)
                                ' Allocates the area to the read buffer.
                                ^{\prime} Reads the read buffer (the maximum number of
Call ibrd(spa, Rdbuff)
                                 ' bytes to be output is determined by the buffer
                                 ' area size).
                                ' Formatting output character string
LENG1 = InStr(1, Rdbuff, Chr(44), 0)
                                 ' Searches for the first comma.
FC = Mid(Rdbuff, 1, LENG1 - 1) 'Reads the character before the comma.
DoEvents
LENG2 = InStr((LENG1 + 1), Rdbuff, Chr(13), 0)
                                ^{\prime} Determines the last data by searching for the
                                ^{\prime} delimiter.
OBW = Mid(Rdbuff, (LENG1 + 1), (LENG2 - LENG1-1))
                                 ' Reads the data between the second comma and
                                 ^{\prime} the delimiter.
RichTextBox1.Text = "OBW = " & OBW & vbCrLf & "Fc = " & FC & vbCrLf
                                ' Displays the data on the screen.
An example display:
OBW = +9.81000000000E+05
FC = +3.000250000000E+07
```

Example 6 Reading and displaying the three largest peak levels

```
Dim pkl As String, pk2 As String, pk3 As String
                                   ' Performs a device clear.
Call ibclr(spa)
Call ibwrt(spa, "CF OMZ")
Call ibwrt(spa, "SP 100MZ")
Call ibwrt(spa, "TS")
                                   ' Applies the settings.
Call ibwrt(spa, "PS")
                                   ' Executes the peak search.
Call ibwrt(spa, "ML?")
                                   ^{\prime} Query command to search for the marker level
Rdbuff = Space(25)
                                   ' Allocates the buffer memory.
                            ' Receives the output.
Call ibrd(spa, Rdbuff)
pk1 = LeftB(Rdbuff, (InStrB(1, Rdbuff, Chr(13), 1) - 1))
                                   ' Reads the data between the starting point and
                                   ' the delimiter.
Call ibwrt(spa, "NXP")
                                   ' Searches for the next peak.
Call ibwrt(spa, "ML?")
Rdbuff = Space(25)
Call ibrd(spa, Rdbuff)
pk2 = LeftB(Rdbuff, (InStrB(1, Rdbuff, Chr(13), 1) - 1))
                                   ^{\prime} Reads the data between the starting point and
                                   ^{\prime} the delimiter.
Call ibwrt(spa, "NXP")
Call ibwrt(spa, "ML?")
Rdbuff = Space(25)
Call ibrd(spa, Rdbuff)
pk3 = LeftB(Rdbuff, (InStrB(1, Rdbuff, Chr(13), 1) - 1))
                                   ' Reads the data between the starting point and
                                   ^{\prime} the delimiter.
RichTextBox1.Text = "1st PK = " & pk1 & vbCrLf & "2nd PK = " & pk2 & vbCrLf &
                                   "3rd PK = " & pk3 & vbCrLf
                                   ' Displays the data on the screen.
An example display:
1st PK = -8.553906250000E+01
2nd PK = -7.004687500000E+01
3rd PK = -8.655468750000E+01
```

6.9.1.4 Sample Programs for Inputting or Outputting Trace Data

Trace data on the screen includes data for 501 or 1001 points on the frequency axis. For inputting and outputting data, it is necessary to transfer data for 501 or 1001 points from the left side (start frequency) in order. Each point level is expressed by an integer from 1792 to 14592 (however, if the trace exceeds the upper limit of the vertical scale, a value greater than 14592 is transferred).

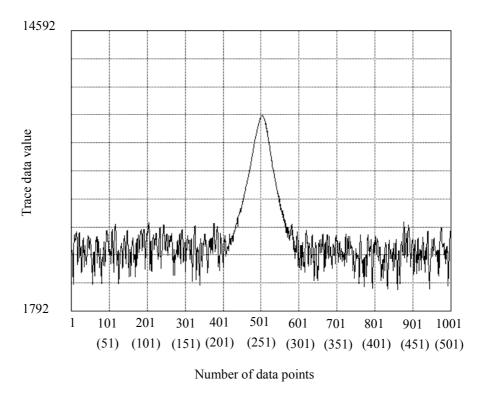


Figure 6-7 Relationship between the Screen Graticule and Trace Data

Trace data can be input or output in either ASCII or binary format.

Specify the output by using 16-bit integer data or the absolute value when outputting a value with binary data.

For the "FORM1" or "FORM3" format, transfer data in order from the high-order byte of the data. For the "FORM2" or "FORM4" format, transfer data in order from the low-order byte.

NOTE: Only "dB" can be used as a unit for the absolute value output.

When the Units setting is Watts or Volts, a value with a unit of dBm is output.

Table 6-4 Trace Point Specification Codes

GPIB Code	Description
TPS	Sets the number of measurement points to 501.
TPL	Sets the number of measurement points to 1001.

Table 6-5 Binary Data Output Format Specified Code

GPIB code	Description	Byte order
FORM1 (*1)	16-bit integer value from 1792 to 14592	
FORM2 (*2)	16-bit integer value from 1792 to 14592	Order swap
FORM3 (*2)	Absolute value IEEE 32 bit floating-point type	
FORM4 (*2)	Absolute value IEEE 32 bit floating-point type	Order swap

^{*1:} When not specified, FORM1 is used.

^{*2:} The input format cannot be specified.

Table 6-6 I/O Format

I/O format	Description				
ASCII format	DDDDD CR LF				
	Five-byte data with	hout header			
		Input GPIB code	Output GPIB code		
	Memory A Memory B Memory C	TAA TAB TAC	TAA? TAB? TAC?		
Binary format 16 bit-integer	FORM2 DD DI High-order byte for 1st point FORM2 DD Of for 1st point Low-order byte for 1st point Each point data is order bytes. EOI si continuous 1001 p Memory A	rder byte point High-order for 1001/5 D	DD + EOI Delimiter h-order byte 1001/501st point r byte 501st point s: high-and low-e end of the data for Output GPIB code TBA?		
	Memory B Memory C	TBB TBC	TBB? TBC?		

I/O format Description Binary format FORM3 32-bit floating point \underline{DD} \underline{DD} Delimiter Low-order byte Low-order byte for 1001/501st point for 1st point High-order byte High-order byte for 1st point for 1001/501st point For DDDDDDDD=12345678, data is output in order from 12345678. FORM4 \underline{DD} \underline{DD} \underline{DD} \underline{DD} \underline{DD} \underline{DD} \underline{DD} \underline{DD} + \underline{EOI} Delimiter High-order byte High-order byte for 1st point for 1001/501st point Low-order byte Low-order byte for 1st point for 1001/501st point For DDDDDDDD=12345678, data is output in order from 78563412. Each point data is 32-bit (4 bytes) floating-point type. EOI signal is attached at the end of the data for continuous 1001 points. Output GPIB code TBA? Memory A TBB? Memory B TBC? Memory C

Table 6-7 Absolute Value Output Format

Example 1 Read the trace data in ASCII format

```
Dim tr(1000) As String
                                 ^{\prime} Allocates an array in the buffer for 1001
                                 ' points.
Dim i As Integer
Dim res As String
Call ibclr(spa)
                                 ' Performs a Device Clear.
Call ibwrt(spa, "DLIM0")
                                 ' CR LF EOI
Call ibwrt(spa, "TAA?")
For i = 0 To 1000 Step 1
                                 ' Repeats the operation for 1001 points.
                                 ^{\prime} Allocates 7 bytes (5 bytes for the data, and
  tr(i) = Space(7)
                                 ' 2 bytes for delimiters).
  Call ibrd(spa, tr(i))
                                 ' Reads the data.
                                 ^{\prime} Displays the data on the screen.
 res = res & "tr(" & Str(i) & ") = " & Left(tr(i), 5) & vbCrLf
  DoEvents
Next i
RichTextBox1.Text = res
```

Example 2 Reading the memory A data in binary format

```
^{\prime} Allocates an array in the buffer for 1001
Dim tr(1000) As Integer
                               ' points.
Dim i As Integer
Dim res As String
Dim Rslt As Integer, tmp As Integer
Call ibclr(spa)
                               'Performs a device clear.
Call ibconfig(0, IbcEndBitIsNormal, 0)
                               ' Sets the GPIB-board software so that the end
                                ' bit of the Ibsta variable is set to 1 only
                               ' when EOI has been received.
                               ' Sets the delimiter to EOI only.
Call ibwrt(spa, "DLIM2")
                              ' Requests Trace A in binary data.
Call ibwrt(spa, "TBA?")
Call ibrdi(spa, tr(), 1001 * 2)' Reads 1001 points of binary data.
For i = 0 To 1000 Step 1
                              ' Repeats the operation for 1001 points.
                               ' Swaps the high and low bites.
    tmp = tr(i)
   Rslt = (tmp And \&HFF\&) * 256
    Rslt = Rslt + ((tmp And &HFF00&) / 256)
    res = res & Str(Rslt) & vbCrLf
                               'Displays the data on the screen.
   DoEvents
Next i
RichTextBox1.Text = res
Call ibwrt(spa, "DLIMO")
                           'Sets the delimiter to the CR, LF and EOI.
Call ibconfig(0, IbcEndBitIsNormal, 1)
```

Example 3 Entering data into memory A in ASCII format

```
Dim trdata(1000) As Integer
Dim i As Integer
trdata(0) = 1792
                                ' Creates a temporary test value used to test
                                ' the input (*).
For i = 1 To 1000 Step 1
 trdata(i) = Str(Val(trdata(i - 1)) + 12)
 DoEvents
Next i
                                ' If measurement data exists, the steps between
                                ^{\prime} the place marked with (*) and this point are
                                ' not required.
                                ' Performs a device clear.
Call ibclr(spa)
Call ibwrt(spa, "AB")
                               ' Sets Trace A to BLANK.
Call ibwrt(spa, "TAA")
                               ' Sets Trace A in ASCII.
                               ' Repeats the operation for 1001 points.
For i = 0 To 1000 Step 1
 Call ibwrt(spa, CStr(trdata(i)))
                                ' Sends the value after it has been converted
                                ' to the ASCII data.
  DoEvents
Next i
Call ibwrt(spa, "AV")
                                ' Sets Trace A to VIEW.
```

<Program example of absolute value output>

When using FORM3, add the line shown below to NIGLOBAL.

The CopyValtoVal API function is required to shift 32 bits.

Declare Sub CopyValtoVal Lib "kernel32" Alias "RtlMoveMemory" (Destination As Any, Source As Any, ByVal length As Long)

Example 4 FORM2 Reading the memory A data in binary 16-bit integer (order swap)

```
Dim tr(1000) As Integer
                               ' Allocates an array in the buffer for 1001
                               ' points.
Dim i As Integer
Dim res As String
Call ibclr(spa)
                               ' Performs a Device Clear.
                              ' Switches to FORM2.
Call ibwrt(Spa, "FORM2")
Call ibconfig(0, IbcEndBitIsNormal, 0)
                               ' Sets the GPIB-board software so that the end
                               ' bit of each Ibsta variable is set to 1 only
                               ' when EOI has been received.
Call ibwrt(Spa, "DLIM2")
                              ' Sets a delimiter to EOI only.
Call ibwrt(Spa, "TBA?")
                              ' Requests Trace A in binary data.
Call ibrdi(Spa, tr(), 1001 * 2)' Reads 1001 points of binary data.
For i = 0 To 1000 Step 1
                             ' Repeats the operation for 1001 points.
   res = res & Str(tr(i)) & vbCrLf
                               ' Displays the data on the screen.
   DoEvents
Next. i
RichTextBox1.Text = res
Call ibwrt(Spa, "DLIM0")
                             ' Sets the delimiter to the CR, LF and EOI.
Call ibconfig(0, IbcEndBitIsNormal, 1)
```

Example 5 FORM3 Reading the memory A data in binary 32-bit floating point

```
^{\prime} Allocates an array in the buffer for 1001
Dim tr(1000) As Single
                                  ' points.
                                 ' 32-bit floating point type
Dim i As Integer
Dim res As String
Dim tra(4) As Byte
                                 ' Variable which swaps the high-order byte and
                                 ' low-order byte
                                 ^{\prime} Variable which swaps the high-order byte and
Dim tran As Byte
                                 ' low-order byte
                                 ' Variable which stores converted data
Dim tmp As Single
Call ibclr(spa)
                                 ' Performs a Device Clear.
Call ibwrt(Spa, "FORM3")
                                 ' Switches to FORM3.
Call ibconfig(0, IbcEndBitIsNormal, 0)
                                 ^{\prime} Sets the GPIB-board software so that the end
                                 ' bit of each Ibsta variable is set to 1 only
                                 ^{\prime} when EOI has been received.
Call ibwrt(Spa, "DLIM2")
Call ibwrt(Spa, "TBA?")
                                 ' Sets a delimiter to EOI only.
                                 ' Requests Trace A in binary data.
Call ibrd32(Spa, tr(0), 1001 * 4)
                                 ' Reads 1001 points of binary data.
                                 ' * 4 for four bytes.
For i = 0 To 1000 Step 1
                                 ' Repeats the operation for 1001 points.
    Call CopyValtoVal(tra(0), tr(i), 4)
                                 ' Copies the 4-byte data stored in tri(i) to
                                 ' tra (0 to 3).
                                 ' Swaps the high and low orders.
    tran = tra(0)
     tra(0) = tra(3)
     tra(3) = tran
     tran = tra(1)
     tra(1) = tra(2)
     tra(2) = tran
     Call CopyValtoVal(tmp, tra(0), 4)
                                 ' Copies the 4-byte data stored in tra (0 to
                                 ' 3), whose high and low orders are swapped, to
                                 ' tmp.
     res = res & Str(tmp) & vbCrLf
     DoEvents
Next i
                            ' Displays the data on the screen.
' Sets the delimiter to the CR, LF and EOI.
RichTextBox1.Text = res
Call ibwrt(Spa, "DLIM0")
Call ibconfig(0, IbcEndBitIsNormal, 1)
```

Example 6 FORM4 Reading the memory A data in binary 32-bit floating point (order swap)

```
Dim tr(1000) As Single
                               ' Allocates an array in the buffer for 1001
                               ' points.
                               ' 32-bit floating point type
Dim i As Integer
Dim res As String
Call ibclr(spa)
                               ' Performs a Device Clear.
                               ' Switches to FORM3.
Call ibwrt(Spa, "FORM4")
Call ibconfig(0, IbcEndBitIsNormal, 0)
                               ' Sets the GPIB-board software so that the end
                               ^{\prime} bit of each Ibsta variable is set to 1 when
                               ' EOI has been received.
Call ibwrt(Spa, "DLIM2")
                               ' Sets a delimiter to EOI only.
Call ibwrt(Spa, "TBA?")
                               ' Requests Trace A in binary data.
Call ibrd32(Spa, tr(0), 1001 * 4)
                                ' Reads 1001 points of binary data.
                               ' * 4 for four bytes.
For i = 0 To 1000 Step 1
                              ' Repeats the operation for 1001 points.
   res = res & Str(tr(i)) & vbCrLf
                               ' Displays the data on the screen.
   DoEvents
Next. i
RichTextBox1.Text = res
Call ibwrt(Spa, "DLIM0")
                               ' Sets the delimiter to the CR, LF and EOI.
Call ibconfig(0, IbcEndBitIsNormal, 1)
```

6.9.1.5 Example Program for Screen Image Output

Example 1 Outputs a current screen image as bitmap data and writes it to a file.

Data, which is approximately 150 KB for the BMP format or approximately 5 KB for the PNG format, is output.

```
Call ibclr(spa) 'Performs a Device Clear.

Call ibwrt(spa, "DLIM2") 'Sets a delimiter to EOI only.

Call ibwrt(spa, "BMP?") 'Requests bitmap data output.

Call ibrdf(spa, "bitmap.bmp") 'Writes bitmap data to a file.

Call ibwrt(spa, "DLIM0") 'Returns delimiter setting to CR, LF and EOI.
```

Example 2 Writes a screen image that is copied into a USB memory to a file.

```
Call ibclr(spa) 'Performs a Device Clear.

Call ibwrt(spa, "DLIM2") 'Sets a delimiter to EOI only.

Call ibwrt(spa, "GIMAG :copy003.bmp") 'Specifies a screen image name and requests 'its output.

Call ibrdf(spa, "copy003.bmp") 'Writes a screen image to a file.

Call ibwrt(spa, "DLIM0") 'Returns delimiter setting to CR, LF and EOI.
```

6.9.1.6 Example Program Which Uses the TS (Take Sweep) Command

Example 1 An ACP measurement is taken and then the measurement result is read (using the TS command).

```
Dim state As Integer
Dim sep1 As Integer, sep2 As Integer
Dim i As Integer, j As Integer
Dim cnt As Integer
Dim LvlH As String, LvlL As String
Dim FrqH As String, FrqL As String
Call ibclr(spa)
                                ' Performs a Device Clear.
Call ibwrt(spa, "SI")
                                ' Sets the single mode.
Call ibwrt(spa, "CF 1500MZ")
                              ' Sets the center frequency to 1500 MHz.
                                ^{\prime} Sets the frequency span to 250 kHz.
Call ibwrt(spa, "SP 250KZ")
                               ' Sets RBW to 1 kHz.
Call ibwrt(spa, "RB 1KZ")
Call ibwrt(spa, "VB 3KZ")
                                ' Sets VBW to 3 kHz.
Call ibwrt(spa, "ST 20SC")
                                ' Sets the sweep time to 20 sec.
Call ibwrt(spa, "CSBSDEL")
                                ^{\prime} Clears the channel space and bandwidth
                                ' previously set.
Call ibwrt(spa, "CSBSIN 50KZ,21KZ")
                                ' Sets CS to 50 kHz, and BS to 21 kHz.
                                ' Starts the ACP measurement.
Call ibwrt(spa, "ACP ON")
For j = 1 To 10 Step 1
                                ' Executes one sweep.
  Call ibwrt(spa, "TS")
  Call ibwrt(spa, "ACP?")
                                ' Requests the result of the ACP measurement.
                                ^{\prime} Assigns 1 byte for an integer and 2 bytes for
  Rdbuff = Space(3)
                                ' a delimiter before reading the result.
                                ' Reads the data.
  Call ibrd(spa, Rdbuff)
                                ' Converts the contents of the buffer into
  cnt = CInt(Rdbuff)
                                ' integers.
  For i = 1 To cnt Step 1
                                ^\prime Assigns an area of 81 bytes (Real number x 4
    Rdbuff = Space(81)
                                ' + ',' x 3 + CRLF).
                                ' Reads the data.
    Call ibrd(spa, Rdbuff)
    sep1 = InStr(1, Rdbuff, ",", 0)
                                  Searches for the first comma starting from
                                ' the top of the buffer.
    FrqL = Left(Rdbuff, sep1 - 1)
                                ' Reads the string between the top and the
                                ' character string.
    sep2 = InStr(sep1 + 1, Rdbuff, ", ", 0)
                                ' Searches for the next comma.
    LvlL = Mid(Rdbuff, sep1 + 1, sep2 - sep1 - 1)
                                 Reads the string between the first and second
                                ' commas.
    sep1 = InStr(sep2 + 1, Rdbuff, ", ", 0)
                                ' Searches for the next comma.
    FrqH = Mid(Rdbuff, sep2 + 1, sep1 - sep2 - 1)
                                ^{\prime} Reads the string between the second and third
                                ' commas.
    sep2 = InStr(sep1, Rdbuff, Chr(13), 0)
                                 Searches for the terminator (CR).
```

6.9.1.7 Example Programs Which Use the Status Byte

Example 1 Execute a single sweep and wait until its finished (when not using SRQ).

```
Dim state As Integer
Call ibclr(spa)
                               ' Performs a Device Clear.
Call ibwrt(spa, "SI")
                              ^{\prime} Turns the single sweep mode on.
Call ibwrt(spa, "OPR8")
                              ' Enables the sweep-end bit of the operation
                               ' status register.
Call ibwrt(spa, "*CLS")
                               ' Clears the status byte.
                               ' Begins sweeping.
Call ibwrt(spa, "SI")
Do
  Call ibwrt(spa, "*STB?")
                              ' Requests the value of the status byte.
                               ' Reserve a maximum of 8 bytes including the
  Rdbuff = Space(8)
                               ' delimiter.
                               ' Reads the data.
 Call ibrd(spa, Rdbuff)
                               ' Converts the character string into numeric
  state = Val(Rdbuff)
                               ' values.
  DoEvents
                               ' Checks the loop for other events currently
                               ' taking place.
Loop Until (state And 128)
                               ' Exits from the loop if the sweep-end bit is
                               ' set to 1.
```

Example 2 Reading the peak frequency and level at the end of a single sweep (when using SRQ)

```
Dim boardID As Integer
Dim I As Integer
Dim res As Integer
Dim CFLEV As String
                                ' Sets the board ID.
boardID = 0
Call ibclr(spa)
                                ' Performs a Device Clear.
Call ibwrt(spa, "SI")
                                ' Turns the single sweep mode on.
Call ibwrt(spa, "*CLS")
                                ' Clears the status byte.
Call ibwrt(spa, "OPR 8")
                               ^{\prime} Enables the Sweep-end bit of the operation
                                ' status register
                               ' Enables the Operation status bit of the
Call ibwrt(spa, "*SRE 128")
                               ' status byte.
                               ' Specifies Send mode for the SRQ signal.
Call ibwrt(spa, "S0")
```

```
' Sets up a 10-loop.
For I = 1 To 10 Step 1
                               ' Begins sweeping.
  Call ibwrt(spa, "SI")
                              ' Waits until SRQ interruption occurs.
  Call WaitSRQ(boardID, res)
                                ' Executes serial polling.
 Call ibrsp(spa, res)
  Call ibwrt(spa, "PS")
                                ' Executes the peak search.
                                ^{\prime} Request the values of the marker frequency ^{\prime} and level.
  Call ibwrt(spa, "MFL?")
                                ' Reserves 43 bytes.
 Rdbuff = Space(43)
  Call ibrd(spa, Rdbuff)
                                ' Reads the data.
  CFLEV = Left(Rdbuff, InStr(1, Rdbuff, Chr(13), 0) - 1)
  RichTextBox1.Text = RichTextBox1.Text & "Freq ,Level = " & CFLEV & vbCrLf
                                ' Display data on the screen and start a new
                                 ' line.
  DoEvents
                                ' Executes any other events in Windows.
Next I
```

6.9.1.8 Program Examples Using the LAN

Example 1 Connection LAN Interface

```
Public Sub ConnectTCP()
Dim Ini as String
tcpClient.RemoteHost = "192.168.1.1"
                              ' Sets IP Address of SA
tcpClient.Protocol = sckTCPProtocol
                             ' Sets protocol to TCP
                              ' Sets port no. 5025 of SA
tcpClient.RemotePort = 5025
                              ' Connects to SA's port
tcpClient.Connect
  Do While (tcpClient.BytesReceived = 0)
                               'Waits connection
   DoEvents
  Loop
  tcpClient.GetData Ini
  ErrRet = SendDtFunc("REN" & vbLf)
                              'Remote enable
End Sub
```

Example 2 Initialize Spectrum Analyzer

Example 3 Brief setting of Spectrum Analyzer

(Set Center freq. to 1.9984 GHz, Span to 10 MHz and Reference level to 10 dBm)

```
Public Sub SASetting()
tcpClient.SendData "CF 1.9984GZ" & vbLf
tcpClient.SendData "SP 10MZ" & vbLf
tcpClient.SendData "RL 10DB" & vbLf
End Sub
```

Example 4 Read the setting value of Spectrum Analyzer

```
Public Sub ReadSASetting( )
CF$= Space$(20)
                               ' Prepares the text variable for read
tcpClient.SendData "CF?" & vbLf' Reads request of center freq.
Do While (tcpClient.BytesReceived = 0)
                               ' Waits for receiving a character
 DoEvents
Loop
tcpClient.GetData CF$
                              ' Reads setting value
                              ' Prepares the text variable for read
SP$= Space$(20)
tcpClient.SendData "SP?" & vbLf' Reads request of span freq.
Do While (tcpClient.BytesReceived = 0)
                               ' Waits for receiving a character
 DoEvents
Loop
tcpClient.GetData SP$
                              ' Reads setting value
```

Example 5 Display setting value

```
Call MsgBox( "Center freq.: " & CF$ & "Span freq.: " & SP$) End Sub
```

Example 6 Read signal level using the marker function

```
Public Sub ReadMkrSignal( )
MKLevel$= Space$(20)
                             ' Prepares the text variable for read
tcpClient.SendData "MLN ON"& vbLf
                              ' Turns on the marker
tcpClient.SendData "PS" & vbLf ' Searches peak point of signal
tcpClient.SendData "MF?" & vbLf' Query the marker frequency
Do While (tcpClient.BytesReceived = 0)
                              ' Waits for receiving a character
 DoEvents
Loop
tcpClient.GetData MKFreq$
                             ' Reads it
tcpClient.SendData "ML?" & vbLf' Query the marker level
Do While (tcpClient.BytesReceived = 0)
                               ' Waits for receiving a character
 DoEvents
Loop
tcpClient.GetData MKlevel$
                             ' Reads it
```

Example 7 Display the freq. and level of signal

```
Call MsgBox("Marker freq.: " & MKFreq$ & " Level: " & MKLevel$) End Sub
```

6.9.1 Basic Steps for GPIB Bus Control

Example 8 Measure Adjacent Channel Power

```
Public Sub MeasACP()
ResultACP$ = Space(200)
tcpClient.SendData "CF 2GZ" & vbLf' Sets carrier freq.
tcpClient.SendData "SP 25MZ" & vbLf
```

Example 9 Setting of Adjacent channel parameters

Example 10 Setting of Root Nyquist filter's parameters

```
tcpClient.SendData "ACPNQST ON" & vbLf
                               ' Sets Nyq. Filter operation to on
tcpClient.SendData "SYMRT 3.84MZ" & vbLf
' Sets Symbol rate of filter
tcpClient.SendData "RFACT 0.22" & vbLf
                               ' Sets Roll off factor of filter
tcpClient.SendData "ACPTM 10" & vbLf
                               ' Sets average times
tcpClient.SendData "PMEASAVG ON" & vbLf
                               ' Sets average func. to ON
tcpClient.SendData "ACP" & vbLf' Starts measurement
tcpClient.SendData "*CLS;OPR 16;*SRE 128" & vbLf
                               'Sets status byte
Stb$ = Space(10)
  tcpClient.SendData "*STB?" + vbLf
  Do While (tcpClient.BytesReceived = 0)
                               ' Waits for receiving a character
   DoEvents
 Loop
  tcpClient.GetData Stb
  If CLng(Val(Stb)) And 128 Then Exit Do
tcpClient.SendData "ACP?" + vbLf
tcpClient.GetData ResultACP$ ' Reads out all meas. results of ACP
Call MsgBox("ACP results : " & ResultACP$)
End Sub
```

6.10 SCPI Command Reference

6.10 SCPI Command Reference

This chapter describes the SCPI command reference for this instrument.

6.10.1 Command Reference Syntax

This section describes the function, syntax, and parameter of each SCPI command discussed in this chapter

- [Function description]

 How to use a command or operations when the command is executed are described.
- [SCPI command]
 Syntax when the command is sent from an external controller to this instrument is described.
 Example: Marker setting

Function description	SCPI command	Parameter	Query reply
Enable Marker	:CALCulate#1:MARKer#2:STATe @3 \$1 = :CALCulate#1:MARKer#2:STATe?	Context index, Marker index, ON OFF	1 0
	Space		#1 #2 @3

- 1. The syntax consists of a command section and parameter section.

 The command section and parameter section are delimited by a space.
- 2. #1, #2, and @3 are parameters required for sending a command.

 A number that follows on # or @ corresponds to a row number in the parameter column.

 The # parameter may be omitted. If omitted, the parameter is set to 1.

 The @ parameter cannot be omitted.
- 3. Lowercase alphabetical characters written in syntax can be omitted.
- 4. [] shows that the command is optional. This command can be omitted.
- 5. "|" shows that only one item is required to be selected from multiple items.

6.10.1 Command Reference Syntax

• [Parameter]

Following parameters from 1 to 7 can be omitted:

1. Context Index

1|2|0

1 = Context A (RF2)

2 = Context B (RF1)

0 = Active context

2. Marker Index

1|2|3|4|5|6|7|8|9|10|0

0 = Active marker

3. Trace Index

1|2|3|0

1 = Trace A

2 = Trace B

3 = Trace C

0 = Active trace

4. Limit Line Index

1|2

5. SEM channel Index

1|2|3|4|5|

6. Spurious band Index

1|2|3|4|5|6|7|8|9|10|11|12|13|14|15

7. Spurious Table Index

1|2|3

8. Intermodulation Order Index

3|5|7|9

This parameter cannot be omitted.

- [Query reply]
 - 1. \$1

This query reply shows that one variable is replied. For this example, 1 or 0 is replied.

2. Example of a query reply consisting of multiple variables

\$1,\$2,\$3,\$4=*IDN?

6.10.2 Common Commands

6.10.2 Common Commands

This section describes IEEE common commands.

Function description	SCPI Command	Parameter	Query reply	Remarks
Goto Local (LAN)	GTL	_	_	
Local Lockout (LAN)	LLO	_	_	
Set Operation Register Mask	OPR @1 \$1 = OPR?	16 bit register	16 bit register	
Query Operation Register	\$1 = OPREVT?	_	16 bit register	
Set the parser command set	PARSER @1 \$1 = PARSER ?	ATset SCPIset	AT SCPI	
REN	REN	_	_	
Clear Registers	*CLS	_	_	
Enable Standard Event Register	*ESE @1 \$1 = *ESE?	8 bit register	8 bit register	
Query Standard Event Register	\$1 = *ESR?	_	8 bit register	
Return various identifiers of the instrument	\$1, \$2, \$3, \$4 = *IDN?	_	Corporate Name (String), Model Name (String), Serial Number (String), Software version (String)	
Instrument Preset	*RST	_	_	
Set Service Request Enable	*SRE @1 \$1 = *SRE?	8 bit register	8 bit register	
Query Status Byte	\$1 = *STB?	_	8 bit register	
Execute Self Test	\$1,{\$2,\$3} = *TST?	_	number of rows {check item (SUPP MEM CPU RFRG RFLK LORG LOLK IFRG IFLK TGRG TEMP), check result (Status)}	
Wait	*WAI	_	_	
Query Installed Option Number	\$1,\$2,\$n = *OPT?	_	Option No. (string)	

6.10.3.1 Subsystem-CALCulate

Function description	SCPI command	Parameter	Query reply	Remarks
Set Center Frequency From Delta Marker Postion Difference	:CALCulate#1:MARKer#2:DELTa[:SET] :CENTer	Context index, Marker index		
Set Marker Step From Marker Delta Position Difference	:CALCulate#1:MARKer#2:DELTa[:SET] :MARKer:STEP	Context index, Marker index		
Set Span From Delta Marker Position Difference	:CALCulate#1:MARKer#2:DELTa[:SET] :SPAN	Context index, Marker index		
Set Frequency Step From Marker Delta Position Difference	:CALCulate#1:MARKer#2:DELTa[:SET] :STEP	Context index, Marker index		
Execute X dB Down	:CALCulate#1:MARKer#2:FUNCtion :XDBDown	Context index, Marker index		
Execute X dB Left	:CALCulate#1:MARKer#2:FUNCtion :XDBDown:LEFT	Context index, Marker index		
Execute Peak Search and X dB Down	:CALCulate#1:MARKer#2:FUNCtion :XDBDown:PEAK	Context index, Marker index		
Execute X dB Right	:CALCulate#1:MARKer#2:FUNCtion :XDBDown:RIGHt	Context index, Marker index		
Get Specific Marker Information	\$1,\$2,\$3,\$4 = :CALCulate#1:MARKer#2 :INFO?	Context index, Marker index	marker index (Marker index), marker enable (1 0), marker position (Position (Hz s)), marker amplitude (Amplitude)	
Execute Next Peak Search to the Left	:CALCulate#1:MARKer#2:MAXimum :LEFT	Context index, Marker index		
Execute Next Peak Search	:CALCulate#1:MARKer#2:MAXimum :NEXT	Context index, Marker index		
Execute Next Peak Search to the Right	:CALCulate#1:MARKer#2:MAXimum :RIGHt	Context index, Marker index		
Execute Maximum Peak Search	:CALCulate#1:MARKer#2:MAXimum [:PEAK]	Context index, Marker index		
Execute Next Minimum Search	:CALCulate#1:MARKer#2:MINimum :NEXT	Context index, Marker index		
Execute Minimum Search	:CALCulate#1:MARKer#2:MINimum [:PEAK]	Context index, Marker index		
Execute Minimum Maximum Search	:CALCulate#1:MARKer#2:PTPeak	Context index, Marker index		
Enable Marker	:CALCulate#1:MARKer#2:STATe @3 \$1 = :CALCulate#1:MARKer#2:STATe?	Context index, Marker index ON OFF	1 0	
Select Marker Trace	:CALCulate#1:MARKer#2:TRACe @3 \$1 = :CALCulate#1:MARKer#2:TRACe?	Context index, Marker index, Trace index	Trace index	

Function description	SCPI command	Parameter	Query reply	Remark
Set Marker Position	:CALCulate#1:MARKer#2:X @3 \$1 = :CALCulate#1:MARKer#2:X?	Context index, Marker index, Frequency Time	Position (Hz s)	
Get Marker Absolute Position	\$1 = :CALCulate#1:MARKer#2:X :ABSolute?	Context index, Marker index	Position (Hz s)	
Get Marker Coordinates	\$1, \$2 = :CALCulate#1:MARKer#2:XY?	Context index, Marker index	Position (Hz s), amplitude (Amplitude)	
Get Marker Amplitude	\$1 = :CALCulate#1:MARKer#2:Y?	Context index, Marker index	Amplitude	
Get Marker Absolute Amplitude	\$1 = :CALCulate#1:MARKer#2:Y :ABSolute?	Context index, Marker index	Amplitude	
Set Center Frequency from Marker Position	:CALCulate#1:MARKer#2[:SET] :CENTer	Context index, Marker index		
Set Marker Step from Marker Position	:CALCulate#1:MARKer#2[:SET] :MARKer:STEP	Context index, Marker index		
Set Reference Level from Marker Amplitude	CALCulate#1:MARKer#2[:SET] :RLEVel	Context index, Marker index		
Set Span from Marker Delta Position Difference	:CALCulate#1:MARKer#2[:SET] :SPAN	Context index, Marker index		
Set Center Frequency Step from Marker Position	:CALCulate#1:MARKer#2[:SET] :STEP	Context index, Marker index		
Select Active Marker	:CALCulate#1:MARKer:ACTive @2 \$1 = :CALCulate#1:MARKer:ACTive?	Context index, Marker index	Marker index	
Query Markers List	\$1, {\$2,\$3,\$4,\$5} = :CALCulate#1 :MARKer:ALL:INFO?	Context index	number of rows {marker index (Marker index), marker enable (1 0), marker position (Position (Hz s)), marker amplitude (Amplitude)}	
Clear All Markers	:CALCulate#1:MARKer:AOFF	Context index		
Enable Continuous Peak Search	:CALCulate#1:MARKer :CPEak[:STATe] @2 \$1 = :CALCulate#1:MARKer :CPEak[:STATe]?	Context index, ON OFF	1 0	
Enable Fixed Reference Marker Mode	:CALCulate#1:MARKer:DELTa :FIXed[:STATe] @2 \$1 = :CALCulate#1:MARKer:DELTa :FIXed[:STATe]?	Context index, ON OFF	1 0	
Enable Marker Delta Mode	:CALCulate#1:MARKer:DELTa [:STATe] @2 \$1 = :CALCulate#1:MARKer:DELTa [:STATe]?	Context index, ON OFF	1 0	
Set Center Frequency from Peak	:CALCulate#1:MARKer:MAXimum [:SET]:CENTer	Context index		
Set Reference Level from Peak	:CALCulate#1:MARKer:MAXimum [:SET]:RLEVel	Context index		
Set Marker Mode	:CALCulate#1:MARKer:MODE @2 \$1 = :CALCulate#1:MARKer:MODE?	Context index, POSition DELTa	POS DELT	

Function description	SCPI command	Parameter	Query reply	Remarks
Set Peak Excursion	:CALCulate#1:MARKer:PEAK :EXCursion @2 \$1 = :CALCulate#1:MARKer:PEAK :EXCursion?	Context index, Number	Number	
Set the Delta Marker Reference Object	:CALCulate#1:MARKer:REFerence :OBJEct @2 \$1 = :CALCulate#1:MARKer:REFerence :OBJEct ?	Context index, RMARker RLINe	RMAR RLIN	
Query Reference Marker Absolute Position	\$1 = :CALCulate#1:MARKer:REFerence :X?	Context index	Position (Hz s)	
Query Reference Marker Absolute Amplitude	\$1 = :CALCulate#1:MARKer:REFerence :Y?	Context index	Amplitude	
Turn Off Multi-Marker Mode	:CALCulate#1:MARKer:RESet	Context index		
Set X Axis Marker Search Area Mode	:CALCulate#1:MARKer:SEARch:X :MODE @2 \$1 = :CALCulate#1:MARKer:SEARch:X :MODE?	Context index, ALL INNer OUTer	ALL INN OUT	
Set X Axis Marker Search Area Center Position	:CALCulate#1:MARKer:SEARch:X :POSition @2 \$1 = :CALCulate#1:MARKer:SEARch:X :POSition?	Context index, Frequency Time	Position (Hz s)	
Set X axis Marker Search Area Width	:CALCulate#1:MARKer:SEARch:X :WIDTh @2 \$1 = :CALCulate#1:MARKer:SEARch:X :WIDTh?	Context index, Frequency Time	Position (Hz s)	
Set the Marker Search Area Relative to the Display Line	:CALCulate#1:MARKer:SEARch:Y :DLINe @2 \$1 = :CALCulate#1:MARKer:SEARch:Y :DLINe?	Context index, OFF ABOVe BELow	OFF ABOV BEL	
Set the Marker Search Area Relative to Limit Line 1	:CALCulate#1:MARKer:SEARch:Y :LIM#2 @3 \$1 = :CALCulate#1:MARKer:SEARch:Y :LIM#2?	Context index, Limit line index, OFF ABOVe BELow	OFF ABOV BEL	
Set Marker Step	:CALCulate#1:MARKer:STEP @2 \$1 = :CALCulate#1:MARKer:STEP?	Context index, Frequency Time	Position (Hz s)	
Enable Marker Step Auto	:CALCulate#1:MARKer:STEP :AUTO @2 \$1 = :CALCulate#1:MARKer:STEP :AUTO?	Context index, ON OFF	1 0	
Set Signal Track Y Ranging Excursion	:CALCulate#1:MARKer:TRCKing :EXCursion @2 \$1 = :CALCulate#1:MARKer:TRCKing :EXCursion?	Context index, Relative amplitude	Relative amplitude	
Enable Signal Track Y Ranging	:CALCulate#1:MARKer:TRCKing :EXCursion:STATe @2 \$1 = :CALCulate#1:MARKer:TRCKing :EXCursion:STATe?	Context index, ON OFF	1 0	
Set Marker Readout Mode	:CALCulate#1:MARKer:X:READout @2 \$1 = :CALCulate#1:MARKer:X :READout?	Context index, NORMal INVerse	NORM INV	
Set Measuring Window Position	:CALCulate#1:WINDow:POSition @2 \$1 = :CALCulate#1:WINDow:POSition?	Context index, Frequency Time	Position (Hz s)	

Function description	SCPI command	Parameter	Query reply	Remark
Set Measuring Window Width	:CALCulate#1:WINDow:WIDTh @2 \$1 = :CALCulate#1:WINDow:WIDTh?	Context index, Frequency Time	Position (Hz s)	
Insert a Limit Line Vertex	:CALCulate:LLINe#1:DATA @2 :CALCulate:LLINe#1:DATA @2	Limit line index, X-coordinate of limit line point (Time), ordinate of limit line point (Relative amplitude)		
Insert a Frequency Domain Limit Line Vertex	:CALCulate:LLINe#1:DATA :FREQuency @2	Limit line index, X-coordinate of table point (Frequency), ordi- nate of table point (Relative amplitude)		
Insert a Time Domain Limit Line Vertex	:CALCulate:LLINe#1:DATA:TIME @2	Limit line index, X-coordinate of limit line point (Time), ordinate of limit line point (Relative amplitude)		
Erase a Limit Line	:CALCulate:LLINe#1:DELete	Limit line index		
Erase a Frequency Domain Limit Line	:CALCulate:LLINe#1:DELete :FREQuency	Limit line index		
Erase a Time Domain Limit Line	:CALCulate:LLINe#1:DELete:TIME	Limit line index		
Enable a Limit Line	:CALCulate:LLINe#1:DISPlay @2 \$1 = :CALCulate:LLINe#1:DISPlay?	Limit line index, ON OFF	1 0	
Set Limit Lines Detection Type	:CALCulate:LLINe#1:TYPE @2 \$1 = :CALCulate:LLINe#1:TYPE?	Limit line index, UPPer LOWer	UPP LOW	
Set Limit Lines X axis Reference	:CALCulate:LLINe:CMODe @1 \$1 = :CALCulate:LLINe:CMODe?	FIXed RELative	FIX REL	
Set Limit Lines X axis Reference	:CALCulate:LLINe:CMODe:X @1 \$1 = :CALCulate:LLINe:CMODe:X?	ABSolute CENTer LEFT	ABS CENT LEFT	
Set Limit Lines Frequency Offset	:CALCulate:LLINe:CMODe:X :OFFSet:FREQuency @1 \$1 = :CALCulate:LLINe:CMODe:X :OFFSet:FREQuency?	Frequency	Frequency	
Enable Limit Lines X axis Offset	:CALCulate:LLINe:CMODe:X :OFFSet:STATe @1 \$1 = :CALCulate:LLINe:CMODe:X :OFFSet:STATe?	ON OFF	1 0	
Set Limit Lines Time Offset	:CALCulate:LLINe:CMODe:X :OFFSet:TIME @1 \$1 = :CALCulate:LLINe:CMODe:X :OFFSet:TIME?	Time	Time	
Select Limit Lines Y axis Positioning	:CALCulate:LLINe:CMODe:Y @1 \$1 = :CALCulate:LLINe:CMODe:Y ?	ABSolute TOP DLINe	ABS TOP DLIN	
Set Limit Lines Y axis Offset	:CALCulate:LLINe:CMODe:Y :OFFSet @1 \$1 = :CALCulate:LLINe:CMODe:Y :OFFSet?	Relative amplitude	Relative amplitude	

Function description	SCPI command	Parameter	Query reply	Remarks
Enable Limit Line Y axis Offset	:CALCulate:LLINe:CMODe:Y :OFFSet:STATe @1 \$1 = :CALCulate:LLINe:CMODe:Y :OFFSet:STATe?	ON OFF	1 0	
Select Limit Line Domain	:CALCulate:LLINe:CONrol :DOMain @1 \$1 = :CALCulate:LLINe:CONrol :DOMain?	FREQuency TIME	FREQ TIME	
Query Limit Line Application Result	\$1 = :CALCulate:LLINe:FAIL?		Pass Fail Result	
Enable Limit Line Application	:CALCulate:LLINe:TESTing [:STATe] @1 \$1 = :CALCulate:LLINe:TESTing [:STATe]?	ON OFF	1 0	
Execute Noise Per Herz	:CALCulate:MARKer#1:FUNCtion @2 \$1 = :CALCulate:MARKer:FUNCtion?	Marker index, NOISe OFF DBUV DBC	NOIS OFF DBUV DBC	
Set Frequency Counter Position	:CALCulate:MARKer:FCOunt :POSition @1 \$1 = :CALCulate:MARKer:FCOunt :POSition?	Frequency	Frequency	
Set Frequency Counter Resolution	:CALCulate:MARKer:FCOunt :RESolution @1 \$1 = :CALCulate:MARKer:FCOunt :RESolution?	Frequency	Frequency	
Query Frequency Counter Measurement	\$1 = :CALCulate:MARKer:FCOunt:X?		Frequency	
Enable Frequency Counter	:CALCulate:MARKer:FCOunt [:STATe] @1 \$1 = :CALCulate:MARKer:FCOunt [:STATe]?	ON OFF	1 0	
Read Noise Measurement	\$1 = :CALCulate:MARKer:FUNCtion :NOISe?		Power per Herz	
Set Noise Per Herz Bandwidth	:CALCulate:MARKer:FUNCtion :NOISe:BANDwidth BWIDth @1 \$1 = :CALCulate:MARKer:FUNCtion :NOISe:BANDwidth BWIDth?	Frequency	Frequency	
Enable Continuous X dB Down	:CALCulate:MARKer:FUNCtion :XDBDown:CONTinuous[:STATe] @1 \$1 = :CALCulate:MARKer:FUNCtion :XDBDown:CONTinuous[:STATe]?	ON OFF	1 0	
Set X dB Down Excursion	:CALCulate:MARKer:FUNCtion :XDBDown:LEVel @1 \$1 = :CALCulate:MARKer:FUNCtion :XDBDown:LEVel?	Relative amplitude	Relative amplitude	
Set X dB Down Display Mode	:CALCulate:MARKer:FUNCtion :XDBDown:MODE @1 \$1 = :CALCulate:MARKer:FUNCtion :XDBDown:MODE?	RELative ABSLeft ABSRight	REL ABSL ABSR	
Enable Marker List Display	:CALCulate:MARKer:TABLe :STATe @1 \$1 = :CALCulate:MARKer:TABLe :STATe?	ON OFF	1 0	

Function description	SCPI command	Parameter	Query reply	Remarks
Enable Signal Track	:CALCulate:MARKer:TRCKing [:STATe] @1 \$1 = :CALCulate:MARKer:TRCKing [:STATe]?	ON OFF	1 0	
Set Marker Persistent Attribute	:CALCulate:MARKer:X:PERSist @1 \$1 = :CALCulate:MARKer:X:PERSist?	INDex VALue	IND VAL	
Enable AM Measurement	:CALCulate:MARKer#1:FUNCtion :AM:STATe @2 \$1=:CALCulate:MARKer#1:FUNCtion :AM:STATe?	Marker index ON OFF	1 0	
Query AM Modulation Depth	:CALCulate:MARKer:FUNCtion :AM[:DEPTh]?		Percent	
Query AM Modulation Frequency	:CALCulate:MARKer:FUNCtion :AM:FREQuency?		Frequency	
Enable FM Measurement	:CALCulate:MARKer#1:FUNCtion :FM:STATe @2 \$1=:CALCulate:MARKer#1:FUNCtion :FM:STATe?	Marker index ON OFF	1 0	
Query FM Deviation	:CALCulate:MARKer:FUNCtion:FM?		Frequency	
Enable Modulation Freq to Sweep Time	:CALCulate:MARKer:FUNCtion :FM:COUPle[:STATe] @1 \$1=:CALCulate:MARKer:FUNCtion :FM:COUPle[:STATe]?	ON OFF	1 0	
Set Modulation Frequency	:CALCulate:MARKer:FUNCtion :FM:COUPle:FREQuency @1 \$1=:CALCulate:MARKer:FUNCtion :FM:COUPle:FREQuency?	Frequency	Frequency	
Enable VSWR Measurement	:CALCulate:MARKer:FUNCtion :VSWR[:STATe] @1 \$1=:CALCulate:MARKer:FUNCtion :VSWR[:STATe]?	ON OFF	1 0	
Query VSWR	:CALCulate:MARKer:FUNCtion :VSWR:RATio?		Real	
Query Return Loss	:CALCulate:MARKer:FUNCtion :VSWR:LOSS?		DB	

6.10.3.2 Subsystem-CALibration

Function description	SCPI command	Parameter	Query reply	Remarks
Get Step Attenuator Calibration Report	:CALibration:ATTenuation \$1 = :CALibration:ATTenuation @1?		Status	
Enable Calibration Correction	:CALibration:CORRection[:STATe] @1 \$1 = :CALibration:CORRection[:STATe]?	ON OFF	1 0	
Select Frequency Reference Source	:CALibration:FREQuency :REFerence @1 \$1 = :CALibration:FREQuency :REFerence?	INTernal EXTernal XTAL	INT EXT XTAL	
Coarse Adjust Internal Frequency Reference	:CALibration:FREQuency:REFerence :COARse @1 \$1 = :CALibration:FREQuency:REFerence :COARse?	8 bit register	8 bit register	
Restore Frequency Reference Adjustment Defaults	:CALibration:FREQuency:REFerence :DEFault			
Fine Adjust Internal Frequency Reference	:CALibration:FREQuency:REFerence :FINE @1 \$1 = :CALibration:FREQuency:REFerence :FINE?	8 bit register	8 bit register	
Set External Frequency Reference	:CALibration:FREQuency:REFerence :FREQuency @1 \$1 = :CALibration:FREQuency:REFerence :FREQuency?	Frequency	Frequency	
Save Frequency Reference Adjustments	:CALibration:FREQuency:REFerence :STORe			
Enable Flatness Correction	:CALibration:FREQuency[:STATe] @1 \$1 = :CALibration:FREQuency[:STATe]?	ON OFF	1 0	
Get Total Gain Calibration Report	:CALibration:GAIN @1 \$1 = :CALibration:GAIN?	RFC1 RFC2	Status	
Get PBW Calibration Report	:CALibration:PBW @1 \$1 = :CALibration:PBW?		Status	
Get RBW Calibration Report	:CALibration:RBW \$1 = :CALibration:RBW?		Status	
Execute Full Calibration	:CALibration[:ALL] @1 :CALibration[:ALL]	RFC1 RFC2		

6.10.3.3 Subsystem-CONFigure

Function description	SCPI command	Parameter	Query reply	Remarks
Get the Current Measurement	\$1 = :CONFigure?		NORM ACP AVP CHP HARM IM OBW SEM SPUR TOTP XDB DBMH DBUH DBCH SG AM FM	
Enable ACP Measurement	:CONFigure:ACPower			
Enable Power Average Measurement	:CONFigure:AVPower			
Enable Channel Power Measurement	:CONFigure:CHPower			
Enable Harmonics Measurement	:CONFigure:HARMonics			
Enable Intermodulation Measurement	:CONFigure:IM			
Disable All Measurements	:CONFigure:NORMal			
Enable Occupied Band Width Measurement	:CONFigure:OBW			
Enable Spectrum Emission Mask Measurement	:CONFigure:SEMask			
Enable Spurious Measurement	:CONFigure:SPURious			
Enable Total Power Measurement	:CONFigure:TOTPower			

6.10.3.4 Subsystem-COUPle

Function description	SCPI command	Parameter	Query reply	Remarks
Enable All Auto Coupling	:COUPle @1 \$1 = :COUPle?	ALL NONE	ALL NONE	

6.10.3.5 Subsystem-DISPlay

Function description	SCPI command	Parameter	Query reply	Remarks
Set Title	:DISPlay:ANNotation:TITLe:DATA @1 \$1 = :DISPlay:ANNota- tion:TITLe:DATA?	String	String	
Preset Dual Channel Viewer	:DISPlay:DUALchannel:PRESet			
Enable Dual Channel Viewer Mode	:DISPlay:DUALchannel:STATe @1 \$1 = :DISPlay:DUALchannel:STATe ?	ON OFF	1 0	
Enable Normalize Correction	:DISPlay:NTData#1[:STATe] @2 \$1 = :DISPlay:NTData#1[:STATe]?	Trace index, ON OFF	1 0	
Set Frequency Offset	:DISPlay:WINDow#1:TRACe :X[:SCALe]:OFFSet @2 \$1 = :DISPlay:WINDow#1:TRACe :X[:SCALe]:OFFSet?	Context index, Frequency	Frequency	

Function description	SCPI command	Parameter	Query reply	Remarks
Enable Frequency Offset	:DISPlay:WINDow#1:TRACe :X[:SCALe]:OFFSet:STATe @2 \$1 = :DISPlay:WINDow#1:TRACe :X[:SCALe]:OFFSet:STATe?	Context index, ON OFF	1 0	
Set Display Line Amplitude	:DISPlay:WINDow#1:TRACe:Y :DLINe @2 \$1 = :DISPlay:WINDow#1:TRACe:Y :DLINe?	Context index, Amplitude	Amplitude	
Enable Display Line	:DISPlay:WINDow#1:TRACe:Y :DLINe:STATe @2 \$1 = :DISPlay:WINDow#1:TRACe:Y :DLINe:STATe?	Context index, ON OFF	1 0	
Set Reference Line Amplitude	:DISPlay:WINDow#1:TRACe :Y[:SCALe]:NRLevel @2 \$1 = :DISPlay:WINDow#1:TRACe :Y[:SCALe]:NRLevel?	Context index, Amplitude	Amplitude	
Enable Reference Line	:DISPlay:WINDow#1:TRACe :Y[:SCALe]:NRLevel:STATe @2 \$1 = :DISPlay:WINDow#1:TRACe :Y[:SCALe]:NRLevel:STATe?	Context index, ON OFF	1 0	
Select Active Context	:DISPlay:WINDow:ACTive @1 \$1 = :DISPlay:WINDow:ACTive?	TOP BOTtom	TOP BOT	
Enable Annotation Display	:DISPlay:WINDow :ANNotation[:ALL] @1 \$1 = :DISPlay:WINDow :ANNotation[:ALL]?	ON OFF	1 0	
Set Measuring Window Position	:DISPlay:ZOOM:FREQuency :CENTer @1 \$1 = :DISPlay:ZOOM:FREQuency :CENTer?	Frequency	Frequency	
Set Measuring Window Width	:DISPlay:ZOOM:FREQuency:SPAN @1 \$1 = :DISPlay:ZOOM:FRE- Quency:SPAN?	Frequency	Frequency	
Select Multiple Screen Mode	:DISPlay:ZOOM:MODE @1 \$1 = :DISPlay:ZOOM:MODE?	OFF ZMFF ZMTT ZMFT	OFF ZMFF ZMTT ZMFT	
Set Frequency versus Time Frequency Position	:DISPlay:ZOOM:TIME:CENTer @1 \$1 = :DISPlay:ZOOM:TIME:CENTer?	Frequency	Frequency	
Set Averaging Count	:DISPlay[:WINDow#1]:TRACe#2 :AVERage:COUNt @3 \$1 = :DISPlay[:WINDow#1]:TRACe#2 :AVERage:COUNt?	Context index, Trace index, Integer	Integer	
Set Trace Calculation Mode	:DISPlay[:WINDow#1]:TRACe#2 :CALCulate:MODE @3 \$1 = :DISPlay[:WINDow#1]:TRACe#2 :CALCulate:MODE?	Context index, Trace index, WRITe MAXHold MAXCont MINHold VideoAVG PowerAVG	WRIT MAXH MAXC MINH VAVG PAVG	

Function description	SCPI command	Parameter	Query reply	Remarks
Select Trace Mode	:DISPlay[:WINDow#1]:TRACe#2 :MODE @3 \$1 = :DISPlay[:WINDow#1]:TRACe#2 :MODE?	Context index, Trace index, WRITe MAXHold MAXCont MINHold VideoAVG PowerAVG VIEW BLANK	WRIT MAXH MAXC MINH VAVG PAVG VIEW BLAN	
Enable Trace Power Average Pause	:DISPlay[:WINDow#1]:TRACe#2 :PAVG:PAUSe @3} \$1 = :DISPlay[:WINDow#1]:TRACe#2 :PAVG:PAUSe?	Context index, Trace index, ON OFF	1 0	
Enable Trace Video Average	:DISPlay[:WINDow#1]:TRACe#2 :PAVG:STATe @3 \$1 = :DISPlay[:WINDow#1]:TRACe#2 :PAVG:STATe?	Context index, Trace index, ON OFF	1 0	
Set Trace Power Average Control Mode	:DISPlay[:WINDow#1]:TRACe#2 :PAVG:TCONrol @3 \$1 = :DISPlay[:WINDow#1]:TRACe#2 :PAVG:TCONrol?	Context index, Trace index, ONCE SLIDe EXPonential	ONCE SLID	
Set Trace Refresh Mode	:DISPlay[:WINDow#1]:TRACe#2 :REFResh:MODE @3 \$1 = :DISPlay[:WINDow#1]:TRACe#2 :REFResh:MODE?	Context index, Trace index, WRITe VIEW BLANk	WRIT VIEW BLAN	
Enable Trace Video Average Pause	:DISPlay[:WINDow#1]:TRACe#2 :VAVG:PAUSe @3 \$1 = :DISPlay[:WINDow#1]:TRACe#2 :VAVG:PAUSe?	Context index, Trace index, ON OFF	1 0	
Enable Trace Video Average	:DISPlay[:WINDow#1]:TRACe#2 :VAVG:STATe @3 \$1 = :DISPlay[:WINDow#1]:TRACe#2 :VAVG:STATe?	Context index, Trace index, ON OFF	1 0	
Set Trace Video Average Control Mode	:DISPlay[:WIN-Dow#1]:TRACe#2:VAVG:TCONrol @3\$1 = :DISPlay[:WIN-Dow#1]:TRACe#2:VAVG:TCONrol?	Context index, Trace index, ONCE SLIDe EXPonential	ONCE SLID	
Select Active Trace	:DISPlay[:WINDow#1]:TRACe :ACTive @2 \$1 = :DISPlay[:WINDow#1]:TRACe :ACTive?	Context index, Trace index	Trace index	
Order Peak in Position or Amplitude Order	:DISPlay[:WINDow#1]:TRACe:MATH :PEAK:SORT @2	Context index, FREQuency AMPLitude		
Set dB per Screen Division	:DISPlay[:WINDow#1]:TRACe :Y[:SCALe]:PDIVision @2 \$1 = :DISPlay[:WINDow#1]:TRACe :Y[:SCALe]:PDIVision?	Context index, Relative amplitude	Relative amplitude	
Set Reference Level	:DISPlay[:WINDow#1]:TRACe :Y[:SCALe]:RLEVel @2 \$1 = :DISPlay[:WINDow#1]:TRACe :Y[:SCALe]:RLEVel?	Context index, Amplitude	Amplitude	

Function description	SCPI command	Parameter	Query reply	Remarks
Set Reference Level Offset	:DISPlay[:WINDow#1]:TRACe :Y[:SCALe]:RLEVel:OFFSet @2 \$1 = :DISPlay[:WINDow#1]:TRACe :Y[:SCALe]:RLEVel:OFFSet?	Context index, Relative amplitude	Relative amplitude	
Enable Reference Level Offset	:DISPlay[:WINDow#1]:TRACe :Y[:SCALe]:RLEVel:OFFSet:STATe @2 \$1 = :DISPlay[:WINDow#1]:TRACe :Y[:SCALe]:RLEVel:OFFSet:STATe?	Context index, ON OFF	1 0	
Set Vertical Scale	:DISPlay[:WINDow#1]:TRACe :Y[:SCALe]:SPACing @2 \$1 = :DISPlay[:WINDow#1]:TRACe :Y[:SCALe]:SPACing?	Context index, LINear LOGarithmic	LIN LOG	
Acquire Trace Normalization Data	:DISPlay[:WINDow]:TRACe#1 :NCORrection:STORe	Trace index		

6.10.3.6 Subsystem-FETch

Function description	SCPI command	Parameter	Query reply	Remark
Fetch ACP results	\$1, {\$2,\$3,\$4,\$5} = :FETch:ACPower?		number of rows {lower channel frequency (Frequency), lower channel amplitude (Amplitude), upper channel frequency (Frequency), upper channel amplitude (Amplitude)}	
Fetch ACP Reference Power	\$1 = :FETch:ACPower:RPOWer?		Amplitude	
Fetch Average Power Measurement	\$1 = :FETch:AVPower?		Amplitude	
Fetch the Channel Power	\$1 = :FETch:CHPower?		Amplitude	
Fetch the Power Spectral Density for Channel Power Measurement	\$1 = :FETch:CHPower:DENSity?		Power per Herz	
Fetch Harmonics Results	\$1, {\$2,\$3,\$4,\$5} = :FETch:HAR- Monics?		number of rows {marker index (Integer), frequency (Frequency), amplitude (Amplitude), amplitude difference (Relative amplitude)}	
Fetch the Intermodulation Results (array)	\$1, {\$2,\$3,\$4,\$5, \$6,\$7,\$8,\$9, \$10} = :FETch:IM?		number of rows {Lower Frequency Marker Index (Integer), Lower Frequency Marker Number (Integer), Lower Frequency Distortion Amplitude (Amplitude), Upper Frequency Marker Index (Integer), Upper Frequency Marker Number (Integer), Upper Frequency Distortion Amplitude (Amplitude), Intermodulation Product (Amplitude), Lower Frequency Test Result (Pass Fail Result), Upper Frequency Test Result (Pass Fail Result)}	
Fetch the Intermodulation Gap	\$1 = :FETch:IM:DELTa?		Frequency	
Fetch the Intermodulation Frequency Reference	\$1 = :FETch:IM:REFerence?		Frequency	

Function description	SCPI command	Parameter	Query reply	Remarks
Fetch OBW Results	\$1, \$2 = :FETch:OBW?		Occupied Bandwidth (Frequency), Frequency Error (Frequency)	
Fetch Spectrum Emission Mask Results	\$1, {\$2,\$3,\$4,\$5, \$6,\$7,\$8} = :FETch:SEMask?		number of rows {channel enabled (1 0), channel start frequency (Frequency), channel stop frequency (Frequency), channel center frequency (max power) (Frequency), absolute power (Amplitude), power relative to the carrier (Relative amplitude), test result (Pass Fail Result)}	
Fetch Spectrum Emission Mask Reference Power	\$1 = :FETch:SEMask:RPOWer?		Amplitude	
Fetch All Spurious Results	\$1, {\$2,\$3,\$4} = :FETch:SPURious:BAND#1 ?	Spurious band index	number of rows {spurious frequency (Frequency), spurious level (Amplitude), test (Pass Fail Result)}	
Fetch Total Power	\$1 = :FETch:TOTPower?		Amplitude	
Fetch Power Spectral Density for Total Power Measurement	\$1 = :FETch:TOTPower:DENSity?		Power per Herz	

6.10.3.7 Subsystem-FORMat

Function description	SCPI command	Parameter	Query reply	Remarks
Set File Format	:FORMat:FILE @1 \$1 = :FORMat:FILE?	BINary XML	BIN XML	
Set Trace Buffer Transfer Format	:FORMat[:TRACe][:DATA] @1 \$1 = :FORMat[:TRACe][:DATA]?	ASCii BINary	ASC BIN	

6.10.3.8 Subsystem-HCOPy

Function description	SCPI command	Parameter	Query reply	Remarks
Set Hard Copy Device	:HCOPy:DEVice:TYPE @1 \$1 = :HCOPy:DEVice:TYPE ?	PRINter USB	PRIN USB	
Copy to the Selected Device	:HCOPy[:IMMediate]			

6.10.3.9 Subsystem-INITiate

Function description	SCPI command	Parameter	Query reply	Remarks
Set Sweep Mode	INITiate:CONTinuous @1 \$1 = :INITiate:CONTinuous?	ON OFF	1 0	
Abort and Restart Sweep	INITiate:RESTart			
Start Sweeping Until Measurement End	:INITiate:SMEAsure			
Execute Sweep to the End	:INITiate:TS			

6.10.3.10 Subsystem-INPut

Function description	SCPI command	Parameter	Query reply	Remarks
Set Input RF Connector	INPut:CONNector @1 \$1 = :INPut:CONNector?	RFC1 RFC2	RFC1 RFC2	

6.10.3.11 Subsystem-MMEMory

Function description	SCPI command	Parameter	Query reply	Remarks
Delete File	:MMEMory:DELete @1	File name		
Enable Saving ACP Configuration	:MMEMory:ITEM:ACP @1 \$1 = :MMEMory:ITEM:ACP?	ON OFF	1 0	
Enable Saving Antenna Correction Table	:MMEMory:ITEM:ANTEnna @1 \$1 = :MMEMory:ITEM:ANTEnna?	ON OFF	1 0	
Enable Saving Channel Table	:MMEMory:ITEM:CHANnel @1 \$1 = :MMEMory:ITEM:CHANnel?	ON OFF	1 0	
Enable Saving General Instrument Setup	:MMEMory:ITEM:CONFig @1 \$1 = :MMEMory:ITEM:CONFig?	ON OFF	1 0	
Enable Saving Limit Lines	:MMEMory:ITEM:LIMit#1 @2 \$1 = :MMEMory:ITEM:LIMit#1?	Limit line index, ON OFF	1 0	
Enable Saving SEM Configuration	:MMEMory:ITEM:SEMask @1 \$1 = :MMEMory:ITEM:SEMask?	ON OFF	1 0	
Enable Saving Spurious Tables	:MMEMory:ITEM:SPURious#1 @2 \$1 = :MMEMory:ITEM:SPURious#1?	Spurious Table Index, ON OFF	1 0	
Enable Saving Trace Data	:MMEMory:ITEM[:WINDow#1] :TRACe#2 @3 \$1 = :MMEMory:ITEM[:WINDow#1] :TRACe#2?	Context index, Trace index, ON OFF	1 0	
Enable Normalize Data	:MMEMory:ITEM[:WINDow#1] :TRACe#2:NRMalize @3 \$1 = :MMEMory:ITEM[:WINDow#1] :TRACe#2:NRMalize?	Context index, Trace index, ON OFF	1 0	
Recall Information from a File	:MMEMory:LOAD:ITEMs @1	File name		
Set File Media	:MMEMory:MEDIA @1 \$1 = :MMEMory:MEDIA?	FLASh USB	FLAS USB	

Function description	SCPI command	Parameter	Query reply	Remarks
Rename File	:MMEMory:MOVE @1, @2	Source filename (String), Destination file- name (String)		
Save File Save File AS	:MMEMory:STORe:ITEMs MMEMory:STORe:ITEMs @1			
Synchronize File to Media	:MMEMory:SYNChronize @1	FLASh USB	FLAS USB	
Enable File Write Protection	:MMEMory:WLOCk[:STATe] @1, @2	File name (String), Write protect enable (ON OFF)		
Get BMP/PNG Screen Image	:MMEMory:DUMP @1?	BMP PNG	Binary stream	
Get Data File	:MMEMory:DATA @1	String (file name)	Binary stream	
Get Screen Image File	:MMEMory:IMAGe @1	String (file name)	Binary stream	

6.10.3.12 Subsystem-OUTPut

Function description	SCPI command	Parameter	Query reply	Remarks
Enable Tracking Generator	:OUTPut[:STATe] @1 \$1 = :OUTPut[:STATe]?	ON OFF	1 0	

6.10.3.13 Subsystem-READ

Function description	SCPI command	Parameter	Query reply	Remarks
Read ACP results	\$1, {\$2,\$3,\$4,\$5} = :READ:ACPower?		number of rows {lower channel frequency (Frequency), lower channel amplitude (Amplitude), upper channel frequency (Frequency), upper channel amplitude (Amplitude)}	
Read ACP Reference Power	\$1 = :READ:ACPower:RPOWer?		Amplitude	
Read Average Power Measurement	\$1 = :READ:AVPower?		Amplitude	
Read the Channel Power	\$1 = :READ:CHPower?		Amplitude	
Read the Power Spectral Density for Channel Power Measurement	\$1 = :READ:CHPower:DENSity?		Power per Herz	
Read Harmonics Results	\$1, {\$2,\$3,\$4,\$5} = :READ:HARMonics?		number of rows {marker index (Integer), frequency (Frequency), amplitude (Amplitude), amplitude difference (Relative amplitude)}	

Function description	SCPI command	Parameter	Query reply	Remark
Read the Intermodulation Results (array)	\$1, {\$2,\$3,\$4,\$5, \$6,\$7,\$8,\$9, \$10} = :READ:IM?		number of rows {Lower Frequency Marker Index (Integer), Lower Frequency Marker Number (Integer), Lower Frequency Distortion Amplitude (Amplitude), Upper Frequency Marker Index (Integer), Upper Frequency Marker Number (Integer), Upper Frequency Distortion Amplitude (Amplitude), Intermodulation Product (Amplitude), Lower Frequency Test Result (Pass Fail Result), Upper Frequency Test Result (Pass Fail Result)}	
Read the Intermodulation Gap	\$1 = :READ:IM:DELTa?		Frequency	
Read the Intermodulation Frequency Reference	\$1 = :READ:IM:REFerence?		Frequency	
Read OBW Results	\$1, \$2 = :READ:OBW?		Occupied Bandwidth (Frequency), Frequency Error (Frequency)	
Read Spectrum Emission Mask Results	\$1, {\$2,\$3,\$4,\$5, \$6,\$7,\$8} = :READ:SEMask?		number of rows {channel enabled (1 0), channel start frequency (Frequency), channel stop frequency (Frequency), channel center frequency (max power) (Frequency), absolute power (Amplitude), power relative to the carrier (Relative amplitude), test result (Pass Fail Result)}	
Read Spectrum Emission Mask Reference Power	\$1 = :READ:SEMask:RPOWer?		Amplitude	
Read All Spurious Results	\$1, {\$2,\$3,\$4} = :READ:SPURious:BAND#1?	Spurious band index	number of rows {spurious frequency (Frequency), spurious level (Amplitude), test (Pass Fail Result)}	
Read Total Power	\$1 = :READ:TOTPower?		Amplitude	
Read Power Spectral Density for Total Power Measurement	\$1 = :READ:TOTPower:DENSity?		Power per Herz	

6.10.3.14 Subsystem-SENSe

Function description	SCPI command	Parameter	Query reply	Remark
Set Averaging Count	[:SENSe#1]:AVERage:COUNt @2 \$1 = [:SENSe#1]:AVERage:COUNt?	Context index, Integer	Integer	
Enable RMS Detector	[:SENSe#1]:AVERage:TYPE @2 \$1 = [:SENSe#1]:AVERage:TYPE?	Context index, RMS VIDeo	RMS VID	
Set EMC Filter	[:SENSe#1]:BANDwidth:EMC @1 \$1 = [:SENSe#1]:BANDwidth:EMC ?	Context index, AUTO W200 W9K W120k W1M	AUTO W200 W9K W120 W1M	
Set EMC Enable	[:SENSe#1]:BANDwidth:EMC :STATe @1 \$1 = [:SENSe#1]:BANDwidth:EMC :STATe ?	Context index, ON OFF	1 0	
Set Video Bandwidth	[:SENSe#1]:BANDwidth:VIDeo @2 \$1 = [:SENSe#1]:BANDwidth:VIDeo?	Context index, Frequency	Frequency	
Enable Video Band Width Auto Coupling	[:SENSe#1]:BANDwidth:VIDeo :AUTO @2 \$1 = [:SENSe#1]:BANDwidth:VIDeo :AUTO?	Context index, ON OFF	1 0	
Set Resolution Band Width	[:SENSe#1]:BANDwidth [:RESolution] @2 \$1 = [:SENSe#1]:BANDwidth [:RESolution]?	Context index, Frequency	Frequency	
Enable Resolution Band Width Auto Coupling	[:SENSe#1]:BANDwidth [:RESolution]:AUTO @2 \$1 = [:SENSe#1]:BANDwidth [:RESolution]:AUTO?	Context index, ON OFF	1 0	
PLL Band Width	[:SENSe]:BANDwidth:PLL @1 \$1 = [:SENSe]:BANDwidth:PLL?	AUTO MEDIum NARRow	AUTO MEDI NARR	
Enable All Auto Coupling - Context Dependent Command	[:SENSe#1]:COUPle @2 \$1 = [:SENSe#1]:COUPle?	Context index, ALL NONE	ALL NONE	
Enable Trace Detector Auto Selection	[:SENSe#1]:DETector#2:AUTO @3 \$1 = [:SENSe#1]:DETector#2:AUTO?	Context index, Trace index, ON OFF	1 0	
Set Trace Detector	[:SENSe#1]:DETector#2 [:FUNCtion] @3 \$1 = [:SENSe#1]:DETector#2 [:FUNCtion]?	Context index, Trace index, NORMal POSitive NEGative SAMPle AVERage QPEak	NORM POS NEG SAMP AVER QPE	
Set Center Frequency	[:SENSe#1]:FREQuency:CENTer @2 \$1 = [:SENSe#1]:FREQuency:CENTer?	Context index, Frequency	Frequency	
Set Center Frequency Step	[:SENSe#1]:FREQuency:CENTer :STEP @2 \$1 = [:SENSe#1]:FREQuency:CENTer :STEP?	Context index, Frequency	Frequency	
Enable Center Frequency Step Auto	[:SENSe#1]:FREQuency:CENTer :STEP:AUTO @2 \$1 = [:SENSe#1]:FREQuency:CENTer :STEP:AUTO?	Context index, ON OFF	1 0	

Function description	SCPI command	Parameter	Query reply	Remar
Set Center Channel	[:SENSe#1]:FREQuency:CHANnel :CENTer @2 \$1 = [:SENSe#1]:FREQuency:CHANnel :CENTer?	Context index, Channel number	Channel number	
Enable Setting Center Frequency as Channel	[:SENSe#1]:FREQuency:CHANnel :CENTer:STATe @2 \$1 = [:SENSe#1]:FREQuency:CHANnel :CENTer:STATe?	Context index, ON OFF	1 0	
Enable Channel Formula	[:SENSe#1]:FREQuency:CHANnel :FORMula#2:STATe @3 \$1 = [:SENSe#1]:FREQuency:CHANnel :FORMula#2:STATe?	Context index, Integer, ON OFF	1 0	
Enable Start Channel Frequency Offset	[:SENSe#1]:FREQuency:CHANnel :OFFSet:STARt:STATe @2 \$1 = [:SENSe#1]:FREQuency:CHANnel :OFFSet:STARt:STATe?	Context index, ON OFF	1 0	
Enable Stop Channel Frequency Offset	[:SENSe#1]:FREQuency:CHANnel :OFFSet:STOP:STATe @2 \$1 = [:SENSe#1]:FREQuency:CHANnel :OFFSet:STOP:STATe?	Context index, ON OFF	1 0	
Set Start Channel	[:SENSe#1]:FREQuency:CHANnel :STARt @2 \$1 = [:SENSe#1]:FREQuency:CHANnel :STARt?	Context index, Channel number	Channel number	
Enable Setting Start Frequency as Channel	[:SENSe#1]:FREQuency:CHANnel :STARt:STATe @2 \$1 = [:SENSe#1]:FREQuency:CHANnel :STARt:STATe?	Context index, ON OFF	1 0	
Set Stop Channel	[:SENSe#1]:FREQuency:CHANnel :STOP @2 \$1 = [:SENSe#1]:FREQuency:CHANnel :STOP?	Context index, Channel number	Channel number	
Enable Setting Stop Frequency as Channel	[:SENSe#1]:FREQuency:CHANnel :STOP:STATe @2 \$1 = [:SENSe#1]:FREQuency:CHANnel :STOP:STATe?	Context index, ON OFF	1 0	
Enable Image Identification Mode	[:SENSe#1]:FREQuency :IMIDentify[:STATe] @2 [:SENSe#1]:FREQuency :IMIDentify[:STATe]?	Context index, ON OFF	1 0	
Enable Image Suppression Mode	[:SENSe#1]:FREQuency :IMSUppression[:STATe] @2 [:SENSe#1]:FREQuency :IMSUppression[:STATe]?	Context index, ON OFF	1 0	
Set Frequency Span	[:SENSe#1]:FREQuency:SPAN @2 \$1 = [:SENSe#1]:FREQuency:SPAN?	Context index, Frequency	Frequency	
Set Span to Full Span	[:SENSe#1]:FREQuency:SPAN:FULL	Context index		
Restore Last Span Setting	[:SENSe#1]:FREQuency:SPAN:PREVious	Context index		
Set Span to Zero Span (Time Domain)	[:SENSe#1]:FREQuency:SPAN:ZERO	Context index		
Set Start Frequency	[:SENSe#1]:FREQuency:STARt @2 \$1 = [:SENSe#1]:FREQuency:STARt?	Context index, Frequency	Frequency	

Function description	SCPI command	Parameter	Query reply	Remarks
Set Stop Frequency	[:SENSe#1]:FREQuency:STOP @2 \$1 = [:SENSe#1]:FREQuency:STOP?	Context index, Frequency	Frequency	
Set Input Attenuation	[:SENSe#1]:POWer[:RF] :ATTenuation @2 \$1 = [:SENSe#1]:POWer[:RF] :ATTenuation?	Context index, Relative amplitude	Relative amplitude	
Enable Attenuation Auto	[:SENSe#1]:POWer[:RF] :ATTenuation:AUTO @2 \$1 = [:SENSe#1]:POWer[:RF] :ATTenuation:AUTO?	Context index, ON OFF	1 0	
Set Minimum Attenuation	[:SENSe#1]:POWer[:RF] :ATTenuation:MINimum @2 \$1 = [:SENSe#1]:POWer[:RF] :ATTenuation:MINimum?	Context index, Relative amplitude	Relative amplitude	
Enable High Sensitivity	[:SENSe#1]:POWer[:RF] :GAIN[:STATe] @2 \$1 = [:SENSe#1]:POWer[:RF] :GAIN[:STATe]?	Context index, ON OFF	1 0	
Set Sweep Time	[:SENSe#1]:SWEep:TIME @2 \$1 = [:SENSe#1]:SWEep:TIME?	Context index, Time	Time	
Enable Sweep Time Auto Coupling	[:SENSe#1]:SWEep:TIME:AUTO @2 \$1 = [:SENSe#1]:SWEep:TIME:AUTO?	Context index, ON OFF	1 0	
Set Window Sweep Enable	[:SENSe#1]:SWEep :WINDow[:STATe] @2 \$1 = [:SENSe#1]:SWEep :WINDow[:STATe] ?	Context index, ON OFF	1 0	
Set ACP Maximum Sweep Count	[:SENSe]:ACPower:AVERage :COUNt @1 \$1 = [:SENSe]:ACPower:AVERage :COUNt?	Integer	Integer	
Set ACP Average Control Mode	[:SENSe]:ACPower:AVERage :TCONrol @1 \$1 = [:SENSe]:ACPower:AVERage :TCONrol?	ONCE SLIDe EXPonential	ONCE SLID	
Enable ACP Averaging	:SENSe]:ACPower:AVERage [:STATe] @1 \$1 = [:SENSe]:ACPower:AVERage [:STATe]?	ON OFF	1 0	
Set ACP Carrier Band Width	[:SENSe]:ACPower :BANDwidth BWIDth:INTegration @1 \$1 = [:SENSe]:ACPower :BANDwidth BWIDth:INTegration?	Frequency	Frequency	
Enable ACP Channel Window Display	[:SENSe]:ACPower:BSWIndow @1 \$1 = [:SENSe]:ACPower:BSWIndow?	FULL CARRier	FULL CARR	
Restore Previous Settings for ACP	[:SENSe]:ACPower:DATA:LOAD			
Save Current Settings for ACP	[:SENSe]:ACPower:DATA:SAVE			
Set Root Nyquist Filter Roll-off Factor (ACP)	[:SENSe]:ACPower:FILTer[:RRC] :ALPHA @1 \$1 = [:SENSe]:ACPower:FILTer[:RRC] :ALPHA?	Number	Number	

Function description	SCPI command	Parameter	Query reply	Remark
Set Root Nyquist Filter Symbol Rate (ACP)	[:SENSe]:ACPower:FILTer[:RRC] :SRATe @1 \$1 = [:SENSe]:ACPower:FILTer[:RRC] :SRATe?	Frequency	Frequency	
Enable Root Nyquist Filter	[:SENSe]:ACPower :FILTer[:RRC][:STATe] @1 \$1 = [:SENSe]:ACPower :FILTer[:RRC][:STATe]?	ON OFF	1 0	
Enable ACP Graph Display	[:SENSe]:ACPower:GRAPh @1 \$1 = [:SENSe]:ACPower:GRAPh?	ON OFF	1 0	
Insert New Channel in ACP Channel Table	[:SENSe]:ACPower:OFFSet:DATA @1	Channel Spacing (Frequency), Channel Width (Frequency)		
Delete ACP Channel Table	[:SENSe]:ACPower:OFFSet:DATA :DELete			
Select ACP Trace	[:SENSe]:ACPower:TRACe @1 \$1 = [:SENSe]:ACPower:TRACe?	Trace index	Trace index	
Set Average Power Maximum Sweep Count	[:SENSe]:AVPower:AVERage :COUNt @1 \$1 = [:SENSe]:AVPower:AVERage :COUNt?	Integer	Integer	
Set Average Power Averaging Control Mode	[:SENSe]:AVPower:AVERage :TCONrol @1 \$1 = [:SENSe]:AVPower:AVERage :TCONrol?	ONCE SLIDe EXPonential	ONCE SLID	
Enable Average Power Averaging	[:SENSe]:AVPower:AVERage [:STATe] @1 \$1 = [:SENSe]:AVPower:AVERage [:STATe]?	ON OFF	1 0	
Restore Power Average Setting	[:SENSe]:AVPower:DATA:LOAD			
Save Current Settings for Power Average	[:SENSe]:AVPower:DATA:SAVE			
Set Power Average Trace	[:SENSe]:AVPower:TRACe @1 \$1 = [:SENSe]:AVPower:TRACe?	Trace index	Trace index	
Set Power Average Range	[:SENSe]:AVPower:WINDow @1 \$1 = [:SENSe]:AVPower:WINDow?	ON OFF	1 0	
Set Measuring Window Position (Average Power)	[:SENSe]:AVPower:WINDow :POSition @1 \$1 = [:SENSe]:AVPower:WINDow :POSition?	Frequency	Frequency	
Set Measuring Window Width (Average Power)	[:SENSe]:AVPower:WINDow :WIDTh @1 \$1 = [:SENSe]:AVPower:WINDow :WIDTh?	Frequency	Frequency	
Set VBW to RBW Ration	[:SENSe]:BANDwidth:VIDeo :RATio @1 \$1 = [:SENSe]:BANDwidth:VIDeo :RATio?	Number	Number	
Enable VBW to RBW ratio Auto	[:SENSe]:BANDwidth:VIDeo:RATio :AUTO @1 \$1 = [:SENSe]:BANDwidth:VIDeo:RATio :AUTO?	ON OFF	1 0	

Function description	SCPI command	Parameter	Query reply	Remarks
Set RBW to SPAN ratio	[:SENSe]:BANDwidth[:RESolution] :RATio @1 \$1 = [:SENSe]:BANDwidth[:RESolution] :RATio?	Number	Number	
Enable RBW to SPAN Ration Auto	[:SENSe]:BANDwidth[:RESolution] :RATio:AUTO @1 \$1 = [:SENSe]:BANDwidth[:RESolution] :RATio:AUTO?	ON OFF	1 0	
Set Channel Power Maximum Sweep Count	[:SENSe]:CHPower:AVERage :COUNt @1 \$1 = [:SENSe]:CHPower:AVERage :COUNt?	Integer	Integer	
Set Channel Power Average Control Mode	[:SENSe]:CHPower:AVERage :TCONrol @1 \$1 = [:SENSe]:CHPower:AVERage :TCONrol?	ONCE SLIDe EXPonential	ONCE SLID	
Enable Channel Power Averaging	[:SENSe]:CHPower:AVERage [:STATe] @1 \$1 = [:SENSe]:CHPower:AVERage [:STATe]?	ON OFF	1 0	
Restore Channel Power Settings	[:SENSe]:CHPower:DATA:LOAD			
Save Current Settings for Channel Power	[:SENSe]:CHPower:DATA:SAVE			
Select Channel Power Trace	[:SENSe]:CHPower:TRACe @1 \$1 = [:SENSe]:CHPower:TRACe?	Trace index	Trace index	
Set Measuring Window Position (Channel Power)	[:SENSe]:CHPower:WINDow :POSition @1 \$1 = [:SENSe]:CHPower:WINDow :POSition?	Frequency	Frequency	
Set Measuring Window Width (Channel Power)	[:SENSe]:CHPower:WINDow :WIDTh @1 \$1 = [:SENSe]:CHPower:WINDow :WIDTh?	Frequency	Frequency	
Insert New Correction Factor Vertex	[:SENSe]:CORRection:CSET:DATA @1	X-coordinate of table point (Frequency), ordinate of table point (Relative amplitude)		
Delete Correction Factor Table	[:SENSe]:CORRection:CSET:DELete			
Enable User Correction Factor	[:SENSe]:CORRection:CSET:STATe @1 \$1 = [:SENSe]:CORRection:CSET:STATe?	ON OFF	1 0	
Set Input Impedance	[:SENSe]:CORRection:IMPedance [:INPut][:MAGNitude] @1 \$1 = [:SENSe]:CORRection:IMPedance [:INPut][:MAGNitude]?	Input impedance	Input impedance	

Function description	SCPI command	Parameter	Query reply	Remarks
Define Channel Formula Parameters	[:SENSe]:FREQuency:CHANnel :FORMula#1 @2	Integer, Minimum Channel (Channel number), Maximum Channel (Channel number), Origin Frequency (Frequency), Channel Spacing (Frequency), Channel Offset (Channel number)		
Select Channel Setting Mode	[:SENSe]:FREQuency:CHANnel :MODE @1 \$1 = [:SENSe]:FREQuency:CHANnel :MODE?	CALCulate TABLe	CALC TABL	
Set Start Channel Frequency Offset	[:SENSe]:FREQuency:CHANnel :OFFSet:STARt @1 \$1 = [:SENSe]:FREQuency:CHANnel :OFFSet:STARt?	Frequency	Frequency	
Set Stop Channel Frequency Offset	[:SENSe]:FREQuency:CHANnel :OFFSet:STOP @1 \$1 = [:SENSe]:FREQuency:CHANnel :OFFSet:STOP?	Frequency	Frequency	
Insert New Channel Into Channel Table	[:SENSe]:FREQuency:CHANnel :TABLe:DATA @1	Channel (Channel number), Frequency (Frequency)		
Delete Channel Table	[:SENSe]:FREQuency:CHANnel :TABLe:DELete			
Query Current Measurement Function	\$1 = [:SENSe]:FUNCtion?		NORM ACP AVP CHP HARM IM OBW SEM SPUR TOTP XDB DBMH DBUH DBCH SG AM FM	
Auto tune	[:SENSe]:TUNE:AUTO			
Peak Zoom	[:SENSe]:FREQuency:SPAN:ZOOM			
Set Harmonics Maximum Sweep Count	[:SENSe]:HARMonics:AVERage :COUNt @1 \$1 = [:SENSe]:HARMonics:AVERage :COUNt?	Integer	Integer	
Set Harmonics Averaging Control Mode	[:SENSe]:HARMonics:AVERage :TCONrol @1 \$1 = [:SENSe]:HARMonics:AVERage :TCONrol?	ONCE SLIDe EXPonential	ONCE SLID	
Enable Harmonics Averaging	[:SENSe]:HARMonics: AVERage[:STATe] @1 \$1 = [:SENSe]:HARMonics: AVERage[:STATe]?	ON OFF	1 0	
Set User Defined Harmonics Fundamental Frequency	[:SENSe]:HARMonics :FUNDamental @1 \$1 = [:SENSe]:HARMonics :FUNDamental?	Frequency	Frequency	

Function description	SCPI command	Parameter	Query reply	Remarks
Enable User Defined Harmonics Fundamental Frequency	[:SENSe]:HARMonics:FUNDamental :STATe @1 \$1 = [:SENSe]:HARMonics:FUNDamental :STATe?	ON OFF	1 0	
Set Harmonics Maximum Order	[:SENSe]:HARMonics:NUMBer @1 \$1 = [:SENSe]:HARMonics:NUMBer?	Integer	Integer	
Set Intermodulation Maximum Sweep Count	[:SENSe]:IM:AVERage:COUNt @1 \$1 = [:SENSe]:IM:AVERage:COUNt?	Integer	Integer	
Set Intermodulation Averaging Control	[:SENSe]:IM:AVERage:TCONrol @1 \$1 = [:SENSe]:IM:AVERage:TCONrol?	ONCE SLIDe EXPonential	ONCE SLID	
Enable Intermodulation Averaging	[:SENSe]:IM:AVERage[:STATe] @1 \$1 = [:SENSe]:IM:AVERage[:STATe]?	ON OFF	1 0	
Restore Intermodulation Settings	[:SENSe]:IM:DATA:LOAD			
Save Current Settings for Intermodulation	[:SENSe]:IM:DATA:SAVE			
Enable Limit Testing for Intermodulation	[:SENSe]:IM:LIM:STATe @1 \$1 = [:SENSe]:IM:LIM:STATe?	ON OFF	1 0	
Set Intermodulation Maximum Order	[:SENSe]:IM:ORDER @1 \$1 = [:SENSe]:IM:ORDER?	Integer	Integer	
Set Intermodulation Limits	[:SENSe]:IM:THReshold#1 @2 \$1 = [:SENSe]:IM:THReshold#1?	Intermodulation order index, Relative amplitude	Relative amplitude	
Set Occupied Band Width Maximum Sweep Count	[:SENSe]:OBWidth:AVERage :COUNt @1 \$1 = [:SENSe]:OBWidth:AVERage :COUNt?	Integer	Integer	
Set Occupied Band Width Averaging Control Mode	[:SENSe]:OBWidth:AVERage :TCONrol @1 \$1 = [:SENSe]:OBWidth:AVERage :TCONrol?	ONCE SLIDe EXPonential	ONCE SLID	
Enable Occupied Band Width Averaging	[:SENSe]:OBWidth:AVERage [:STATe] @1 \$1 = [:SENSe]:OBWidth:AVERage [:STATe]?	ON OFF	1 0	
Restore Occupied Band Width Settings	[:SENSe]:OBWidth:DATA:LOAD			
Save Current Settings for Occupied Band Width	[:SENSe]:OBWidth:DATA:SAVE			
Set Occupied Band Width Percentage	[:SENSe]:OBWidth:PERCent @1 \$1 = [:SENSe]:OBWidth:PERCent?	Percent	Percent	
Select Occupied Band Width Trace	[:SENSe]:OBWidth:TRACe @1 \$1 = [:SENSe]:OBWidth:TRACe?	Trace index	Trace index	
Set Spectrum Emission Mask Maximum Sweep Count	[:SENSe]:SEMask:AVERage :COUNt @1 \$1 = [:SENSe]:SEMask:AVERage :COUNt?	Integer	Integer	
Set Spectrum Emission Mask Averaging Control Mode	[:SENSe]:SEMask:AVERage :TCONrol @1 \$1 = [:SENSe]:SEMask:AVERage :TCONrol?	ONCE SLIDe EXPonential	ONCE SLID	

Function description	SCPI command	Parameter	Query reply	Remarks
Enable Spectrum Emission Mask Averaging	[:SENSe]:SEMask:AVERage [:STATe] @1 \$1 = [:SENSe]:SEMask:AVERage [:STATe]?	ON OFF	1 0	
Set Spectrum Emission Mask Carrier Band Width	[:SENSe]:SEMask :BANDwidth BWIDth @1 \$1 = [:SENSe]:SEMask :BANDwidth BWIDth?	Frequency	Frequency	
Restore Spectrum Emission Mask Settings	[:SENSe]:SEMask:DATA:LOAD			
Save Current Settings for Spectrum Emission Mask	[:SENSe]:SEMask:DATA:SAVE			
Set Root Nyquist Filter Roll-off Factor (SEM)	[:SENSe]:SEMask:FILTer[:RRC] :ALPHA @1 \$1 = [:SENSe]:SEMask:FILTer[:RRC] :ALPHA?	Number	Number	
Set Root Nyquist Filter Symbol Rate (SEM)	[:SENSe]:SEMask:FILTer[:RRC] :SRATe @1 \$1 = [:SENSe]:SEMask:FILTer[:RRC] :SRATe?	Frequency	Frequency	
Enable Root Nyquist Filter (SEM)	[:SENSe]:SEMask:FILTer[:RRC] [:STATe] @1 \$1 = [:SENSe]:SEMask:FILTer [:RRC][:STATe]?	ON OFF	1 0	
Insert New Row into SEM Definition Table	[:SENSe]:SEMask:OFFSet:DATA @1	start frequency (Frequency), stop frequency (Frequency), ibw (Frequency), start absolute limit (Relative amplitude), stop absolute limit (Relative amplitude), start relative limit (Relative amplitude), start relative limit (Relative amplitude), stop relative limit (Relative amplitude), stop relative limit (Relative amplitude), stop relative limit (Relative amplitude), test mode (ABSolute RELative AND OR)		
Delete SEM Definition Table	[:SENSe]:SEMask:OFFSet:DATA:DELete			
Set Reference Power Calculation Mode (SEM)	[:SENSe]:SEMask:RPOWer @1 \$1 = [:SENSe]:SEMask:RPOWer?	CHANnel PEAK	CHAN PEAK	
Select Spectrum Emission Mask Trace	[:SENSe]:SEMask:TRACe @1 \$1 = [:SENSe]:SEMask:TRACe?	Trace index	Trace index	
Set Spurious Active Configuration Table	[:SENSe]:SPURious:LIST:ACTive @1 \$1 = [:SENSe]:SPURious:LIST:ACTive?	Spurious Table Index	Spurious Table Index	

Function description	SCPI command	Parameter	Query reply	Remarks
Insert New Band into Active Spurious Configuration Table	[:SENSe]:SPURious:LIST:DATA @1, @2, @3, @4, @5, @6, @7, @8, @9	Band start frequency (Frequency), Band stop frequency (Frequency), Resolution bandwidth (), Video bandwidth (), Sweep time (), Reference level (Amplitude), Attenuation (), Pre-amplifier (ON OFF), Limit (Amplitude)		
Delete Active Spurious Configuration Table	[:SENSe]:SPURious:LIST:DELete			
Set Number of Points in Trace Buffers	[:SENSe]:SWEep:POINts @1 \$1 = [:SENSe]:SWEep:POINts?	Integer	Integer	
Set Total Power Maximum Sweep Count	[:SENSe]:TOTPower:AVERage :COUNt @1 \$1 = [:SENSe]:TOTPower:AVERage :COUNt?	Integer	Integer	
Set Total Power Averaging Control Mode	[:SENSe]:TOTPower:AVERage :TCONrol @1 \$1 = [:SENSe]:TOTPower:AVERage :TCONrol?	ONCE SLIDe EXPonential	ONCE SLID	
Enable Total Power Averaging	[:SENSe]:TOTPower :AVERage[:STATe] @1 \$1 = [:SENSe]:TOTPower :AVERage[:STATe]?	ON OFF	1 0	
Restore Total Power Settings	[:SENSe]:TOTPower:DATA:LOAD			
Save Current Settings for Total Power	[:SENSe]:TOTPower:DATA:SAVE			
Select Total Power Trace	[:SENSe]:TOTPower:TRACe @1 \$1 = [:SENSe]:TOTPower:TRACe?	Trace index	Trace index	

6.10.3.15 Subsystem-SOURce

Function description	SCPI command	Parameter	Query reply	Remarks
Enable TG Reference Line	:SOURce:CORRection :RLINe[:STATe] @1 \$1 = :SOURce:CORRection :RLINe[:STATe]?	ON OFF	1 0	
Acquire Trace Normalization Data	:SOURce:CORRection:TRACe#1 :CAPTure	Trace index		
Enable TG Normalization Correction	:SOURce:CORRection:TRACe#1 :STATe @2 \$1 = :SOURce:CORRection:TRACe#1 :STATe?	Trace index, ON OFF	1 0	
Set TG Frequency Offset	:SOURce:FREQuency[:OFFSet] @1 \$1 = :SOURce:FREQuency[:OFFSet]?	Frequency	Frequency	
Enable TG Frequency Offset	:SOURce:FREQuency[:OFFSet] :STATe @1 \$1 = :SOURce:FREQuency[:OFFSet] :STATe?	ON OFF	1 0	
Set TG Level Offset	:SOURce:POWer[:LEVel] [:IMMediate]:OFFSet @1 \$1 = :SOURce:POWer[:LEVel] [:IMMediate]:OFFSet?	Relative amplitude	Relative amplitude	
Enable TG Level Offset	:SOURce:POWer[:LEVel] [:IMMediate]:OFFSet:STATe @1 \$1 = :SOURce:POWer[:LEVel] [:IMMediate]:OFFSet:STATe?	ON OFF	1 0	
Set TG Level	:SOURce:POWer[:LEVel] [:IMMediate][:AMPLitude] @1 \$1 = :SOURce:POWer[:LEVel] [:IMMediate][:AMPLitude]?	Amplitude	Amplitude	

6.10.3.16 Subsystem-SYSTem

Function description	SCPI command	Parameter	Query reply	Remarks
Execute Factory Initialization	:SYSTem:FACTory:PRESet			
Execute System Preset	:SYSTem:PRESet			
Enable Menu Refresh	:SYSTem:REFResh:MENU[:STATe] @1 \$1 = :SYSTem:REFResh:MENU[:STATe]	ON OFF	1 0	
Enable Screen Refresh	:SYSTem:REFResh:SCREen[:STATe] @1 \$1 = :SYSTem:REFResh:SCREen[:STATe]	ON OFF	1 0	
Date	:SYSTem:DATE @1, @2, @3	<year>,<month>, <day></day></month></year>		
Time	:SYSTem:TIME @1, @2, @3	<hour>,<minute>,</minute></hour>		

6.10.3.17 Subsystem-TRACe

Function description	SCPI command	Parameter	Query reply	Remarks
Copy Traces	:TRACe:COPY @1, @2	TRACE1 TRACE2 TRACE3, TRACE1 TRACE2 TRACE3		
Set Trace Buffer	:TRACe:DATA @1, @2 \$1 = :TRACe:DATA @1 ?	TRACE1 TRACE2 TRACE3, Binary block {Integer}	Binary Block {Integer}	
Disable Trace Math Operations	:TRACe:MATH:NORMal			
Order Peak in Position or Amplitude Order	:TRACe:MATH:PEAK:SORT @1	FREQuency AMPLitude		
Subtract Traces	:TRACe:MATH:SUBTract @1, @2, @3	TRACE1 TRACE2 TRACE3, TRACE1 TRACE2 TRACE3, TRACE1 TRACE2 TRACE3		
Subtract Display Line To Trace	:TRACe:MATH:SUBTract:DLINe @1	TRACE1 TRACE2 TRACE3		

6.10.3.18 Subsystem-TRIGger

Function description	SCPI command	Parameter	Query reply	Remarks
Set Trigger Delay	:TRIGger#1[:SEQuence]:DELay @2 \$1 = :TRIGger#1[:SEQuence]:DELay?	Context index, Time	Time	
Set External Trigger Level (V)	:TRIGger#1[:SEQuence]:EXTernal :LEVel @2 \$1 = :TRIGger#1[:SEQuence]:EXTernal :LEVel?	Context index, Amplitude	Amplitude	
Set External Trigger Slope	:TRIGger#1[:SEQuence]:EXTernal[1] :SLOPe @2 \$1 = :TRIGger#1[:SEQuence]:EXTernal[1] :SLOPe?	Context index, NEGative POSitive	NEG POS	
Set IF Trigger Level	:TRIGger#1[:SEQuence]:IF:LEVel @2 \$1 = :TRIGger#1[:SEQuence]:IF:LEVel?	Context index, Amplitude	Amplitude	
Set IF Trigger Slope	:TRIGger#1[:SEQuence]:IF:SLOPe @2 \$1 = :TRIGger#1[:SEQuence]:IF:SLOPe?	Context index, NEGative POSitive	NEG POS	
Set Trigger Source	:TRIGger#1[:SEQuence]:SOURce @2 \$1 = :TRIGger#1[:SEQuence]:SOURce?	Context index, IMMediate IF VIDeo EXT	IMM IF VID EXT	
Set Video Trigger Level	:TRIGger#1[:SEQuence]:VIDeo :LEVel @2 \$1 = :TRIGger#1[:SEQuence]:VIDeo :LEVel?	Context index, Amplitude	Amplitude	
Set Video Trigger Slope	:TRIGger#1[:SEQuence]:VIDeo :SLOPe @2} \$1 = :TRIGger#1[:SEQuence]:VIDeo :SLOPe?	Context index, NEGative POSitive	NEG POS	

6.10.3.19 Subsystem-UNIT

I	Function description	SCPI command	Parameter	Query reply	Remarks
	Set Amplitude Units	:UNIT#1:POWer @2 \$1 = :UNIT#1:POWer?	Context index, DBM DBMV DBUV DBUE DBPW V W	DBM DBMV DBUV DBUE DBPW V W	

6.10.3.20 Units

Function	Code
dB	DB
dBm	DBM
dBmV	DBMV
dBμV	DBUV
dBμVemf	DBUE
dBpW	DBPW
Volt	V
milliVolt	MV
microVolt	UV
nanoVolt	NV
Watt	W
milliWatt	MW
Hz	HZ
kHz = 1e3 Hz	KHZ
MHz = 1e6 Hz	MHZ
GHz = 1e9 Hz	GHZ
second	S
millisecond	MS
microsecond	US
ppm	PPM

6.10.4 Example Programs in which SCPI Commands Are Used

6.10.4 Example Programs in which SCPI Commands Are Used

Example 1 Master-resetting this instrument and setting the center frequency

```
Private Sub cmdEx1_Click()
   'Initialization
   Dim spa As Integer
   spa = ildev(0, 8, 0, T10s, 1, 0)
   ilclr (spa)

   ' Reset the instrument, then set center frequency to 30 MHz
   Call ibwrt(spa, "*RST")
   Call ibwrt(spa, ":FREQ:CENT 30 MHZ")
End Sub
```

Example 2 Setting the start frequency to 300 kHz, stop frequency to 800 kHz, and frequency offset to 50 kHz

```
Private Sub cmdEx2_Click()
   'Initialization
   Dim spa As Integer
   spa = ildev(0, 8, 0, T10s, 1, 0)
   ilclr (spa)

   'Set Start Frequency to 300 kHz, Stop Frequency to 800 kHz
   'Set frequency Offset to 50 kHz
   Call ibwrt(spa, ":FREQ:START 300 KHZ;STOP 800 KHZ")
   Call ibwrt(spa, ":DISPLay:WINDow:TRACe:X:OFFSet 50KHZ;OFFSET:STATE ON")
End Sub
```

Example 3 Setting the reference level to 87 dBµV, dB/div to 5 dB, and RBW to 100 kHz

```
Private Sub cmdEx3_Click()
  'Initialization
  Dim spa As Integer
  spa = ildev(0, 8, 0, T10s, 1, 0)
  ilclr (spa)
  ^{\mbox{\scriptsize I}} Set the units to dBUV
 Call ibwrt(spa, ":UNIT:POWER DBUV")
  ' Set the reference level to 87 dBuV
 Call ibwrt(spa, ":DISP:TRACE:Y:RLEVEL 87")
  ' Both commands above have the same effect as:
     call ibwrt(spa,":disp:trace:y:rlevel 87 dbuv")
  ' Set the amplitude per division to 5 db / division
 Call ibwrt(spa, ":DISP:TRACE:Y:PDIV 5 DB")
  ' Set the resolution bandwidth to 100 kHz
 Call ibwrt(spa, ":SENS:BAND:RESOLUTION 100 KHZ")
End Sub
```

6.10.4 Example Programs in which SCPI Commands Are Used

Example 4 Setting the center frequency, frequency span, and attenuator by using variables

```
Private Sub cmdEx4_Click()
   'Initialization
   Dim spa As Integer
   spa = ildev(0, 8, 0, T10s, 1, 0)
   ilclr (spa)

   ' tbxCenter, tbxSpan and tbxAttenuation are 3 text boxes on the form
   ' A user would give a value in MHz to center, span and a value in dB to attenuation
   ' in this example we shall show how to use these
   Call ibwrt(spa, ":FREQ:CENTER " + tbxCenter.Text + " MHZ")
   Call ibwrt(spa, ":FREQ:SPAN " + tbxSpan.Text + " MHZ")
   Call ibwrt(spa, ":POWER:ATT " + tbxAttenuation.Text + " DB")
End Sub
```

Example 5 Saving and recalling the set values

```
Private Sub cmdEx5_Click()
  'Initialization
  Dim spa As Integer
  spa = ildev(0, 8, 0, T10s, 1, 0)
  ilclr (spa)
  ' In this example, we shall setup a few instrument parameters,
  ' set a title, and save these information to a file.
  ^{\mbox{\tiny I}} Execute an instrument preset, then restore the saved configuration
  ' Define the instrument title
  Dim LabelBuff As String
 LabelBuff = "Spectrum Analyzer U37xx"
  ' Set up the instrument
 Call ibwrt(spa, ":FREQ:CENT 30 MHZ")
 Call ibwrt(spa, ":FREQ:SPAN 1 MHZ")
  Call ibwrt(spa, ":DETECTOR POS")
Call ibwrt(spa, ":DISP:ANN:TITLE:DATA """ + LabelBuff + """") ' set the title
  ' Save the data to a file called "SET5"
 Call ibwrt(spa, ":MMEMORY:STORE:ITEMS ""SET5""")
  ' Clear the configuration
 Call ibwrt(spa, "*RST")
  ' Recall the configuration
 Call ibwrt(spa, ":MMEMORY:LOAD:ITEMS ""SET5""")
End Sub
```

6.10.4 Example Programs in which SCPI Commands Are Used

Example 6 Filling limit line table 1 and displaying limit line 1

```
Configuring a Limit Line
Private Sub cmdEx6 Click()
  'Initialization
  Dim spa As Integer
  spa = ildev(0, 8, 0, T10s, 1, 0)
  ilclr (spa)
  ' in this example, we shall use the frequency specific commands
  ' however, it is also possible to select the limit line domain
  ' call ibwrt(spa,":CALC:LLIN:CONT:DOMAIN FREQ")
  ' and to use the genertic commands ":CALC:LLIN:DELETE" and ":CALC:LLIN:DATA"
  ' Clear limit line table 1 (frequency)
 Call ibwrt(spa, ":CALC:LLIN1:DELETE:FREQ")
  ' select dBuV as Amplitude Units
  Call ibwrt(spa, ":UNIT:POWER DBUV")
  ' Fill in the limit line table (1)
 Call ibwrt(spa, ":CALC:LLIN1:DATA:FREQ 25 MHZ, 49.5")
Call ibwrt(spa, ":CALC:LLIN1:DATA:FREQ 35 MHZ, 49.5")
  Call ibwrt(spa, ":CALC:LLIN1:DATA:FREQ 35 MHZ, 51.5")
  Call ibwrt(spa, ":CALC:LLIN1:DATA:FREQ 55 MHZ, 51.5")
  Call ibwrt(spa, ":CALC:LLIN1:DATA:FREQ 55 MHZ, 54.3")
 Call ibwrt(spa, ":CALC:LLIN1:DATA:FREQ 65 MHZ, 54.3")
Call ibwrt(spa, ":CALC:LLIN1:DATA:FREQ 65 MHZ, 57.0")
  Call ibwrt(spa, ":CALC:LLIN1:DATA:FREQ 68 MHZ, 57.0")
  Call ibwrt(spa, ":CALC:LLIN1:DATA:FREQ 68 MHZ, 60.0")
 Call ibwrt(spa, ":CALC:LLIN1:DATA:FREQ 75 MHZ, 60.0")
Call ibwrt(spa, ":CALC:LLIN1:DATA:FREQ 75 MHZ, 62.5")
  Call ibwrt(spa, ":CALC:LLIN1:DATA:FREQ 82 MHZ, 62.5")
 Call ibwrt(spa, ":CALC:LLIN1:DATA:FREQ 82 MHZ, 64.7")
  ' Set up the instrument
  Call ibwrt(spa, ":FREQ:START 0 HZ")
  Call ibwrt(spa, ":FREQ:STOP 100 MHZ")
  ' Display limit line 1
  Call ibwrt(spa, ":CALC:LLIN1:DISPLAY ON")
End Sub
```

Example 7 Reading and displaying the marker level

```
Private Sub cmdEx2_1_Click()
  'Initialization
  Dim spa As Integer
  spa = ildev(0, 8, 0, T10s, 1, 0)
  ilclr (spa)
  ' Reading and displaying the marker level
  'Set up the instrument
  Call ibwrt(spa, ":FREQ:CENT 30 MHZ")
 Call ibwrt(spa, ":FREQ:SPAN 1 MHZ")
  ' Enable marker 1
 Call ibwrt(spa, ":CALC:MARK1:STATE ON")
' Set the marker to 30 MHz
 Call ibwrt(spa, ":CALC:MARK1:x 30 MHZ")
    Call ibwrt(spa, ":SENS:SWEEP:TIME 2 S")
  ' Execute a single-uninterruptible sweep
  Call ibwrt(spa, ":INIT:TS")
  ' Request the marker level read-out and read the answer
  Call ibwrt(spa, ":CALC:MARK1:y ?")
  Dim myBuff As String
 Dim sepa As Integer
 myBuff = Space(30)
 Call ilrd(spa, myBuff, 30)
  sepa = InStr(1, myBuff, vbCrLf)
  txbAnswer.Text = "MarkerLevel " + Left(myBuff, sepa - 1)
```

End Sub

Example 8 Reading trace A data in ASCII format

```
Private Sub cmdAsciiTraceGet Click()
    'Initialization
   Dim spa As Integer
   spa = ildev(0, 8, 0, T10s, 1, 0)
   ilclr (spa)
   Dim i
   Dim trace(1001) As Integer ^{\prime} array to contain the trace points amplitudes
                                ' at the end
   Dim tmp As String
   Dim before As Integer
   Dim after As Integer
   Dim cnt
   Dim buf As String
   buf = Space(1001 * 6)
       ' set the trace transfer format to ASCII
   Call ibwrt(spa, ":FORMAT ASCII")
      ' query trace A (1) amplitudes
   Call ibwrt(spa, ":TRACE:DATA TRACE1 ?")
         ' read trace A buffer ascii points on 5 maximum characters (digits)
         ' separated by a comma
   Call ilrd(spa, buf, 1001 * 6)
   cnt = ibcnt
   i = 1
   before = 1
        ' loop on each point in the buffer
       ' find the next comma separator
       after = InStr(before, buf, ",")
       If after = 0 Then
           tmp = Mid(buf, before)
       Else
           tmp = Mid(buf, before, after - before)
       End If
          ' tmp contains the next point amplitude in ASCII
       trace(i) = CInt(tmp)
       before = after + 1
       i = i + 1
   Loop Until (i > 1001)
End Sub
```

Example 9 Reading trace A data in binary format

```
Private Sub cmdGetBinary Click()
    'Initialization
   Dim spa As Integer
   spa = ildev(0, 8, 0, T10s, 1, 0)
   ilclr (spa)
   Dim buf (1001 * 2 + 5 + 2) As Integer
   Dim cnt As Integer
   Dim tmp As Integer
   Dim ch As String
   Dim size As Integer
   Dim Hsize As Integer
   Dim sSize As String
   Dim word As Integer
   Dim trace(1001) As Integer
       ' set trace A in view mode to guaranty data integrity
   Call ibwrt(spa, ":DISP:TRACE1:MODE VIEW ")
      ' select trace transfer mode as BINARY
   Call ibwrt(spa, ":FORMAT BIN")
       ' read the buffer
   Call ibwrt(spa, ":TRACE:DATA TRACE1 ?")
   Call ilrdi(spa, buf, 1001 * 2 + 5 + 2)
   cnt = ibcnt
    ' interpret the header
   tmp = buf(0) And &HFF&
   ch = Chr(tmp)
   If ch \ll "#" Then Exit Su 'this is incorrect - first character of the
                               'header is a #
   tmp = (buf(0) And &HFF00&) / 256
    Hsize = tmp - Asc("0")
                                ' header size
    sSize = ""
       ' next Hsize characters describe the buffer size in bytes
    For i = 1 To Hsize / 2
       word = buf(i)
       tmp = word And &HFF&
       ch = Chr(tmp)
       sSize = sSize + ch
       tmp = (word And \&HFF00\&) / 256
       ch = Chr(tmp)
        sSize = sSize + ch
   Next.
    'now we know how many bytes the binary buffer contains: size
   size = CInt(sSize)
   Dim offset As Integer
   offset = 2 ' number of integers we have read in the buffer - assuming the
              ' number of bytes is on 4 digits
   For i = 1 To size / 2
           ' loop on each integer and re-interpret the bytes
        word = buf(offset + i)
        trace(i) = (word And &HFF&) * 256 + (word And &HFF00&) / 256
   Next
End Sub
```

Example 10 Entering data to trace A buffer in ASCII format

```
'Initialization
    Dim spa As Integer
    spa = ildev(0, 8, 0, T10s, 1, 0)
    ilclr (spa)
    Dim buf As String
    Dim tracePoint As Integer
    ' set trace A in view mode (otherwise, sent data would be cleared
    ' immediately by the next acquisition)
    Call ibwrt(spa, ":DISP:TRACE1:MODE VIEW")
       ^{\mbox{\tiny I}} select ASCII as the trace transfer format
    Call ibwrt(spa, ":FORMAT ASCII")
       ' build the trace setting command
       ' header first
    buf = ":trace:data trace1 "
                                     'note the ending space. required!
       ' then each point amplitude, separated by a comma
    For i = 0 To 1000
       tracePoint = 7000 + 5000# * Sin(i / 50#)
       Debug.Print tracePoint
       buf = buf + ", " + CStr(tracePoint)
    Next
       ' send the trace setting command
    Call ibwrt(spa, buf)
End Sub
```

Example 11 Outputs a current screen image as bitmap data and writes it to a file.

Data, which is approximately 150 KB for the BMP format or approximately 7 KB for the PNG format, is output.

```
Call ibclr(spa) ' Performs a Device Clear.

Call ibwrt(spa, ":MMEM:DUMP BMP?") ' Requests bitmap data output.

Call ibrdf(spa, "bitmap.bmp") ' Writes bitmap data to a file.
```

Example 12 Writes a screen image that is copied into a USB memory to a file.

7. SPECIFICATIONS

This chapter describes the specifications of this instrument.

The performance of this instrument is guaranteed under the following conditions unless otherwise specified.

- The specified calibration period must be adhered to.
- After turning on the power and warming-up for 5 minutes or more under the specified environmental conditions.
- After automatic calibration has been performed.

Reference data is provided to help you use the product efficiently, but it will not guarantee the performance of this instrument. The data is described by using the following notation.

Specifications (spec.): Indicates the specifications within which the performance of the product can be

guaranteed. Includes variations in the performance of each product, uncertainty

in calibrations, and changes in performance due to the environment.

Typical value (typ.): Indicates the average performance of the product. Excludes variations in the per-

formance of each product, uncertainty in measurements, and changes in perfor-

mance due to the environment.

Nominal value (nom.): Indicates the general performance of the product and does not refer to the guar-

anteed performance.

7.1 U3741 Performance Specifications

7.1 U3741 Performance Specifications

7.1.1 Frequency

Description	Specifications
Frequency range	9 kHz to 3 GHz
Built-in preamp	10 MHz to 3 GHz
Frequency readout accuracy	± (Marker readout × Freq.reference accuracy + SPAN × SPAN accuracy + Residual FM)
Internal frequency reference stability	
Aging rate	$\pm 2 \times 10^{-6}$ / year
Temperature stability	$\pm 2.5 \times 10^{-6} (0^{\circ}\text{C to } 50^{\circ}\text{C})$
Marker frequency counter	RBW < 100 kHz, Signal level S/N > 50 dB, SPAN < 100 MHz
Resolution	1 Hz to 1 kHz
Accuracy	± (Counter readout × Freq.reference accuracy + Residual FM + 1LSB)
Frequency stability	(When the internal frequency reference is used.)
Residual FM	\leq 60 Hz p-p/100 ms
Frequency span	
Range	0, 5 kHz to Full
Accuracy	± 1%
Signal purity (When the internal frequency reference is used.)	-85 dBc/Hz, 10 kHz offset (SPAN < 200 kHz)
Resolution bandwidth (RBW)	
Range	100 Hz to 1 MHz (1, 3 sequence)
Accuracy	±12%
Video bandwidth (VBW)	
Range	10 Hz to 3 MHz (1, 3 sequence)

7.1.2 Sweep

Description	Specifications
Sweep	
Sweep time setting range	
Zero span	50 μs to 1000 s
Spectrum mode	20 ms to 1000 s
Sweep time accuracy	±2% (Zero Span)
Sweep mode	CONTINUOUS, SINGLE, GATE
Trigger function	
Trigger source	Free run, Video, IF, External

7.1.3 Amplitude

Description	Specifications
Amplitude measurement range	+30 dBm to displayed average noise level
Maximum safe input level	
Average continuous power	+30 dBm (Input attenuator ≥ 10 dB) Preamp Off +13 dBm (Input attenuator ≥ 0 dB) Preamp On
DC voltage	±50 VDCmax
Input attenuator range	0 to 50 dB, 10 dB step
Display range	100, 50, 20, 10, 5 dB, Linear
Scale unit	dBm, dBmV, dBμV, dBμVemf, dBpW, W, V
Reference level setting range	
Log scale	-140 dBm to +40 dBm
Detector mode	Normal, Positive Peak, Negative Peak, Sample, RMS, Video Average

7.1.4 Amplitude Accuracy

7.1.4 Amplitude Accuracy

Description	Specifications
Calibration signal accuracy (20 MHz)	
Frequency	20 MHz
Amplitude	-20 dBm
Accuracy	±0.3 dB
Scale display accuracy	
Log	$\pm 0.5 \text{ dB}/10 \text{ dB}$
	±0.5 dB/80 dB
	$\pm 0.2 \text{ dB/1 dB}$
Total level accuracy	(After performing the automatic calibration, Signal level: -10
	dBm to -50 dBm, Preamp Off, Input attenuator: 10 dB, REF = 0
	dBm, Temperature +20°C to +30°C)
	±0.8 dB Frequency range 10 MHz to 3 GHz
	±1.0 dB Frequency range 9 kHz to 3 GHz

7.1.5 Dynamic Range

Description	Specifications
Displayed average noise level	Ref level < -45 dBm RBW = 100 Hz -123 dBm + 2 f (GHz)dB
1 dB gain compression	Frequency range > 20 MHz > -5 dBm Preamp Off > -25 dBm Preamp On
Second harmonic distortion	< -70 dBc (Preamp Off, Mixer input level: -30 dBm, Frequency > 20 MHz)
Third order intermodulation distortion (TOI)	(Frequency range > 20 MHz, Preamp Off, Mixer input level: -20 dBm, Frequency separation: 200 kHz) < -60 dBc
Image responses, Multiple responses, and Out-of-band responses	< -60 dBc, Mixer input level: -20 dBm
Residual responses	(Frequency > 1 MHz, Preamp Off) < -90 dBm

7.1.6 Input and Output

Description	Specifications
RF input	
Connector	Type-N (f) on the front panel
Impedance	50 Ω (nom.)
VSWR	Input attenuator $\geq 10 \text{ dB}$
	< 1.5:1
Calibration signal output	
Connector	BNC (f) on the front panel
Impedance	50 Ω (nom.)
Frequency	20 MHz
Level	-20 dBm
External trigger input	
Connector	BNC (f) on the rear panel
Impedance	$10 \text{ k}\Omega$ (nom.), DC coupling
Trigger level	0 V to 5 V
Frequency reference input	
Connector	BNC (f) on the rear panel
Impedance	50 Ω (nom.)
Frequency [MHz]	1, 1.544, 2.048, 5, 10, 12.8, 13, 13.824, 14.4, 15.36, 15.4, 16.8,
	19.2, 19.44, 19.6608, 19.68, 19.8, 20, 26
Level	0 dBm to +16 dBm
21.4 MHz IF output	
Connector	BNC (f) on the rear panel
Impedance	50 Ω (nom.)
Output level	Approximately mixer input level +10 dB at 20 MHz center frequency
Battery mount	
Connector	Antonbauer QR mount
External DC input	
Connector	XLR-4
Voltage range	11 V to 17 V
GPIB	IEEE-488 bus connector
USB-A	USB1.1 on the front and rear panels
LAN	RJ45 on the rear panel
	10/100Base-T, Protocol TCP/IP
Video out	VGA (15pin f) on the rear panel
Sound out	Small monophonic jack

7.2 U3751 Performance Specifications

7.2 U3751 Performance Specifications

7.2.1 Frequency

Description	Specifications
Frequency range	9 kHz to 8 GHz
Frequency band	9 kHz to 3.1 GHz Band 0 3.0 GHz to 8 GHz Band 1
Built-in preamp	10 MHz to 8 GHz
Frequency readout accuracy	\pm (Marker readout \times Freq.reference accuracy $+$ SPAN \times SPAN accuracy $+$ Residual FM)
Internal frequency reference stability	
Aging rate	$\pm 2 \times 10^{-6}$ / year
Temperature stability	$\pm 2.5 \times 10^{-6} $ (0°C to 50°C)
Marker frequency counter	RBW < 100 kHz, Signal level S/N > 50 dB, SPAN < 100 MHz
Resolution	1 Hz to 1 kHz
Accuracy	± (Counter readout × Freq.reference accuracy + Residual FM + 1LSB)
Frequency stability	(When the internal frequency reference is used.)
Residual FM	\leq 60 Hz p-p/100 ms
Frequency span	
Range	0, 5 kHz to Full
Accuracy	± 1%
Signal purity (When the internal frequency reference is used.)	-85 dBc/Hz, 10 kHz offset (SPAN < 200 kHz)
Resolution bandwidth (RBW)	
Range	100 Hz to 3 MHz (1, 3 sequence)
Accuracy	±12%
Video bandwidth (VBW)	
Range	10 Hz to 3 MHz (1, 3 sequence)

7.2.2 Sweep

Description	Specifications
Sweep	
Sweep time setting range	
Zero span	50 μs to 1000 s
Spectrum mode	20 ms to 1000 s
Sweep time accuracy	±2% (Zero Span)
Sweep mode	REPEAT, SINGLE
Trigger function	
Trigger source	Free run, Video, IF, External

7.2.3 Amplitude

Description	Specifications
Amplitude measurement range	+30 dBm to displayed average noise level
Maximum safe input level	
Average continuous power	+30 dBm (Input attenuator ≥ 10 dB) Preamp Off +13 dBm (Input attenuator ≥ 10 dB) Preamp On
DC voltage	±15 VDCmax
Input attenuator range	0 to 50 dB, 10 dB step
Display range	100, 50, 20, 10, 5 dB, Linear
Scale unit	dBm, dBmV, dBμV, dBμVemf, dBpW, W, V
Reference level setting range	
Log scale	-140 dBm to +40 dBm
Detector mode	Normal, Positive Peak, Negative Peak, Sample, RMS, Video Average

7.2.4 Amplitude Accuracy

7.2.4 Amplitude Accuracy

Description	Specifications
Calibration signal accuracy (20 MHz)	
Frequency	20 MHz
Amplitude	-20 dBm
Accuracy	±0.3 dB
Scale display accuracy	
Log	$\pm 0.5 \text{ dB}/10 \text{ dB}$
	$\pm 0.5 \text{ dB/80 dB}$
	$\pm 0.2 \text{ dB/1 dB}$
Total level accuracy	(After performing the automatic calibration, Image Suppression
	Off, Signal level: -10 dBm to -50 dBm, Preamp Off, Input attenu-
	ator: 10dB, REF = 0 dBm, Temperature 20°C to 30°C)
	±0.8 dB Frequency range 10 MHz to 3.1 GHz
	±1.0 dB Frequency range 3.1 GHz to 8 GHz
	±1.5 dB Frequency range 9 kHz to 10 MHz

7.2.5 Dynamic Range

Description	Specifications
Displayed average noise level	Frequency range 10 MHz to 8 GHz Ref level < -45 dBm RBW = 100 Hz -123 dBm + 2 f (GHz)dB Band 0 Preamp Off -122 dBm + 1 f (GHz)dB Band 1 Preamp Off -138 dBm + 3 f (GHz)dB Band 0 Preamp On -139 dBm + 1.3 f (GHz)dB Band 1 Preamp On
1 dB gain compression	Frequency range 10 MHz to 8 GHz > -8 dBm Preamp Off > -25 dBm Preamp On
Second harmonic distortion	<-70 dBc (Preamp Off, Mixer input level: -40 dBm, Frequency > 200 MHz) <-75 dBc typ (Preamp Off, Mixer input level: -30 dBm, Frequency > 300 MHz)
Third order intermodulation distortion (TOI)	(Frequency range 10 MHz to 8 GHz, Preamp Off, Mixer input level: -20 dBm, Frequency separation: 200 kHz) -50 dBc
Image responses, Multiple responses, and Out-of-band responses	(Image Suppression On) < 60 dBc
Residual responses	(Frequency 10 MHz to 8 GHz) < -80 dBm Preamp Off

7.2.6 Input and Output

Description	Specifications
RF input	
Connector	Type-N (f) on the front panel
Impedance	50 Ω (nom.)
VSWR	Input attenuator ≥ 10 dB
	< 1.7:1 (< 3.0 GHz)
	< 2.0:1 (> 3.0 GHz)
Calibration signal output	
Connector	BNC (f) on the front panel
Impedance	50 Ω (nom.)
Frequency	20 MHz
Level	-20 dBm
External trigger input	
Connector	BNC (f) on the rear panel
Impedance	10 kΩ (nom.), DC coupling
Trigger level	0 V to 5 V
Frequency reference input	
Connector	BNC (f) on the rear panel
Impedance	50 Ω (nom.)
Frequency [MHz]	1, 1.544, 2.048, 5, 10, 12.8, 13, 13.824, 14.4, 15.36, 15.4, 16.8,
	19.2, 19.44, 19.6608, 19.68, 19.8, 20, 26
Level	0 dBm to +16 dBm
21.4 MHz IF output	
Connector	BNC (f) on the rear panel
Impedance	50 Ω (nom.)
Output level	Approximately mixer input level +10 dB at 20 MHz center fre-
	quency
Battery mount	
Connector	Antonbauer QR mount
External DC input	
Connector	XLR-4
Voltage range	11 V to 17 V
GPIB	IEEE-488 bus connector
USB-A	USB1.1 on the front and rear panels
LAN	RJ45 on the rear panel
	10/100Base-T, Protocol TCP/IP
Video out	VGA (15pin f) on the rear panel

7.3 U3771/U3772 Performance Specifications

7.3.1 Frequency

Description	Specifications		
Frequency range [RF Input 1]	9 kHz to 8 GHz: U3771/U3772		
Frequency band	9 kHz to 3.1 GHz: Band 0		
1	3.0 GHz to 8 GHz: Band 1		
Built-in preamp	10 MHz to 8 GHz		
Frequency range [RF Input 2]	10 MHz to 31.8 GHz U3771		
	10 MHz to 43 GHz U3772		
Frequency band	10 MHz to 3.1 GHz Band 0 (N=1)		
	3.0 GHz to 8.0 GHz Band 1 (N=1)		
	7.8 GHz to 14.573 GHz Band 2 (N=2)		
	14.4288 GHz to 28.0 GHz Band 3 (N=4)		
	27.8 GHz to 31.8 GHz Band 4 (N=6) (U3771)		
D 1 .	27.8 GHz to 43.0 GHz Band 4 (N=6) (U3772)		
Frequency readout accuracy	\pm (Marker readout \times Freq.reference accuracy $+$ SPAN \times SPAN accuracy $+$ Residual FM)		
Internal frequency reference stability			
Aging rate	$\pm 2 \times 10^{-6}$ / year		
Temperature stability	$\pm 2.5 \times 10^{-6} $ (0°C to 50°C)		
Marker frequency counter	RBW < 100 kHz, Signal level S/N > 50 dB, SPAN < 100 MHz		
Resolution	1 Hz to 1 kHz		
Accuracy	± (Counter readout × Freq.reference accuracy + Residual FM + 1LSB)		
Frequency stability	(When the internal frequency reference is used.)		
Residual FM	\leq 60 Hz *N p-p/100 ms		
Frequency span	11		
Range	0, 5 kHz to Full		
Accuracy	± 1%		
Signal purity	(-85 + 20logN) dBc/Hz, 10 kHz offset (SPAN < 200 kHz)		
(When the internal frequency reference is			
used.)			
Resolution bandwidth (RBW)			
Range	100 Hz to 3 MHz (1, 3 sequence)		
Accuracy	±12%		
Video bandwidth (VBW)			
Range	10 Hz to 3 MHz (1, 3 sequence)		

7.3.2 Sweep

Description	Specifications
Sweep	
Sweep time setting range	
Zero span	50 μs to 1000 s
Spectrum mode	20 ms to 1000 s
Sweep time accuracy	±2% (Zero Span)
Sweep mode	REPEAT, SINGLE
Trigger function	
Trigger source	Free run, Video, IF, External

7.3.3 Amplitude

Description	Specifications	
Amplitude measurement range		
[RF Input 1]	Noise to +30 dBm	
[RF Input 2]	Noise to +10 dBm	
Maximum safe input level		
[RF Input 1]	+30 dBm (Input attenuator ≥ 10 dB) Preamp Off +13 dBm (Input attenuator = 0 dB) Preamp On	
DC voltage	±15 VDCmax	
[RF Input 2]	+10 dBm (Input attenuator = 0 dB)	
DC voltage	±25 VDCmax	
Input attenuator range		
[RF Input 1]	0 to 50 dB, 10 dB step	
[RF Input 2]	0 to 30 dB, 10 dB step	
Display range	100, 50, 20, 10, 5 dB, Linear	
Scale unit	dBm, dBmV, dBμV, dBμVemf, dBpW, W, V	
Reference level setting range		
[RF Input 1]	-140 dBm to +40 dBm	
[RF Input 2]	-140 dBm to +20 dBm	
Detector mode	Normal, Positive Peak, Negative Peak, Sample, RMS, Video Average	

7.3.4 Amplitude Accuracy

7.3.4 Amplitude Accuracy

Description		Specifications
Calibration signal accuracy (20 MHz)		
Frequency	20 MHz	
Amplitude	-20 dBm	
Accuracy	±0.3 dB	
Scale display accuracy		
Log	±0.5 dB/10 dB ±0.5 dB/80 dB ±0.2 dB/1 dB	
Total level accuracy	Off, Signal level: -1	he automatic calibration, Image Suppression 0 dBm to -50 dBm, Preamp Off, Input attenu-0 dBm, Temperature 20°C to 30°C)
[RF Input 1]	±0.8 dB (Band 0) ±1 dB (Band 1) ±1.5 dB	Frequency 10 MHz to 3.1 GHz Frequency 3.1 GHz to 8 GHz Frequency 9 kHz to 10 MHz
[RF Input 2]	±0.8 dB (Band 0) ±1 dB (Band 1) ±3.0 dB (Band 2) ±3.5 dB (Band 3) ±4.5 dB (Band 4) ±4.5 dB (Band 4)	Frequency 10 MHz to 3.1 GHz Frequency 3.1 GHz to 8 GHz Frequency 7.8 GHz to 14.573 GHz Frequency 14.4288 GHz to 28.0 GHz Frequency 27.8 GHz to 31.8 GHz (U3771) Frequency 27.8 GHz to 43 GHz (U3772)

7.3.5 Dynamic Range

Description	Specifications
Displayed average noise level	Frequency range > 10 MHz Ref level < -45 dBm RBW = 100 Hz
[RF Input 1]	-123 dBm + 2 f (GHz)dB Band 0 Preamplifier Off -122 dBm + 1.2 f (GHz)dB Band 1 Preamplifier Off -138 dBm + 3 f (GHz)dB(TBD) Band 0 Preamplifier On -139 dBm + 1.4 f (GHz)dB Band 1 Preamplifier On
[RF Input 2]	-121 dBm + 2 f (GHz)dB Band 0 -120 dBm + 1.5 f (GHz)dB Band 1 -111 dBm (-118 dBm typ.) Band 2 -109 dBm (-117 dBm typ.) Band 3 -105 dBm (-112 dBm typ.) Band 4
1 dB gain compression	Frequency range > 10 MHz > -8 dBm Preamp Off > -25 dBm Preamp On
Second harmonic distortion	Preamp Off
[RF Input 1]	-70 dBc Mixer input level: -40 dBm, Frequency > 200 MHz <-75 dBc typ Mixer input level: -30 dBm, Frequency > 300 MHz
[RF Input 2]	-40 dBc Mixer input level: -30 dBm, Frequency 300 MHz ~ 31.8 GHz (U3771) 300 MHz ~ 40 GHz (U3772)
Third order intermodulation distortion (TOI)	(Frequency range > 10 MHz, Preamp Off, Mixer input level: -20 dBm, 2-Signal separation:1 MHz) -50 dBc
Image responses, Multiple responses, and Out-of-band responses	(Image Suppression On, Span < 5 GHz) < 60 dBc
Residual responses	(Frequency range > 10 MHz) -80 dBm Preamp Off

7.3.6 Input and Output

7.3.6 Input and Output

Description	Specifications		
RF input 1			
Connector	Type-N (f) on the front panel		
Impedance	50 Ω (nom.)		
VSWR	$< 1.7:1 (< 3.0 \text{ GHz})$ Band 0 Input attenuator $\ge 10 \text{ dB}$		
	$< 2.0:1 (> 3.0 \text{ GHz})$ Band 1 Input attenuator $\ge 10 \text{ dB}$		
RF input 2			
Connector	Type-K (f) on the front panel		
Impedance	50 Ω (nom.)		
VSWR	1.7:1 (typ.) Band 0 Input attenuator \geq 10 dB		
	$2.0:1$ (typ.) Band 1, Band 2, Band 3, Input attenuator ≥ 10 dB		
	2.5 : 1 (typ.) Band 4 Input attenuator ≥ 10 dB		
Calibration signal output			
Connector	BNC (f) on the front panel		
Impedance	50 Ω (nom.)		
Frequency	20 MHz		
Level	-20 dBm		
External trigger input			
Connector	BNC (f) on the rear panel		
Impedance	$10 \text{ k}\Omega$ (nom.), DC coupling		
Trigger level	0 V to 5 V		
Frequency reference input			
Connector	BNC (f) on the rear panel		
Impedance	50 Ω (nom.)		
Frequency [MHz]	1, 1.544, 2.048, 5, 10, 12.8, 13, 13.824, 14.4, 15.36, 15.4, 16.8,		
	19.2, 19.44, 19.6608, 19.68, 19.8, 20, 26		
Amplitude	0 dBm to +16 dBm		
21.4 MHz IF output			
Connector	BNC (f) on the rear panel		
Impedance	$50 \Omega \text{ (nom.)}$		
Output level	Approximately mixer input level +10 dB at 20 MHz center fre-		
	quency		
Battery mount			
Connector	Antonbauer QR mount		
External DC input			
Connector	XLR-4		
Voltage range	11 V to 17 V		
GPIB	IEEE-488 bus connector		
USB-A	USB1.1 on the front and rear panels		
LAN	RJ45 on the rear panel		
	10/100Base-T, Protocol TCP/IP		
Video out	VGA (15pin f) on the rear panel		

7.4 General Specifications

Description	Specifications		
Operation environment	Ambient temperature: 0°C to +50°C Relative humidity: 85% or less (no condensation)		
Storage environmental range	Ambient temperature: -20°C to +60°C Relative humidity: 85% or less (no condensation)		
AC Power supply input	AC100 V to 120 V, 50 Hz/60 Hz AC220 V to 240 V, 50 Hz/60 Hz (Automatically switches the input voltage between 100 V AC and 220 V AC.)		
DC Power input	DC +11 V to +17 V		
Power consumption	100 VA or less For the AC power supply 70 W or less For the DC power supply		
Dimensions	Approximately 308 mm (W) \times 175 mm (H) \times 209 mm (D) Approximately 337 mm (W) \times 190 mm (H) \times 307 mm (D) (Including the handle and feet)		
Mass	Approximately 5.0 kg or less (without option) U3741 Approximately 5.6 kg or less (without option) U3751 Approximately 6 kg or less (without option) U3771/U3772		

7.5 Options

7.5 Options

7.5.1 Option 10 2-Channel Input

Item	Description
Frequency	Conforms to the U3741 standard specifications.
Sweep	Applied to RF INPUT2 (channel 2)
Amplitude range	
Amplitude accuracy	
Dynamic range	

• Differences from U3741/U3751 input output standard specifications

Item	Description	
Crosstalk between input channels	< -90 dBc (Input level -10 dBm, Input attenuator 0 dB)	
RF input 2		
Connector	N type female	
Impedance	50 Ω (nom.)	
VSWR	<1.5 : 1 Input attenuator > 10 dB	
External trigger input	Can be selected as the trigger input of RF input 2 when OPT10 is installed. The input connector is a single line only.	
21.4 MHz IF output	When OPT10 is installed, it is only the IF output which corresponds to RF input 1.	

• Differences from U3771/U3772 standard specifications

Item			Description
Frequency range [RF INPUT 1]	10 MHz - 31.8 GHz (U3771)		
	10 MHz - 43 GHz	z (U3772)	
Crosstalk between input channels	< -90 dBc (Input l	level -10 dBr	n, Input attenuator 0 dB)
RF input 1			
Connector	K type female		
Impedance	50 Ω (nom.)		
VSWR	1.7:1 (typ.)	Band 0	Input attenuator ≥ 10 dB
	2.0 : 1 (typ.)	Band 1, Bar	nd 2, Band 3 Input attenuator ≥ 10 dB
	2.5 : 1 (typ.)	Band 4	Input attenuator ≥ 10 dB
RF input 2			
Connector	N type female		
Impedance	50 Ω (nom.)		
VSWR	<1.5:1	Input attenu	ator > 10 dB
External trigger input	Can be selected as the trigger input of RF input 2 when OPT10 is installed. The input connector is a single line only.		
21.4 MHz IF output	When OPT10 is in	nstalled, it is	only the IF output which corresponds to RF input 1.

7.5.2 Option 11 75 Ω 2-Channel Input (Can be Installed only in the U3741)

7.5.2 Option 11 75 Ω 2-Channel Input (Can be Installed only in the U3741)

Item	Description
Frequency	Conforms to the specifications given when U3741 is equipped with OPT15.
Sweep	
Amplitude range	
Amplitude accuracy	
Dynamic range	

• Difference with the standard specifications

Item	Description
Crosstalk between input channels	< -90 dBc (Input level -10 dBm, Input attenuator 0 dB)
RF input 2	
Connector	N type female
Impedance	75 Ω (nom.)
VSWR	<1.6:1 Input attenuator > 10 dB
External trigger input	Can be selected as the trigger input of RF input 2 when OPT11 is installed. The input connector is a single line only.
21.4 MHz IF output	When OPT11 is installed, it is only the IF output which corresponds to RF input 1.

7.5.3 Option 15 75 Ω Input

7.5.3 Option 15 75 Ω Input

• Frequency

Description	Specifications
Frequency range	9 kHz to 2.2 GHz
Built-in preamp	10 MHz to 2.2 GHz
Tunable frequency	9 kHz to 3 GHz

• Amplitude

Description	Specifications	
Amplitude measurement range	+134 dBµV to displayed average noise level	
Maximum safe input level	Input attenuator ≥ 10 dB	
Average continuous power	+134 dBμV Preamp Off +120 dBμV Preamp On	
DC voltage	±50 VDCmax	
Input attenuator range	0 to 50 dB, 10 dB step	
Display range	100, 50, 20, 10, 5 dB, Linear	
Scale unit	dBm, dBmV, dBμV, dBμVemf, dBpW, W, V	
Reference level setting range		
Log scale	$-31.2~dB\mu V$ to $+148.8~dB\mu V$	
Detector mode	Normal, Positive Peak, Negative Peak, Sample, RMS, Video Average	

Amplitude Accuracy

Description	Specifications	
Calibration signal accuracy (20 MHz)		
Frequency	20 MHz	
Amplitude	-20 dBm	
Accuracy	±0.4 dB	
Scale display accuracy		
Log	±0.5 dB/10 dB	
	$\pm 0.5 \text{ dB/80 dB}$	
	±0.2 dB/1 dB	
Total level accuracy	(After performing the automatic calibration, Signal level: +98.8	
	dBμV to +58.8 dBμV, Preamp Off, Input attenuator: 10 dB, REF	
	= $+108.8 \text{ dB}\mu\text{V}$, Temperature $+20^{\circ}\text{C}$ to $+30^{\circ}\text{C}$)	
	±0.9 dB Frequency range 10 MHz to 2.2 GHz	
	±2.1 dB Frequency range 9 kHz to 2.2 GHz	

7.5.4 Option 20 High Stability Frequency Reference

• Dynamic Range

Description	Specifications	
Displayed average noise level	Ref level $< +63.8 \text{ dB}\mu\text{V RBW} = 100 \text{ Hz}$ -12 dB μV + 2 f (GHz)dB Preamp Off	
	$-27 \text{ dB}\mu\text{V} + 3 \text{ f (GHz)}\text{dB}$ Preamp On	
1 dB gain compression	$\begin{array}{ll} Frequency\ range > 20\ MHz \\ > +102\ dB\mu V & Preamp\ Off \\ > +82\ dB\mu V & Preamp\ On \end{array}$	
Second garmonic distortion	< -70 dBc (Preamp Off, Mixer input level: +77 dBμV, Frequency > 20 MHz)	
Third order intermodulation distortion (TOI)	(Frequency range > 10 MHz, Preamp Off, Mixer input level: +88.8 dBμV, Frequency separation: 200 kHz) < -60 dBc	
Image responses, Multiple responses, and Out-of-band responses	< -60 dBc, Mixer input level: +88.8 dBμV	
Residual responses	(Frequency > 1 MHz, Preamp Off) < +21 dBμV	

• Input and Output

Description	Specifications
RF input	
Connector	Type-N (f) on the front panel
Impedance	75 Ω (nom.)
VSWR	Input attenuator ≥ 10 dB
	< 1.6:1
Calibration signal output	
Connector	BNC (f) on the front panel
Impedance	75 Ω (nom.)
Frequency	20 MHz
Level	-20 dBm

7.5.4 Option 20 High Stability Frequency Reference

Description	Specifications
Reference frequency stability	
Aging rate	$\pm 2 \times 10^{-8}$ / day, $\pm 1 \times 10^{-7}$ / year
Warm-up drift (nominal)	$\pm 5 \times 10^{-8}$ (± 25 °C, 10 minutes after turning the power on)
Temperature drift	$\pm 5 \times 10^{-8}$ (0 to +40°C, with reference to +25°C)

7.5.5 Option 28 EMC Filter

7.5.5 Option 28 EMC Filter

Description	Specifications
6 dB bandwidth	
Range	200 Hz, 9 kHz, 120 kHz, 1 MHz
Accuracy	< ±10%
Detector mode	Normal, Positive peak, Negative peak, Sample, RMS, Video aver-
	age, QP

7.5.6 Option 53 Time Domain Analysis Option 54 2-Channel Time Domain Analysis

• Time domain waveform capture

Item	Description
RF frequency range	Conforms to the frequency range for each model of the U3700 series.
RF amplitude range	Noise level to +30 dBm (*1)
Waveform capture format	I/Q vector time waveform
Measurement bandwidth (BW)	100 Hz to 3 MHz (1 to 3 steps)
I/Q sampling rate	713 Hz (BW 100 Hz) to 21.4 MHz (BW 3 MHz)
I/Q waveform capture time	49 msec (BW 3 MHz) to 1000 sec (BW 100 Hz)
Number of I/Q waveform capture samples	1M Samples (I/Q)

^(*1) The noise level conforms to the dynamic range specifications for each model of the U3700 series.

7.5.7 Option 55 Wide Band Time Domain Analysis Option 56 2-Channel Wide Band Time Domain Analysis

7.5.7 Option 55 Wide Band Time Domain Analysis Option 56 2-Channel Wide Band Time Domain Analysis

• Time domain waveform capture

Item	Description
RF frequency range	Conforms to the frequency range for each model of the U3700 series.
RF amplitude range	Noise level to +30 dBm (*1)
Waveform capture format	I/Q vector time waveform
Measurement bandwidth (BW)	100 Hz to 30 MHz (1 to 3 steps), 40 MHz
I/Q sampling rate	500 Hz (BW 100 Hz) to 65 MHz (BW 40 MHz)
I/Q waveform capture time	120 msec (BW 40 MHz) to 1000 sec (BW 100 Hz)
Number of I/Q waveform capture samples	8 M Samples (I/Q)

^(*1) The noise level conforms to the dynamic range specifications for each model of the U3700 series.

7.5.8 Option 70 High C/N Option 71 2-Channel High C/N

1. U3741

• Frequency

Description	Specifications
Frequency span	
Range	0, 1 kHz to Full
Accuracy	± 1%
Signal purity	-98 dBc/Hz, 10 kHz offset (SPAN < 1 MHz)
(When the internal frequency reference is	
used.)	
Resolution bandwidth (RBW)	
Range	30 Hz to 1 MHz (1, 3 sequence)
Accuracy	±12%

• Dynamic Range

Description	Sp	pecifications
Displayed average noise level	Frequency range > 10 MHz, -126 dBm + 2 f (GHz)dB -126 dBm + 2.5 f (GHz)dB	1
	-141 dBm + 3 f (GHz)dB	Preamp On

7.5.8 Option 70 High C/N Option 71 2-Channel High C/N

2. U3751

• Frequency

Description	Specifications
Frequency span	
Range	0, 1 kHz to Full
Accuracy	± 1%
Signal purity	-98 dBc/Hz, 10 kHz offset (SPAN < 1 MHz)
(When the internal frequency reference is	
used.)	
Resolution bandwidth (RBW)	
Range	30 Hz to 3 MHz (1, 3 sequence)
Accuracy	±12%

• Dynamic Range

Description	Specifications
Displayed average noise level	Frequency range > 10 MHz Ref level < -45 dBm RBW = 30 Hz
	-126 dBm + 2 f (GHz)dB Band 0 Preamp Off -125 dBm + 1 f (GHz)dB Band 1 Preamp Off
	-141 dBm + 3 f (GHz)dB Band 0 Preamp On -142 dBm + 1.3 f (GHz)dB Band 1 Preamp On

3. U3771/U3772

• Frequency

Description	Specifications
Frequency span	
Range	0, 1 kHz to Full
Accuracy	± 1%
Signal purity	(-98 + 20logN) dBc/Hz, 10 kHz offset (SPAN < 1 MHz)
(When the internal frequency reference is	
used.)	
Resolution bandwidth (RBW)	
Range	30 Hz to 3 MHz (1, 3 sequence)
Accuracy	±12%

7.5.9 Option 75 75 Ω Tracking Generator

• Dynamic Range

Description	Specifi	ications	
Displayed average noise level	Frequency range > 10 MHz Ref level < -45 dBm RBW = 30 Hz		
[RF Input 1]	-125 dBm + 1.2 f (GHz)dB -141 dBm + 3 f (GHz)dB(TBD)	Band 0 Band 1 Band 0 Band 1	Preamplifier Off Preamplifier Off Preamplifier On Preamplifier On
[RF Input 2]	-123 dBm + 1.5 f (GHz)dB -114 dBm -112 dBm	Band 0 Band 1 Band 2 Band 3 Band 4	

7.5.9 Option 75 75 Ω Tracking Generator

Description	Specifications	
Frequency range	100 kHz to 2.2 GHz	
Frequency offset		
Range	0 to 1 GHz	
Resolution	1 kHz	
Accuracy	±300 Hz	
Output level range	+107 to +47 dBμV	0.5 dB step
Output level accuracy	±0.5 dB	20 MHz, +97 dBμV, +20°C to +30°C
Output level flatness	Reference signal level: +97 dBμV, Frequency: 20 MHz ±1.0 dB (1 MHz to 1 GHz) ±1.5 dB (100 kHz to 2.2 GHz)	
Output level switching uncertainty	Reference level: +97 dBμV ±1.0 dB (1 MHz to 1 GHz) +107 to +47 dBμV ±2.0 dB (1 MHz to 2.2 GHz) +107 to +47 dBμV ±3.0 dB (100 kHz to 2.2 GHz)+107 to +77 dBμV Frequency Offset OFF ±4.0 dB (100 kHz to 2.2 GHz)+77 to +47 dBμV Frequency Offset OFF ±5.0 dB (100 kHz to 2.2 GHz)+107 to +47 dBμV Frequency Offset ON	
Spurious output	Output level: +97 dBμV	
Harmonics	≤ -15 dBc ≤ -20 dBc	(100 kHz to 1 MHz) (1 MHz to 2.2 GHz)
Non-harmonics	≤ -20 dBc	Frequency Offset OFF
TG leakage	≤+39 dBμV	Input attenuator: 0 dB
Output impedance	75 Ω (nom.)	
VSWR	≤ 2 (typ.)	Output level ≤ +97 dBμV
Maximum allowable input	+117 dBμV, ±10 V	

7.5.10 Option 76 Tracking Generator

7.5.10 Option 76 Tracking Generator

Description	Specifications		
Frequency range	100 kHz to 3 GHz		
Frequency offset			
Range	0 to 1 GHz		
Resolution	1 kHz		
Accuracy	±300 Hz		
Output level range	0 to -60 dBm	0.5 dB step	
Output level accuracy	±0.5 dB	20 MHz, -10 dBm, +20°C	to +30°C
Output level flatness	Reference signal level: -10 dBm, Frequency: 20 MHz ±1.0 dB (1 MHz to 1 GHz) ±1.5 dB (100 kHz to 3 GHz)		
Output level switching uncertainty	Reference level: -10 dBm ±1.0 dB (1 MHz to 1 GHz) 0 to -60 dBm ±2.0 dB (1 MHz to 2.6 GHz) 0 to -60 dBm ±3.0 dB (100 kHz to 3 GHz) 0 to -30 dBm Frequency Offset OFF ±4.0 dB (100 kHz to 3 GHz) -30.5 to -60 dBm Frequency Offset OFF ±5.0 dB (100 kHz to 3 GHz) 0 to -60 dBm Frequency Offset ON		
Spurious output	Output level: -10 dBm		
Harmonics	≤ -15 dBc ≤ -20 dBc	(100 kHz to 1 MHz) (1 MHz to 3 GHz)	
Non-harmonics	≤ -20 dBc	Frequency Offset OFF	
TG leakage	≤ -80 dBm	Input attenuator: 0 dB	
Output impedance	50 Ω (nom.)		
VSWR	≤ 2 (typ.)	Output level ≤ -10 dBm	
Maximum allowable input	+10 dBm, ±10 V		

7.5.11 Option 77 6 GHz Tracking Generator

7.5.11 Option 77 6 GHz Tracking Generator

Item	Description	
Frequency range	100 kHz to 6 GHz	
Output level range	0 to -30 dBm (0.5 dB step)	
Output level accuracy	≤ ± 0.5dB 20MHz, -10 dBm, +20°C to +30°C	
Output level flatness	-10 dBm, +20°C to +30°C based on 20 MHz, -10 dBm.	
	$\leq \pm 1$ dB (1 MHz to 1 GHz)	
	$\leq \pm 1.5 \text{ dB } (100 \text{ kHz to } 3.1 \text{ GHz})$	
	\leq ± 2.0 dB (100 kHz to 6 GHz)	
TG leakage	≤ -80 dBm (Input attenuator 0 dB)	
Output impedance	50 Ω (nom.)	
VSWR	\leq 2 (typ.) Output level \leq -10 dBm	
Maximum allowable applied level	$+10 \text{ dBm} \pm 10 \text{ V DC}$	

8. OPTIONS AND ACCESSORIES

This chapter describes the options and accessories for this instrument.

8.1 Options

Table 8-1 Options

Option	Description	Note
OPT10	2-channel input option	
OPT11	2-channel input option 75 Ω	For U3741 only
OPT15	75 Ω input	For U3741 only
OPT20	High stability frequency reference	
OPT28	EMC filter	
OPT53	Time domain analysis option	
OPT54	2-channel time domain analysis option	
OPT55	Wide Band time domain analysis option	
OPT56	2-channel Wide Band time domain analysis option	
OPT70	High C/N	
OPT71	2-channel High C/N	
OPT75	Tracking generator 75 Ω	For U3741 only
OPT76	Tracking generator	
OPT77	6 GHz tracking generator U3751, U3771, and U	

8.2 Accessories

8.2 Accessories

Table 8-2 Accessories

Name	Product Code
$50 \Omega / 75 \Omega$ converter	ZT-130NC
DC cable	A114020
Battery pack	A870008
Battery charger	A870009
Carrying bag	A129001
Transit case	A129002
Rack mount kit (JIS)	A122003
Rack mount kit (EIA)	A124004
Highpass filter (2.8 GHz to 18 GHz)	A899001
Highpass filter (8 GHz to 18 GHz)	A899002
Highpass filter (11 GHz to 26 GHz)	A899003
Highpass filter (18 GHz to 30 GHz)	A899004
VSWR bridge	A199001

9. MAINTENANCE

This chapter describes the following matters related to the maintenance of this instrument in order to maintain its designed performance.

- 9.1 Cleaning
- 9.2 About Calibration
- 9.3 About Replacement of Limited-Life Parts
- 9.4 Method of Storing the Instrument
- 9.5 Transportation
- 9.6 Notes for Requesting Repair, Replacement of Parts, and Periodic Calibration
- 9.7 List of Error Messages
- 9.8 In Case of Difficulty
- 9.9 Product Disposal and Recycle

9.1 Cleaning

This section describes how to clean this instrument and some matters to note.

WARNING:

Turn off the power breaker on the rear panel and extract the power cable from the wall socket to protect yourself from electric shock accidents.

Never attempt to remove the cabinet cover to clean the inside of the instrument.

9.1.1 Cabinet Cleaning

Use the following procedure to clean the cabinet of this instrument.

Clean the cabinet surface with a soft dry cloth.

If the surface is not clean enough, try again with a cloth soaked in a weakened neutral detergent. Then wipe the surface with a soft dry cloth.

CAUTION:

Do not allow water to splash into the inside of the instrument.

Do not use an organic solvent such as benzene, toluene, xylene, or acetone and the cleanser for cleaning. They can cause the paint on the cabinet to come off, deform, or degrade.

9.1.2 Cleaning of Other Parts

9.1.2 Cleaning of Other Parts

Use appropriate caution to protect this instrument from dust.

WARNING: Remove dust periodically from wall sockets and power connector plugs.

Dust that is wet with humidity may cause tracking that could cause a fire.

The rear panel is equipped with an exhaust cooling fan and the side and the bottom panels have exhaust vents. Keep these vents clean for sufficient exhaustion. If dust piled on the vents causes exhaustion to become poor, the temperature inside will rise and the instrument will not work correctly.

9.2 About Calibration

Calibration should be performed periodically to prevent performance deterioration or to adjust chronological performance changes.

The recommended period of regular calibration is once a year.

Calibration is done at the factory site.

For more information, call a sales representative.

9.3 About Replacement of Limited-Life Parts

Table 9-1 lists the proper limited-life parts of this instrument.

The table also shows the number of operations for the expected life spans of each of these parts, to suggest a recommended time of replacement in terms of the number of times of operations. For replacement, call the Service Center (Advantest Customer Support (ACS)).

Note that the life span can become shorter than expected depending on the operation environment, frequency of use, and storage environment.

MEMO: The table shows the expected life spans or recommended time of replacement only for the user's reference. It does not guarantee the life of the components.

Table 9-1 Limited-Life Parts

Name	Life (Reference values)
Panel key switch	10 ⁶ operations
Key switch with LED	10 ⁵ operations
LCD back light	50,000 hours
Rotary encoder	25×10^6 operations
Cooling fan	40,000 hours
Lithium battery cells for data backup	About 3 years
Mechanical relay (For EXT. DC)	10 ⁵ operations
Mechanical relay (For input attenuator)	10 ⁶ operations
Coaxial relay (For RF1 or RF2)	10 ⁶ operations

9.4 Method of Storing the Instrument

9.4 Method of Storing the Instrument

When you store this instrument, keep it in an environment that meets the following requirements.

- Reduced vibration
- Not dusty
- Protected from direct sunlight
- Ambient temperature range: -20°C to +60°C
- Relative humidity: 30% to 85%

When you do not use the instrument for 90 days or more, store it in an appropriate moisture-proof bag with desiccant.

9.5 Transportation

For transportation, use the packing materials used for the shipping of this instrument. If you use other materials, pack the instrument using the following procedure.

- 1. Install the protection cover of the touch screen display on this instrument.
- 2. Cover the instrument with a protective plastic sheet. (Put desiccant inside for protection from moisture.)
- 3. Prepare a carton case.
 - The panels of the case must be 5 mm or more thick. The inner dimensions must be 10 cm or more larger than the physical size of this instrument because cushioning materials are placed inside. Place the instrument so that it is covered with cushioning or plastic foam material on all sides. (The cushioning material must be 4 cm or more thick.)
- 4. Seal the carton case with an industrial stapler or packing tape.

9.6 Notes for Requesting Repair, Replacement of Parts, and Periodic Calibration

9.6.1 Work Request

Attach a tag indicating the following data to this instrument when you send it to a sales representative.

- Your company name and address
- Name of the person in charge
- Serial number (on the rear panel)
- What work to request (repair or periodic calibration)

9.6.2 Destination and Phone Number for Contact

Call Advantest MS (Measuring Instruments) Call Center.

9.7 List of Error Messages

9.7 List of Error Messages

This section describes error messages which are displayed because of function restrictions or errors in operation of this instrument.

Error code	Type	Displayed Message
0/2	WARNING	Some formula parameters are out of range. The system has adjusted automatically the value.
0/3	WARNING	Some channel table parameters are out of range. The system has adjusted automatically the value.
0/4	WARNING	Some limit line table parameters are out of range. The system has adjusted automatically the value.
0/5	WARNING	The table is full. Impossible to insert a new item.
0/7	WARNING	No formula for this channel number.
0/8	WARNING	Channel number not in table.
0/12	WARNING	The pass fail table is empty.
0/15	WARNING	No peak detected.
0/16	WARNING	The bandwidth of the SEM item is null. Insertion forbidden.
0/18	WARNING	The current environment does not authorize this command.
0/23	WARNING	The selected trace is not available.
0/35	WARNING	The Quasi Peak setting became invalid.
0/36	WARNING	The Quasi Peak detector is not available. Please set EMC mode ON and RBW<1MHz
0/37	WARNING	The Quasi Peak detector is active. Please change it to other detector.
0/38	WARNING	The Time Domain Analysis is ON. Please change to OFF.
0/-100	ERROR	There is no normalization data available for the selected trace.
0/-114	ERROR	The ElectroMagnetic Compatibility option is required.
0/-115	ERROR	The target trace is not available in this environment for the store functionality.
0/-116	ERROR	The Window sweep mode is not allowed if a measure is active.
0/-117	ERROR	The Signal Track is not allowed when Image Suppression is active.
0/-118	ERROR	This functionality is not allowed if the Tracking Generator is not active.
0/-119	ERROR	This functionality is not allowed if the Reference Object in Delta mode is not the Ref Marker.
0/-120	ERROR	The Tracking Generator is out of band. Please change the stop frequency or/and TG frequency offset. (Stop Freq + (TG freq offset)<= 3.1 GHz)
0/-121	ERROR	This functionality is not allowed if Channel or Average or Total Power Measure is active.

Error code	Type	Displayed Message
0/-122	ERROR	The Tracking Generator option is required.
0/-123	ERROR	This functionality is not allowed on Spurious Power Measure mode.
0/-124	ERROR	All limit Lines are OFF. Please activiate at least one line.
0/-125	ERROR	The active measure is not allowed in this context mode. The measure has been switched off.
0/-126	ERROR	This functionality is not allowed on Graphical Zoom Mode. Please change the context mode. (Ext Cfg -> Zoom & Context)
0/-127	ERROR	This functionality is not allowed on multi-context Mode. Please change the context mode. (Ext Cfg -> Zoom & Context -> Reset Context)
0/-128	ERROR	The Frequency Reference INT mode is not available with crystal option.
0/-129	ERROR	The crystal option is required.
0/-130	ERROR	Not available in Zoom (F/F) mode.
0/-131	ERROR	Not available in Zoom (T/T) mode.
0/-132	ERROR	Not available in F/T mode (Ext. config).
0/-133	ERROR	Not available in T/T mode (Ext. config).
0/-135	ERROR	The trace subtract result should be in Write mode. Please change it. (operand 1 - operand 2 -> result) (Trace -> Refresh -> Write)
0/-136	ERROR	The second operand trace should not be in Blank mode. Please change it. (operand 1 - operand 2 -> result)
0/-137	ERROR	The first operand trace should not be in Blank mode. Please change it. (operand 1 - operand 2 -> result)
0/-138	ERROR	The table selected for the spurious measure is empty. Please fill the table.
0/-141	ERROR	Impossible to change the Fundamental Frequency . Please change to Fundamental mode ON. (Meas2 -> Harmonics -> Fundamental)
0/-142	ERROR	Impossible to execute recall functionality. The file is not compatible with this FUS version.
0/-145	ERROR	The TTL Trigger level is available only in EXTERNAL mode.
0/-146	ERROR	The Trigger level is available only in IF or VIDEO mode.
0/-147	ERROR	The Trigger slope is not available in FREE RUN mode.
0/-148	ERROR	The Trigger video is only available in zero span mode.
0/-149	ERROR	The ACP graph mode is ON. Watt and Volt Units is not allowed.
0/-150	ERROR	The ACP graph mode is not allowed in multi-context mode.
0/-151	ERROR	The Carrier Band Width is not available when Nyquist Filter is ON. Please change to OFF. (Meas 1 -> ACP -> Config -> Nyquist Filter)
0/-152	ERROR	The Carrier Band Width is not available in FULL mode screen. Please change to CARR mode. (Meas 1 -> ACP -> Mode)
0/-153	ERROR	The ACP Power Measure is executed on Trace A. This trace is actually in blank mode. Please change to Write mode. (Trace -> Refresh -> Write)

9.7 List of Error Messages

Error code	Type	Displayed Message
0/-154	ERROR	The ACP Channel definition table is empty.
0/-155	ERROR	The Carrier Band Width is not available when Nyquist Filter is ON. Please change to OFF. (Meas 1 -> SEM -> Config -> Nyquist Filter)
0/-157	ERROR	The SEM table is empty.
0/-158	ERROR	Impossible to insert in the SEM table. Overlapping Band.
0/-159	ERROR	Pass Fail functionality not authorized. Spectrum Emission Mask active.
0/-160	ERROR	The power measure is performed on a blank trace.
0/-161	ERROR	The OBW Power Measure is active.
0/-162	ERROR	The Power Measure environment is not valid. Please do ensure you have already save an environment for this Power Measure.
0/-163	ERROR	The power measure trace is in blank mode. Please change to Write mode. (Trace -> Refresh -> Write)
0/-166	ERROR	Scale is Linear Mode. Please select dB/div scale. (Level -> dB/div)
0/-167	ERROR	The target stored trace is the same to the active trace.
0/-168	ERROR	Impossible to set all the trace in blank mode.
0/-169	ERROR	The active trace is in blank mode.
0/-170	ERROR	Noise Measure (dBc/Hz) Impossible to work on the reference marker.
0/-171	ERROR	Impossible to work on the reference marker.
0/-172	ERROR	The delta mode is disable.
0/-173	ERROR	The fixed mode is active.
0/-174	ERROR	The active marker is not enable.
0/-175	ERROR	There is no enable marker.
0/-178	ERROR	Span is not set to 0 Hz. Please change span.
0/-179	ERROR	Span is set 0 Hz. Please change span.
0/-180	ERROR	Impossible to change the parameter. Please insert data in channel table.
0/-181	ERROR	Impossible to change the parameter. Please switch on at least one formula.
0/-182	ERROR	Impossible to change the Stop Frequency via normal mode.
0/-183	ERROR	Impossible to change the Start Frequency via normal mode.
0/-184	ERROR	Impossible to change the Center Frequency via normal mode.
0/-185	ERROR	Impossible to change the Stop Frequency via channel mode.
0/-186	ERROR	Impossible to change the Start Frequency via channel mode.
0/-187	ERROR	Impossible to change the Center Frequency via channel mode.
0/-500	ERROR	The Time Domain Analysis option is required.
3/1	ERROR	Could not save screen copy.
3/2	ERROR	The screen copy cannot be saved on the analyzer memory. Please select another media.

Error code	Туре	Displayed Message
3/3	ERROR	Cannot remove protected file: %1
3/4	ERROR	Cannot rename protected file: %1
3/5	ERROR	Cannot replace protected file: %1
3/6	ERROR	Cannot open file: %1
3/7	ERROR	File %1 Unknown data format.
3/8	ERROR	File %1 Corrupted Data.
3/9	ERROR	File %1 Incompatible Version.
3/10	ERROR	Cannot access media.
3/11	ERROR	File not saved. Not enough space on media.
3/12	ERROR	XML files cannot be saved on the analyzer memory. Please select another media.
3/13	ERROR	Cannot create file.
3/14	ERROR	Format media failed.
3/15	ERROR	No printer detected.
3/16	ERROR	No driver available for this printer.
3/17	WARNING	The last power measure mode has been turned off.
3/18	WARNING	The selected button already exist.
3/19	WARNING	The user menu is full.
3/20	WARNING	Incorrect password.
3/21	WARNING	Quit spurious results before.
3/22	WARNING	Quit table edition before.
3/24	WARNING	Cannot format flash memory.
3/25	WARNING	The tracking generator option is required.
3/26	WARNING	No DHCP server found. Please ensure ethernet cable is connected and verify DHCP server configuration.
5/-87	WARNING	NO PEAK FOUND.
5/-88	WARNING	NO MIN PEAK FOUND.
5/-89	WARNING	NO PEAK FOUND.
5/-90	WARNING	IM : NO PEAK FOUND.
5/-92	WARNING	Parameter out of range: Nyquist data must be changed.
5/-93	WARNING	Integration bandwidth out of range.
5/-94	WARNING	Parameter out of range.
5/-95	WARNING	Parameter out of range: the SPAN must be reduced.
5/-96	WARNING	The Channel table is empty.
5/-97	WARNING	ACP parameter out of range.

9.7 List of Error Messages

Error code	Туре	Displayed Message
5/-98	WARNING	Parameter out of range. Please set the span to a value greater than $(1+B)1/T$.
5/-99	WARNING	Parameter out of range. Please change span.
5/-100	WARNING	Parameter out of range.
7/83	WARNING	Frequency Reference Unlocked

CAUTION:

An error may be displayed because of a hardware failure. In this case, contact Advantest.

- 1. An error that occurred when the calibration was performed
- 2. An error that was detected while the self test was performed
- 3. Others

9.8 In Case of Difficulty

Check the following basics before calling Advantest.

No.	Description	Operation
1	"Warning 7/83 Frequency Reference Unlocked" is displayed.	
	Is the Frequency Reference set to EXT?	SYSTEM, Frequency Reference,
	1. Set it to INT.	INT
	2. If EXT is used as the Frequency Reference: Is a frequency reference signal input to the REF IN connector on the rear panel?	
	Is the input reference frequency equal to the reference frequency set in this instrument?	Ref Freq
2	After the power is turned on, the system does not boot up.	
	Is a USB memory key inserted? Remove the USB memory key and then turn the power on again.	
3	Any key input cannot be accepted.	
	Is the key lock set to ON? (Is the LOCK key lamp illuminated?).	
	Set the key lock to OFF.	LOCK, (password x,x,x,x,) Hz, Hz Turning off and on the power is also recommended.
4	If you do not remember the User Password:	
	Perform the Initialization by using the GPIB. The User Password returns to "0,0,0,0".	Command "RPWD"
5	The USB memory key is not recognized.	
	 Check its format. If formatting the USB memory key on a PC, use the FAT format. Some formats such as NTFS are not recognized. 	
	2. The USB memory key with a security function cannot be used.	
	3. A USB port is located on the front and rear panels. Attempt to change the USB memory key to a different port.	
6	An incorrect measured value, which is approx. 6 dB higher than the correct level, is displayed.	
	Is the Input Impedance set to 75 Ω ? Set it to 50 Ω	AMPLITUDE , <i>Input Impedance</i> (50)

9.9 Product Disposal and Recycle

9.9 Product Disposal and Recycle

This product should be disposed of according to the regulations and laws that are established in your country and municipality.

Before this product is disposed of, separately collect components shown in the table below to prevent the spread of substances, which may be harmful to the global environment, humans, and ecology.

Substance/Component	Used/ Not used	Location	Parts and material
Polychlorinated biphenyls (PCB) containing capacitors	Not used	-	-
Mercury containing components	Used	LCD monitor	Fluorescent tube
Batteries	Used	BPG-032411 BPL-035851	Lithium-ion battery
Printed circuit boards	Used	Panel	Printed circuit board
		Power supply	
		Board	
Toner cartridges	Not used	-	-
Plastic containing brominated flame retardants	Used	WBL-FUS#FRONT*E BEB-032400 BEG-032413 BEG-032415 BPG-032410 BPG-032411 BPL-035851 BPG-032412 BPB-032890 BPG-032405 BPG-032409 BPG-033493 BPG-034304 BPG-034495 BPG-034498 BEG-036043 BPG-036392	Connectors, inductors, tantalum capacitors, diodes, transistors, semiconductor packages
Asbestos waste and components which contain asbestos	Not used	-	-
Cathode ray tubes	Not used	-	-
Chlorofluorocarbons (CFC), Hydro- chlorofluorocarbons (HCFC), Hydrof- luorocarbons (HFC) or Hydrocarbons (HC)	Not used	-	-
Gas discharge lamps	Used	LCD monitor	Fluorescent tube

9.9 Product Disposal and Recycle

Substance/Component	Used/ Not used	Location	Parts and material
Liquid crystal displays of a surface greater than 100 square centimeters and all those back-lighted with gas discharge lamps	Used	LCD monitor	Liquid crystal displays
External electric cables	Used	WBL-U3751*F WBL-U377X#F	Power cable
		WBL-U3751*F WBL-U377X#F	Signal cable
Components containing refractory ceramic fibers	Not used	-	-
Components containing radioactive substances	Not used	-	-
Electrolyte capacitors containing substances of concern (height > 25 mm, diameter > 25 mm or proportionately similar volume)	Not used	-	-
Cadmium and Cadmium compounds	Used	BPC-032551	Variable resistor electric contact
Antimony and Antimony compounds	Used	WBL-FUS#FRONT*E BEB-032400 BEG-032413 BEG-032415 BPG-032410 BPG-032411 BPL-035851 BPG-032412 BPB-032890 BPC-032551 BPG-032405 BPG-032409 BPG-033493 BPG-034498 BPG-034498 BEG-036043 BPG-036392 A199001 (Accessory)	Electronic components (Semiconductors, capacitors, inductors, resistors), electric components (Connectors)

9.9 Product Disposal and Recycle

Substance/Component	Used/ Not used	Location	Parts and material
Beryllium and Beryllium compounds	Used	WBL-FUS#COXCBL WBL-U3751*F WBL-U377X#F WBL-FUS#HONTAI*E WHB-THK700 BEG-032413 BPG-033493 BPG-034495 BPG-036392	Electric components (Switches, connectors)
Arsenic and Arsenic compounds	Used	WBL-FUS#FRONT*E WHB-THK700 BEG-032413 BEG-036043 BPL-035851	Module (Inverter), electronic components (GaAs)
Lead and Lead compounds	Used	WBL-FUS#FRONT*E WBL-FUS#COXCBL WBL-FUS#OPT20 WBL-FUS#FRONT*E WBL-FUS#HONTAI*E BEB-032400 BEG-032413 BEG-032415 BPG-032410 BPG-032411 BPL-035851 BPG-032412 BPB-032890 BPC-032551 BPG-032405 BPG-032405 BPG-03409 BPG-034495 BPG-034495 BPG-034498 BEG-036043 BPG-036392 A199001 (Accessory)	Electronic components mounted on the printed circuit board and lead solder used for mounting.
Vinyl chloride (PVC)	Used	WBL-FUS#COXCBL WBL-FUS#OPT20 WBL-FUS#FRONT*E	PVC-material resin parts

APPENDIX

A.1 Initial Setting List

This section describes the default preset parameter setting list.

Values are set for the RF1 input of the U3751, U3771, and U3772. Values in parenthesis are set for the U3741.

Function	Parameter	Initial set value
FREQUENCY	Center Freq setting	4 GHz (1.5 GHz)
	Start Freq setting	0 Hz
	Stop Freq setting	8 GHz (3 GHz)
	Freq Offset setting	0 Hz
	Freq Offset ON/OFF	Off
	CF Step Size setting (Manual)	0.8 GHz (0.3 GHz)
	CF Step Size (Auto/Manual)	Auto
	Channel Input	OFF
SPAN	Span setting	8 GHz
AMPLITUDE	Ref Level setting	0 dBm
	LOG/LIN selection	LOG
	dB/div setting	10 dB/div
	Unit setting	dBm
	ATT (Auto/Manual)	Auto
	ATT setting (Manual)	10 dB
	Min ATT setting	10 dB
	Min ATT ON/OFF	OFF
	High Sensitivity ON/OFF	OFF
	Ref Offset setting	0.00 dB
	Ref Offset ON/OFF	OFF
	Slide Screen	OFF
CPL	RBW setting (Manual)	3 MHz (1 MHz)
	RBW (Auto/Manual)	Auto
	VBW setting (Manual)	3 MHz (1 MHz)
	VBW (ON/OFF)	OFF
	VBW/RBW ratio	1
	VBW/RBW ratio (Auto/Manual)	Auto
	SPAN/RBW ratio	100

A.1 Initial Setting List

Function	Parameter	Initial set value
	SPAN/RBW ratio (ON/OFF)	OFF
	Sweep Time setting (Manual)	90 ms (60 ms)
	Sweep Time (Auto/Manual)	Auto
EXT CFG	Sweep Mode (SGL/CNT)	CNT
	Trigger Source	Free Run
	Limit Lines	OFF
	Display Line ON/OFF	OFF
	Reference Line ON/OFF	OFF
	Measuring Window	OFF
MKR		OFF
MEAS1		
Channel Power	Execute ON/OFF	OFF
Total Power	Execute ON/OFF	OFF
Average Power	Execute ON/OFF	OFF
OBW	Execute ON/OFF	OFF
ACP	Execute ON/OFF	OFF
Spectrum Emission	Execute ON/OFF	OFF
Spurious	Execute ON/OFF	OFF
MEAS2		
Noise/Hz	Execute ON/OFF	OFF
XdB down	XdB setting	OFF
Intermod	Execute ON/OFF	OFF
Harmonic	Execute ON/OFF	OFF
Frequency Counter	Execute ON/OFF	OFF
TRACE	Refresh Mode setting	Write
	Active Trace setting	A
	Trace Detector Normal/Posi/Nega/Sample/Average	Normal
	Calc Mode setting	Write
	Detector (Auto/Manual)	Auto
	Detector Avg Mode RMS/Video	RMS
SYSTEM	Annotation ON/OFF	ON
	GPIB Address	8
	LAN IP Address	refer to "6.3.2"
	Color Pattern	Color1

A.1 Initial Setting List

Function	Parameter	Initial set value
[GPIB Address]	GPIB address of this instrument	8
[Freq Reference]	INT/EXT	INT
	Ext. Reference	10 MHz
[Display]	Title setting	NULL

A.2 Principle of Operation

A.2 Principle of Operation

This section describes a root Nyquist filter used for input saturation and ACP measurement based on the operating principle of this instrument.

A.2.1 Input Saturation

When a large level signal is applied to this instrument, measurement errors may become larger, depending on the attenuator setting. Input saturation may be suspected as a cause of this. This section describes input saturation.

• Cause of Input Saturation

A block diagram of the input section of this instrument is shown in Figure A-1. The signal entering from the input connector is input into the mixer through the attenuator.

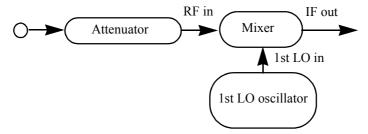


Figure A-1 Block Diagram of the Input Section

Under normal conditions, the input level and output level of the mixer are proportionate to each other. However, if the input level of the mixer increases, the mixer becomes saturated and the output level of the mixer is disproportionate to the input level.

This phenomena is called input saturation and it prevents accurate measurements from being made (see Figure A-2).

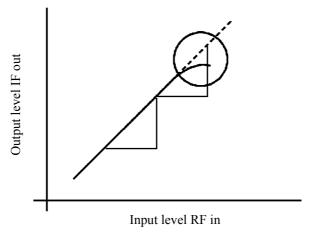


Figure A-2 Relation Between Input and Output of the Mixer

• Preventing Input Saturation

If input saturation occurs, set the most suitable attenuator value to lower the mixer input level.

IMPORTANT: If the attenuator setting is too high, the mixer input signal becomes smaller and analysis becomes impossible. However, if the attenuator setting is too low, the internal mixer circuit may become damaged.

Usually, the appropriate settings are automatically set for a continuous wave (CW) input signal if you set the attenuator to auto and set the peak of the signal to or below the reference level.

If the resolution bandwidth (RBW) is narrower than the modulation bandwidth in the measurement of an input signal with a wide modulation band, the display level decreases. Therefore, the attenuator must be manually set to the optimum value.

- Confirming that the attenuator is set to the optimum value
 - Obtain a rough set value for the attenuator by using the following formula.
 The maximum input level of the mixer is -5 dBm.
 Input attenuator set value (dB) ≥ Input level (dBm) + 10 dB
 - 2. Decrease the attenuator setting in steps while watching the screen. If the peak value on the screen does not change, no input saturation occurs and the measurement can be continued. If the peak value changes, increase the attenuator setting to eliminate the change.

A.2.2 Root Nyquist Filter

When measuring the adjacent channel leakage power, this instrument is able to make a correction to the input signal equivalent to as if the signal passed through the root Nyquist filter.

When calculating the power for each channel by integrating the trace data, the power is multiplied by the coefficient of the root Nyquist filter at the corresponding frequency (H(n)).

$$\begin{split} P"_{U} &= \sum_{n = a}^{b} \frac{P(n)}{10} \\ P"_{U} &= \sum_{n = a}^{b} 10 \\ &= f_{Uch} - \frac{(1 + \alpha)}{2T}, b = f_{Uch} + \frac{(1 + \alpha)}{2T} \\ P"_{L} &= \sum_{n = a}^{b} \frac{P(n)}{10} \\ &= f_{Lch} - \frac{(1 + \alpha)}{2T}, b = f_{Lch} + \frac{(1 + \alpha)}{2T} \end{split}$$

The coefficient of the root Nyquist filter (H(n)) is calculated from the symbol rate (T) and the roll-off factor (α) by using the following formula.

$$|H(n)| = \begin{cases} 1 & 0 \le |f| \le (1-\alpha)/2T \\ \cos[(T/4\alpha) (2\pi |f| -\pi (1-\alpha)/T)] & (1-\alpha)/2T \le |f| \le (1+\alpha)/2T \\ 0 & (1+\alpha)/2T \le |f| \end{cases}$$

A.2.2 Root Nyquist Filter

The characteristics of the root Nyquist filter are shown below.

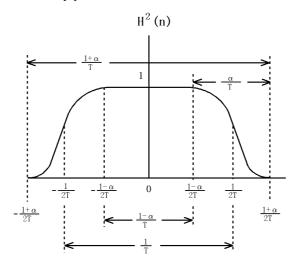


Figure A-3 Characteristics of the Root Nyquist Filter

A.3 Glossary

Resolution Bandwidth

The spectrum analyzer uses the band-pass filter (BPF) to analyze certain frequencies in the input signal. The 3 dB bandwidth of the BPF is called the resolution bandwidth. (See Figure A-4) The BPF characteristics should be set according to the sweep width and the sweep speed used for the trace.

This spectrum analyzer sets the optimal value for the sweep width. In general, smaller bandwidths improve resolution and the resolution of the spectrum analyzer should be expressed by using the narrowest resolution bandwidth (See Figure A-4 (b) below).

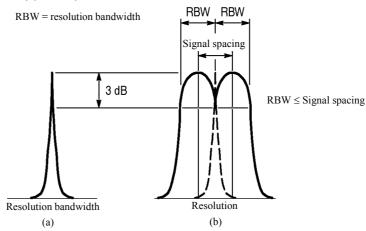


Figure A-4 Resolution Bandwidth

IF Gain Uncertainty

The uppermost scale on the screen is the reference used to read the absolute level of an input signal on the spectrum analyzer. The level set for this uppermost scale is referred to as the reference level.

The reference level is set using the **Ref Level** key and displayed in dBm or dB μ . The absolute accuracy of this display is determined by the IF gain uncertainty assuming the input attenuator is at a constant level.

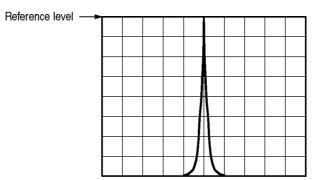


Figure A-5 IF Gain Uncertainty

Gain Compression

If the input signal is greater than a certain value, the correct value is not displayed on the screen, and the input signal appears as if it were compressed. This phenomenon is called gain compression, and it reflects the linearity in the input signal range. Normally, the gain compression for a spectrum analyzer is specified as the input signal level that produces a 1 dB error from a perfect linear response.

A.3 Glossary

Maximum Input Level

This is the maximum level allowed for the input circuit of the spectrum analyzer. The level can be modified by the input attenuator.

Noise Sidebands

Noise sidebands are used to show the purity of the oscillator.

Spectrum analyzer efficiency is reduced by noise generated in the local oscillator and phase lock loop of the analyzer. This noise will appear in the vicinity of the spectrum on the screen.

Therefore, the sideband noise of the analyzer is defined and the signals that are larger than the sideband noise of the analyzer can be analyzed.

The spectrum analyzer's noise sideband characteristics are shown in the following example.

Example Suppose the noise level measured in the resolution bandwidth of 1 kHz is -70 dB at 20 kHz apart from the carrier. The noise level is normally expressed by the energy contained in the 1 Hz bandwidth (Figure A-6 (b)). With a bandwidth of 1 Hz, the following applies: Since the value is -70 dB when the bandwidth is 1 kHz, the signals within the 1 Hz bandwidth will be lower than this by about 10 log 1 Hz/1 kHz [dB], or about 30 dB. Consequently, it is expressed as -100 dBc/Hz at 20 kHz apart from the carrier when the resolution bandwidth is 1 kHz.

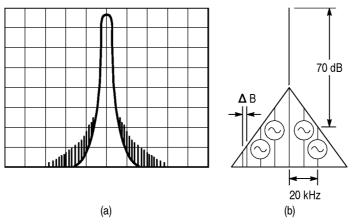


Figure A-6 Noise Sidebands

Residual FM

The short-term frequency stability of the local oscillators built in the spectrum analyzer is expressed as residual FM. The frequency width fluctuating per unit time is expressed as p-p. This also determines the measurement limit value when measuring the residual FM of a signal.

Residual Response

Residual response is how much the spurious signal, which is generated by the spectrum analyzer, is suppressed after being treated as an input signal.

Residual response is generated by the leaking of signals such as local oscillator output in the spectrum analyzer. This should be taken into consideration when analyzing a low-level input signal.

Frequency Response

This term represents the amplitude characteristics for given frequencies (frequency characteristics).

In the spectrum analyzer, frequency response means the frequency characteristics (flatness) of the input attenuator and mixer for the input frequency, and is given in $\pm \Delta dB$.

Spurious Response

Spurious responses that mean any non-measured signal are classified according to their characteristics.

Second Harmonic Distortion:

This is the distortion caused by the non-linearity of a spectrum analyzer (especially generated in the mixer) when an ideal and undistorted signal is input to the spectrum analyzer. This performance determines spectrum analyzer's capability of measuring harmonic distortion.(see Figure A-7)

Third Order Distortion:

The third order distortion is caused by the non-linearity of a spectrum analyzer when two signals with different frequencies f1 and f2 are input and two signals of 2f1-f2 and 2f2-fi are generated near the input signals. The amplitude of these signals depends on the mixer input level. (see Figure A-7)

The maximum value is specified.

Image/Multiple/Out-of-band responses:

In addition to the two types of spurious signals described above, a spurious called "non-harmonic spurious" is generated at particular frequencies by the spectrum analyzer. There are three types of responses in the non-harmonic spurious: the image, multiple and out-of-band responses.




Figure A-7 Spurious Response

Zero Span

The spectrum analyzer sweeps the time in the horizontal axis at certain frequency but does not sweep frequencies in this mode.

A.3 Glossary

Occupied Bandwidth

When information is transmitted through radio waves, the spread of the frequency spectrum is caused along with the modulation. The occupied bandwidth is defined as the width of frequency spectrum that occupies 99% of total average power. (see Figure A-8)




Figure A-8 Occupied Bandwidth

Bandwidth Selectivity

The band-pass filter normally has a Gaussian distribution characteristics instead of the so-called rectangular characteristic. Consequently, if two adjacent signals of different levels exist, the smaller signal hides in the skirt of the larger signal. (See Figure A-9)

Therefore, the bandwidth at a certain attenuation range (60 dB) should also be defined. The ratio between the 3 dB width and 60 dB width is expressed as the bandwidth selectivity.

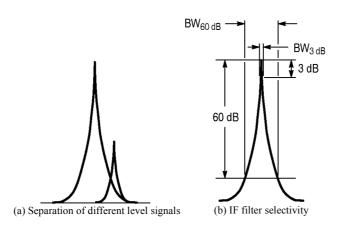


Figure A-9 Bandwidth Selectivity

Bandwidth Accuracy

The bandwidth accuracy of the resolution bandwidth filter is expressed by the deviation from the nominal value of the 3 dB-lowered point. This specification has almost no effect when measuring the level of a continuous signal, but it should be taken into consideration when measuring the level of a noise signal.

Bandwidth Switching Uncertainty

Several resolution bandwidth filters are used to obtain the optimal resolution in a signal spectrum analysis according to the frequency span. When switching from one resolution bandwidth filter to another while measuring one signal, an error is generated because of the differences in loss between resolution bandwidth filters. This error is defined as the bandwidth switching uncertainty.

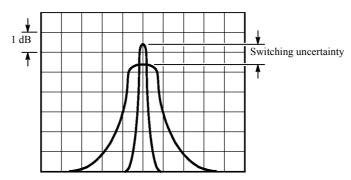


Figure A-10 Bandwidth Switching Uncertainty

Average Noise Level

This sensitivity represents spectrum analyzer's capability of detecting the smallest signal and is directly related with noises generated from a spectrum analyzer itself. The sensitivity, however, varies depends on the used resolution bandwidth. In general, the maximum input sensitivity of a spectrum analyzer is expressed as average noise level when the instrument is used with its minimum resolution bandwidth.

A.3 Glossary

VSWR: Voltage Standing Wave Ratio

This shows the state of impedance matching when a spectrum analyzer is connected to a signal source that includes ideal and nominal output impedance. The VSWR is expressed as the ratio of the maximum value to minimum value of a standing wave, which consists of traveling and reflected waves. The VSWR is another expression of the reflection coefficient or return loss.

Referring to Figure A-11, the signal E1 at the receiving end (the spectrum analyzer input section) is the same as the signal E0 at the transmitting end if the impedance of the receiving end is matched to that of the transmitting end.

The reflection coefficient is expressed in the formula shown below when the reflected wave ER exists due to a mismatch between the impedances.

Reflection coefficient m = Reflected wave E_R / Traveling wave E_0

The Return loss is expressed in the formula shown below.

Return loss = 20 log
$$E_R / E_0$$
 [dB]
VSWR = $(E_0 + E_R) / (E_0 - E_R)$

The relationship of VSWR with the reflection coefficient is as follows.

$$VSWR = (1 + |m|) / (1 - |m|)$$

The range of VSWR is between 1 and ∞ the nearer to 1 this value is, the better the state of impedance matching is.




Figure A-11 VSWR

A.4 dB Conversion Formula

1. Definitions

$$0 \text{ dBV} = 1 \text{ Vrms} \qquad \qquad Y \text{ dBV} = 20 \log \frac{X \text{ V}}{1 \text{ V}}$$

$$0 \text{ dBm} = 1 \text{ mW} \qquad Y \text{ dBm} = 10 \log \frac{X \text{ mW}}{1 \text{ mW}}$$

$$0 \text{ dB}\mu\text{V} = 1 \text{ }\mu\text{Vrms} \qquad Y \text{ dB}\mu\text{V} = 20 \log \frac{X \text{ }\mu\text{V}}{1 \text{ }\mu\text{V}}$$

$$0 \text{ dBpw} = 1 \text{ pW} \qquad Y \text{ dBpw} = 10 \log \frac{X \text{ }p\text{W}}{1 \text{ }p\text{W}}$$

2. Conversion formulas

$$\begin{split} & \text{If R} = 50 \ \Omega; & \text{If R} = 75 \ \Omega; \\ & \text{dBV} \cong (\text{dBm - 13 dB}) & \text{dBV} \cong (\text{dBm - 11 dB}) \\ & \text{dB}\mu\text{V} \cong (\text{dBm + 107 dB}) & \text{dB}\mu\text{V} \cong (\text{dBm + 109 dB}) \\ & \text{dB}\mu\text{Vemf} \cong (\text{dBm + 113 dB}) & \text{dB}\mu\text{Vemf} \cong (\text{dBm + 115 dB}) \\ & \text{dBpw} \cong (\text{dBm + 90 dB}) & \text{dBpw} \cong (\text{dBm + 90 dB}) \end{split}$$

3. Examples


Converting 1 mV into dB
$$\mu$$
V:
$$20 \log \frac{1 \text{ mV}}{1 \mu \text{V}} = 20 \log 10^3 = 60 \text{ dB}\mu\text{V}$$
 Converting 0 dBm into dB μ V:
$$\begin{cases} 0 \text{ dBm} + 107 \text{ dB} = 107 \text{ dB}\mu\text{V} (R = 50 \ \Omega) \\ 0 \text{ dBm} + 109 \text{ dB} = 109 \text{ dB}\mu\text{V} (R = 75 \ \Omega) \end{cases}$$
 Converting 60 dB μ V into dBm:
$$\begin{cases} 60 \text{ dB}\mu\text{V} - 107 \text{ dB} = -47 \text{ dBm} (R = 50 \ \Omega) \\ 60 \text{ dB}\mu\text{V} - 109 \text{ dB} = -49 \text{ dBm} (R = 75 \ \Omega) \end{cases}$$
 Converting 10 V/m into dB μ V/m:
$$20 \log \frac{10 \text{ V/m}}{1 \mu \text{V/m}} = 140 \text{ dB}\mu\text{V/m}$$


4. Relationship between dBm and Watt

+50 dE	m +40 dBm	+30 dBm	+20 dBm	+10 dBm	+0 dBm	-10 dBm	-20 dBm	-30 dBm
100 V	10 W	1 W	100 mW	10 mW	1 mW	0.1 mW	0.01 mW	0.001 mW

A.5 Menu Map List


SYSTEM (1)

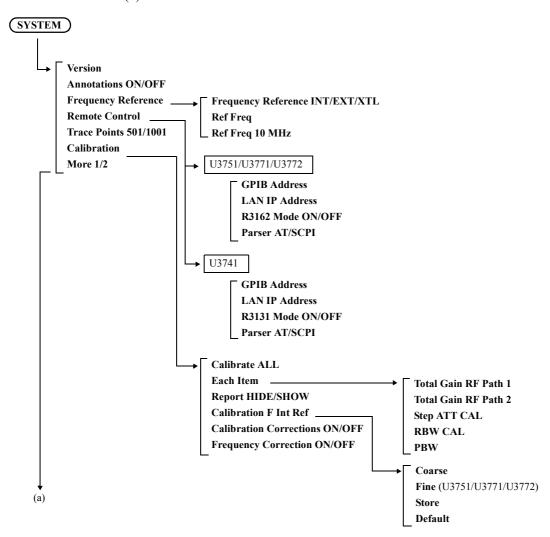

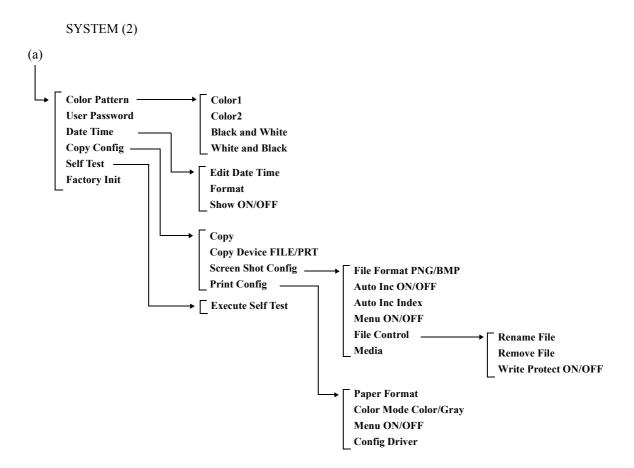


• APPLI Spectrum Analyzer 2 Channels Viewer 2 Channel ON/OFF Spectrum RF1 Spectrum RF2 2 Channel Preset Context RF2|RF1


• FILE

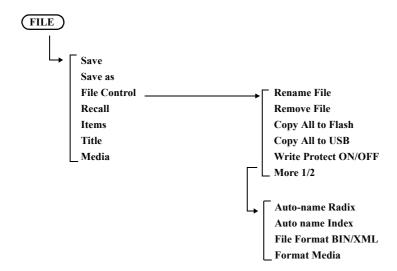


• MEAS 1 (1)

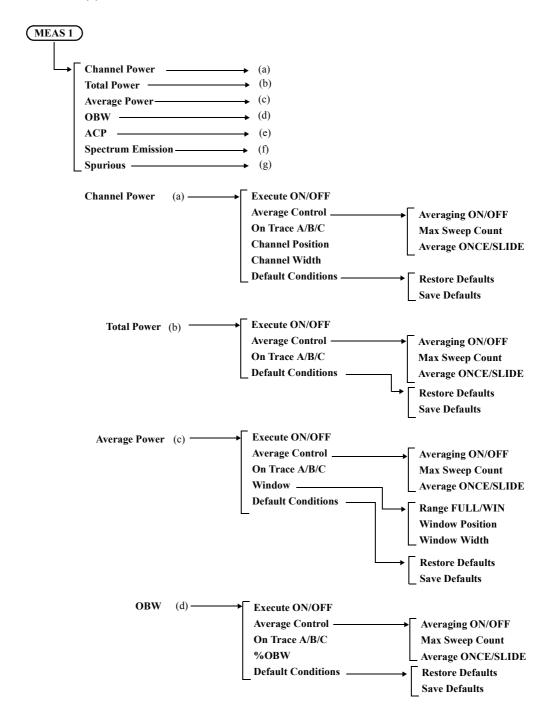


MEAS 1 (2)

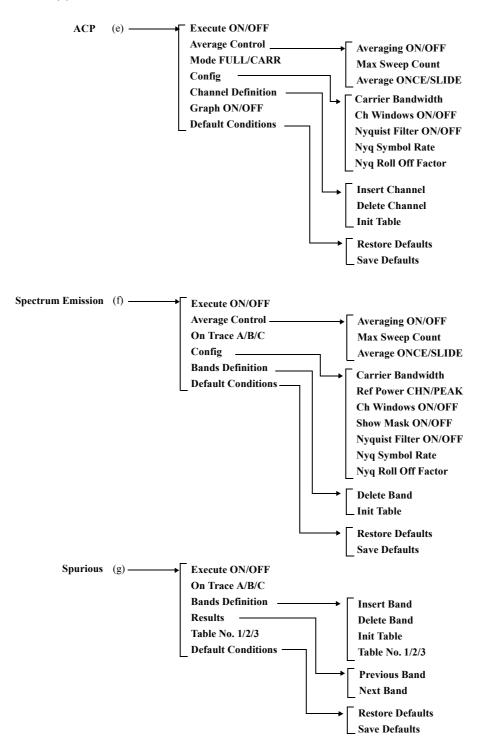


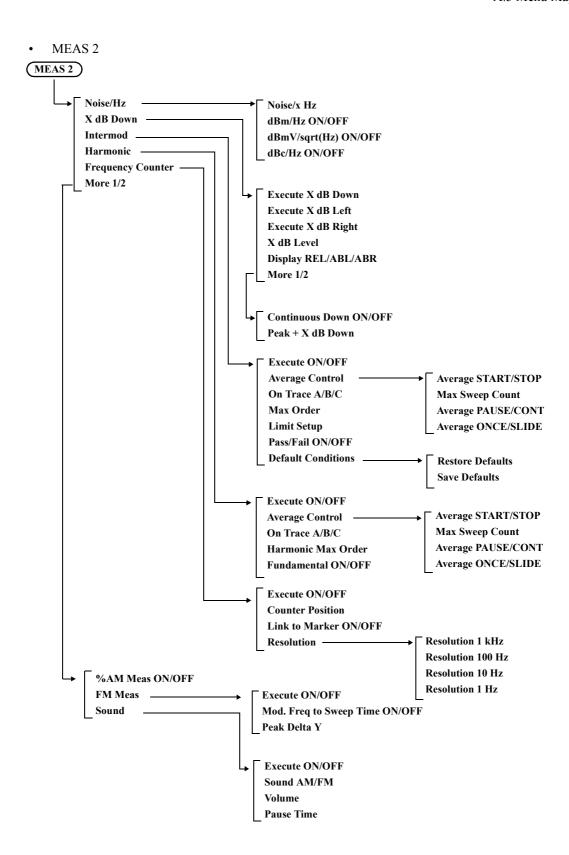


TRACE

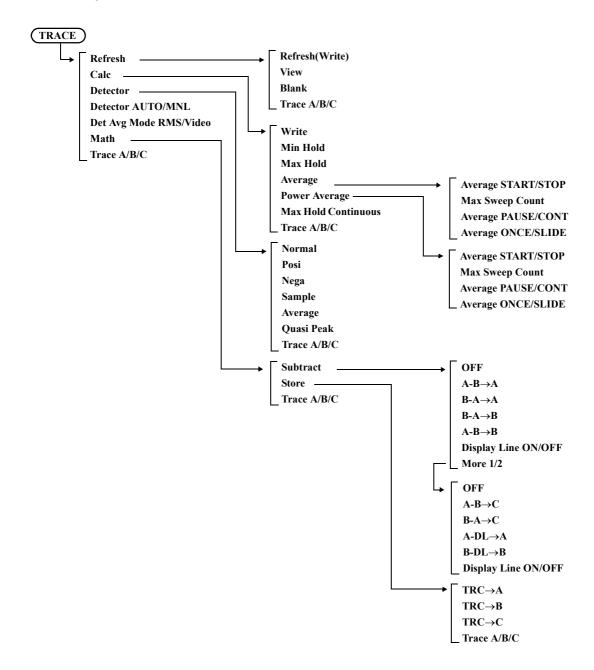


• MKR

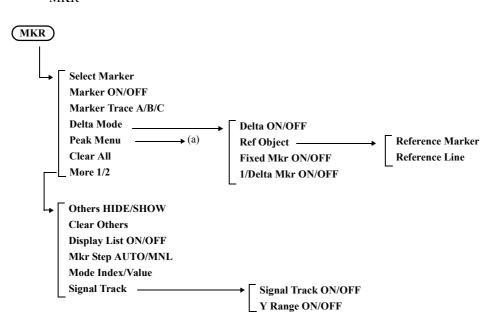


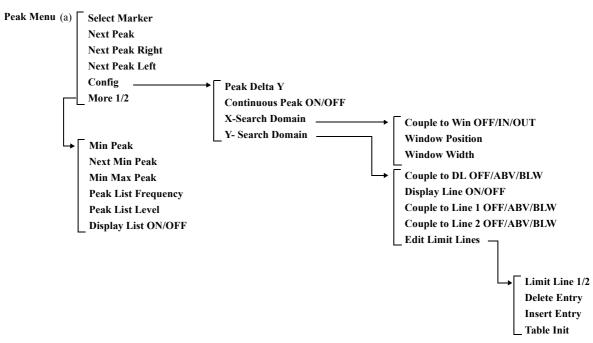


PEAK

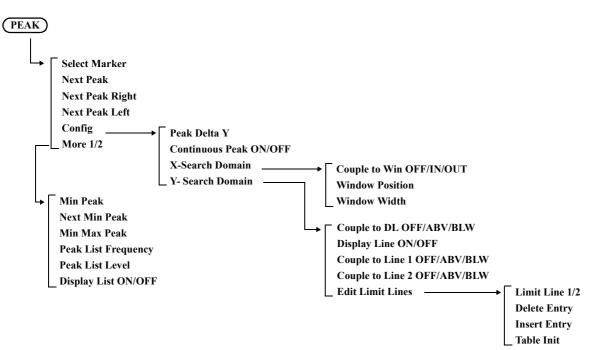


• MKR \rightarrow




• TG (Option)

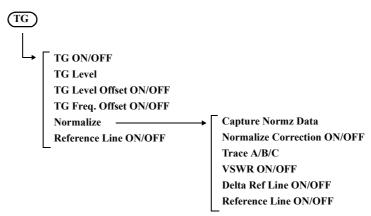


FREQUENCY

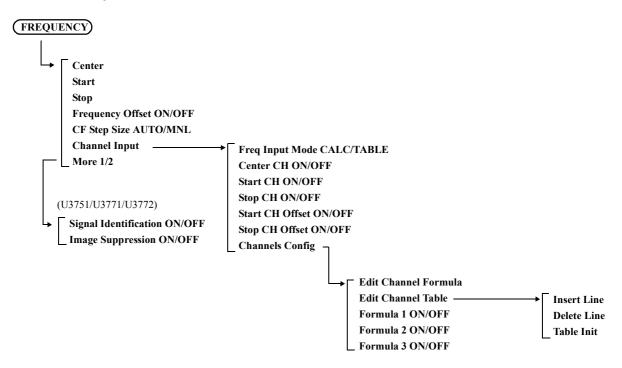


SPAN




AMPLITUDE

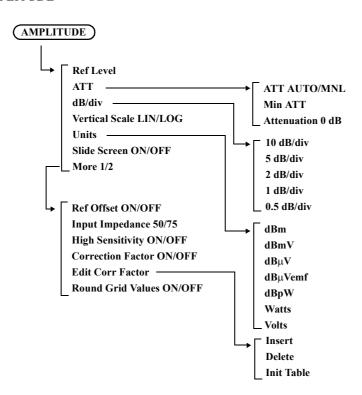


• EXT CFG (Extended Configuration options) (1)

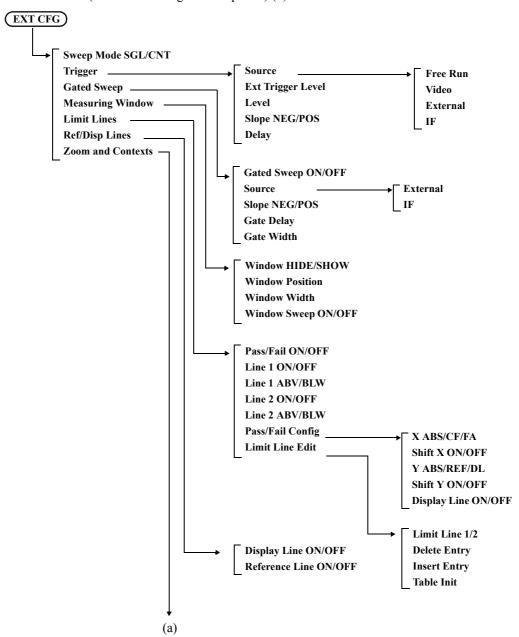

EXT CFG (Extended Configuration options) (1)

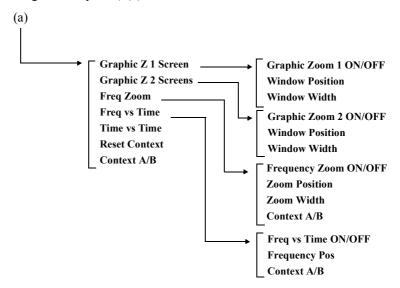

CPL (Coupled function)

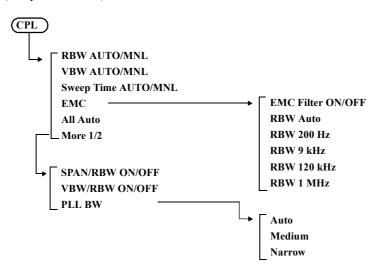

A.6 TV Channel Table (Japan)

A.6.1 CATV Channel Number and Frequency

Analyzer's channel	Channel	Frequency range (MHz)	Center frequency (MHz)	Picture frequency (MHz)	Sound frequency (MHz)
1	1	90.00 ~ 96.00	93	91.25	95.75
2	2	96.00 ~ 102.00	99	97.25	101.75
3	3	102.00 ~ 108.00	105	103.25	107.75
4	4	170.00 ~ 176.00	173	171.25	175.75
5	5	176.00 ~ 182.00	179	177.25	181.75
6	6	182.00 ~ 188.00	185	183.25	187.75
7	7	188.00 ~ 194.00	191	189.25	193.75
8	8	192.00 ~ 198.00	195	193.25	197.75
9	9	198.00 ~ 204.00	201	199.25	203.75
10	10	204.00 ~ 210.00	207	205.25	209.75
11	11	210.00 ~ 216.00	213	211.25	215.75
12	12	216.00 ~ 222.00	219	217.25	221.75
13	Cl3	108.00 ~ 114.00	111	109.25	113.25
14	C14	114.00 ~ 120.00	117	115.25	119.75
15	C15	120.00 ~ 126.00	123	121.25	125.75
16	C16	126.00 ~ 132.00	129	127.25	131.75
17	C17	132.00 ~ 138.00	135	133.25	137.75
18	C18	138.00 ~ 144.00	141	139.25	143.75
19	C19	144.00 ~ 150.00	147	145.25	149.75
20	C20	150.00 ~ 156.00	153	151.25	155.75
21	C21	156.00 ~ 162.00	159	157.25	161.75
22	C22	164.00 ~ 170.00	167	165.25	169.75
23	C23	222.00 ~ 228.00	225	223.25	227.75
24	C24	230.00 ~ 236.00	233	231.25	235.75
25	C25	236.00 ~ 242.00	239	237.25	241.75
26	C26	242.00 ~ 248.00	245	243.25	247.75
27	C27	248.00 ~ 254.00	251	249.25	253.75
28	C28	252.00 ~ 258.00	255	253.25	257.75
29	C29	258.00 ~ 264.00	261	259.25	263.75
30	C30	264.00 ~ 270.00	267	265.25	269.75

A.6.1 CATV Channel Number and Frequency

Analyzer's channel	Channel	Frequency range (MHz)	Center frequency (MHz)	Picture frequency (MHz)	Sound frequency (MHz)
31	C31	$270.00 \sim 276.00$	273	271.25	275.75
32	C32	276.00 ~ 282.00	279	277.25	281.75
33	C33	282.00 ~ 288.00	285	283.25	287.75
34	C34	288.00 ~ 294.00	291	289.25	293.75
35	C35	294.00 ~ 300.00	297	295.25	299.75
36	C36	300.00 ~ 306.00	303	301.25	305.75
37	C37	306.00 ~ 312.00	309	307.25	311.75
38	C38	312.00 ~ 318.00	315	313.25	317.75
39	C39	318.00 ~ 324.00	321	319.25	323.75
40	C40	324.00 ~ 330.00	327	325.25	329.75
41	C41	330.00 ~ 336.00	333	331.25	335.75
42	C42	336.00 ~ 342.00	339	337.25	341.75
43	C43	342.00 ~ 348.00	345	343.25	347.75
44	C44	348.00 ~ 354.00	351	349.25	353.75
45	C45	354.00 ~ 360.00	357	355.25	359.75
46	C46	360.00 ~ 366.00	363	361.25	365.75
47	C47	366.00 ~ 372.00	369	367.25	371.75
48	C48	372.00 ~ 378.00	375	373.25	377.75
49	C49	378.00 ~ 384.00	381	379.25	383.75
50	C50	384.00 ~ 390.00	387	385.25	389.75
51	C51	390.00 ~ 396.00	393	391.25	395.75
52	C52	396.00 ~ 402.00	399	397.25	401.75
53	C53	402.00 ~ 408.00	405	403.25	407.75
54	C54	408.00 ~ 414.00	411	409.25	413.75
55	C55	414.00 ~ 420.00	417	415.25	419.75
56	C56	420.00 ~ 426.00	423	421.25	425.75
57	C57	426.00 ~ 432.00	429	427.25	431.75
58	C58	432.00 ~ 438.00	435	433.25	437.75
59	C59	438.00 ~ 444.00	441	439.25	443.75
60	C60	444.00 ~ 450.00	447	445.25	449.75
61	C61	450.00 ~ 456.00	453	451.25	455.75
62	C62	456.00 ~ 462.00	459	457.25	461.75
63	C63	462.00 ~ 468.00	465	463.25	467.75

A.6.2 VHF/UHF Channel Number and Frequency

1. VHF

Analyzer's channel	Channel	Frequency range (MHz)	Center frequency (MHz)	Picture frequency (MHz)	Sound frequency (MHz)
1	1	90.00 ~ 96.00	93	91.25	95.75
2	2	96.00 ~ 102.00	99	97.25	101.75
3	3	102.00 ~ 108.00	105	103.25	107.75
4	4	170.00 ~ 176.00	173	171.25	175.75
5	5	176.00 ~ 182.00	179	177.25	181.75
6	6	182.00 ~ 188.00	185	183.25	187.75
7	7	188.00 ~ 194.00	191	189.25	193.75
8	8	192.00 ~ 198.00	195	193.25	197.75
9	9	198.00 ~ 204.00	201	199.25	203.75
10	10	204.00 ~ 210.00	207	205.25	209.75
11	11	210.00 ~ 216.00	213	211.25	215.75
12	12	216.00 ~ 222.00	219	217.25	221.75

2. UHF

Analyzer's channel	Channel	Frequency range (MHz)	Center frequency (MHz)	Picture frequency (MHz)	Sound frequency (MHz)
13	13	$470.00 \sim 476.00$	473	471.25	475.75
14	14	476.00 ~ 482.00	479	477.25	481.75
15	15	482.00 ~ 488.00	485	483.25	487.75
16	16	488.00 ~ 494.00	491	489.25	493.75
17	17	494.00 ~ 500.00	497	495.25	499.75
18	18	500.00 ~ 506.00	503	501.25	505.75
19	19	506.00 ~ 512.00	509	507.25	511.75
20	20	512.00 ~ 518.00	515	513.25	517.75
21	21	518.00 ~ 524.00	521	519.25	523.75
22	22	524.00 ~ 530.00	527	525.25	529.75
23	23	530.00 ~ 536.00	533	531.25	535.75
24	24	536.00 ~ 542.00	539	537.25	541.75
25	25	542.00 ~ 548.00	545	543.25	547.75
26	26	548.00 ~ 554.00	551	549.25	553.75
27	27	554.00 ~ 560.00	557	555.25	559.75
28	28	560.00 ~ 566.00	563	561.25	565.75

A.6.2 VHF/UHF Channel Number and Frequency

Analyzer's channel	Channel	Frequency range (MHz)	Center frequency (MHz)	Picture frequency (MHz)	Sound frequency (MHz)
29	29	566.00 ~ 572.00	569	567.25	571.75
30	30	572.00 ~ 578.00	575	573.25	577.75
31	31	578.00 ~ 584.00	581	579.25	583.75
32	32	584.00 ~ 590.00	587	585.25	589.75
33	33	590.00 ~ 596.00	593	591.25	595.75
34	34	596.00 ~ 602.00	599	597.25	601.75
35	35	602.00 ~ 608.00	605	603.25	607.75
36	36	608.00 ~ 614.00	611	609.25	613.75
37	37	614.00 ~ 620.00	617	615.25	619.75
38	38	620.00 ~ 626.00	623	621.25	625.75
39	39	626.00 ~ 632.00	629	627.25	631.75
40	40	632.00 ~ 638.00	635	633.25	637.75
41	41	638.00 ~ 644.00	641	639.25	643.75
42	42	644.00 ~ 650.00	647	645.25	649.75
43	43	650.00 ~ 656.00	653	651.25	655.75
44	44	656.00 ~ 662.00	659	657.25	661.75
45	45	662.00 ~ 668.00	665	663.25	667.75
46	46	668.00 ~ 674.00	671	669.25	673.75
47	47	674.00 ~ 680.00	677	675.25	679.75
48	48	680.00 ~ 686.00	683	681.25	685.75
49	49	686.00 ~ 692.00	689	687.25	691.75
50	50	692.00 ~ 698.00	695	693.25	697.75
51	51	$698.00 \sim 704.00$	701	699.25	703.75
52	52	$704.00 \sim 710.00$	707	705.25	709.75
53	53	710.00 ~ 716.00	713	711.25	715.75
54	54	$716.00 \sim 722.00$	719	717.25	721.75
55	55	722.00 ~ 728.00	725	723.25	727.75
56	56	728.00 ~ 734.00	731	729.25	733.75
57	57	734.00 ~ 740.00	737	735.25	739.75
58	58	740.00 ~ 746.00	743	741.25	745.75
59	59	746.00 ~ 752.00	749	747.25	751.75
60	60	752.00 ~ 758.00	755	753.25	757.75
61	61	758.00 ~ 764.00	761	759.25	763.75
62	62	764.00 ~ 770.00	767	765.25	769.75

A.6.3 Terrestrial Digital Broadcasting Channel Number and Frequency

UHF that supports terrestrial digital broadcasting

Analyzer's channel	Channel	Frequency range (MHz)	Center frequency (MHz)
13	13	$470.00 \sim 476.00$	473.142857
14	14	476.00 ~ 482.00	479.142857
15	15	482.00 ~ 488.00	485.142857
16	16	488.00 ~ 494.00	491.142857
17	17	494.00 ~ 500.00	497.142857
18	18	500.00 ~ 506.00	503.142857
19	19	506.00 ~ 512.00	509.142857
20	20	512.00 ~ 518.00	515.142857
21	21	518.00 ~ 524.00	521.142857
22	22	524.00 ~ 530.00	527.142857
23	23	530.00 ~ 536.00	533.142857
24	24	536.00 ~ 542.00	539.142857
25	25	542.00 ~ 548.00	545.142857
26	26	548.00 ~ 554.00	551.142857
27	27	554.00 ~ 560.00	557.142857
28	28	560.00 ~ 566.00	563.142857
29	29	566.00 ~ 572.00	569.142857
30	30	572.00 ~ 578.00	575.142857
31	31	578.00 ~ 584.00	581.142857
32	32	584.00 ~ 590.00	587.142857
33	33	590.00 ~ 596.00	593.142857
34	34	596 .00 ~ 602.00	599.142857
35	35	602.00 ~ 608.00	605.142857
36	36	608.00 ~ 614.00	611.142857
37	37	614.00 ~ 620.00	617.142857
38	38	620.00 ~ 626.00	623.142857
39	39	626.00 ~ 632.00	629.142857
40	40	632.00 ~ 638.00	635.142857
41	41	638.00 ~ 644.00	641.142857
42	42	644.00 ~ 650.00	647.142857
43	43	650.00 ~ 656.00	653.142857
44	44	656.00 ~ 662.00	659.142857

A.6.3 Terrestrial Digital Broadcasting Channel Number and Frequency

		i	
Analyzer's channel	Channel	Frequency range (MHz)	Center frequency (MHz)
45	45	662.00 ~ 668.00	665.142857
46	46	668.00 ~ 674.00	671.142857
47	47	674.00 ~ 680.00	677.142857
48	48	680.00 ~ 686.00	683.142857
49	49	686.00 ~ 692.00	689.142857
50	50	692.00 ~ 698.00	695.142857
51	51	698.00 ~ 704.00	701.142857
52	52	704.00 ~ 710.00	707.142857
53	53	710.00 ~ 716.00	713.142857
54	54	716.00 ~ 722.00	719.142857
55	55	722.00 ~ 728.00	725.142857
56	56	728.00 ~ 734.00	731.142857
57	57	734.00 ~ 740.00	737.142857
58	58	740.00 ~ 746.00	743.142857
59	59	746.00 ~ 752.00	749.142857
60	60	752.00 ~ 758.00	755.142857
61	61	758.00 ~ 764.00	761.142857
62	62	764.00 ~ 770.00	767.142857

A.6.4 Satellite Broadcasting (BS-IF Band) Channel Number and Frequency

Analyzer's channel	Channel	Frequency range (MHz)	Center frequency (MHz)
1	BS-1	$1032.23 \sim 1066.73$	1049.48
3	BS-3	1070.59 ~ 1105.09	1087.84
5	BS-5	1112.70 ~ 1139.70	1126.20
7	BS-7	1151.06 ~ 1178.06	1164.56
9	BS-9	1189.42 ~ 1216.42	1202.92
11	BS-11	1227.78 ~ 1254.78	1241.28
13	BS-13	1262.39 ~ 1296.89	1279.64
15	BS-15	1300.75 ~ 1335.25	1318.00
17	BS-17	1339.11 ~ 1373.61	1356.36
19	BS-19	1377.47 ~ 1411.97	1394.72
21	BS-21	1415.83 ~ 1450.33	1433.08
23	BS-23	1454.19 ~ 1488.69	1471.44

A.6.5 110 CS (CS-IF Band) Channel Number and Frequency

Analyzer's channel	Channel	Frequency range (MHz)	Center frequency (MHz)
2	ND2	1595.75 ~ 1630.25	1613
4	ND4	1635.75 ~ 1670.25	1653
6	ND6	1675.75 ~ 1710.25	1693
8	ND8	1715.75 ~ 1750.25	1733
10	ND10	1755.75 ~ 1790.25	1773
12	ND12	1795.75 ~ 1830.25	1813
14	ND14	1835.75 ~ 1870.25	1853
16	ND16	1875.75 ~ 1910.25	1893
18	ND18	1915.75 ~ 1950.25	1933
20	ND20	1955.75 ~ 1990.25	1973
22	ND22	1995.75 ~ 2030.25	2013
24	ND24	2035.75 ~ 2070.25	2053

U3741 DIMENSIONAL OUTLINE DRAWING


This drawing shows external dimensions of


Unit:mm NOTE used can cause a change in the appearance


of the instrument.

The difference in products and options

this instrument.

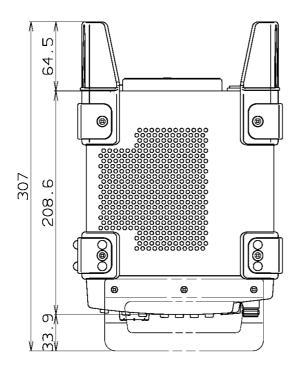

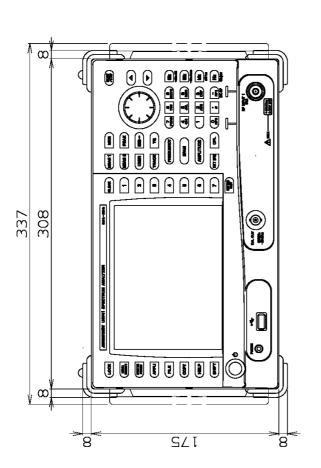

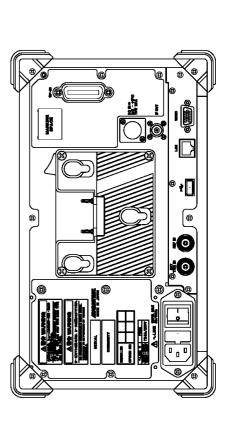

ļ


NOTE


Unit:mm

This drawing shows external dimensions of this instrument.

The difference in products and options used can cause a change in the appearance of the instrument.

U3751 DIMENSIONAL OUTLINE DRAWING

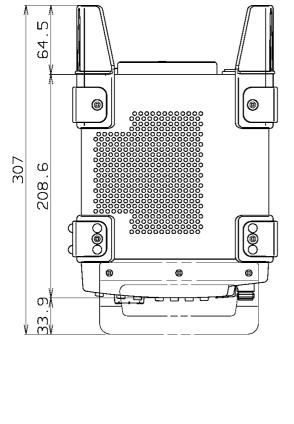

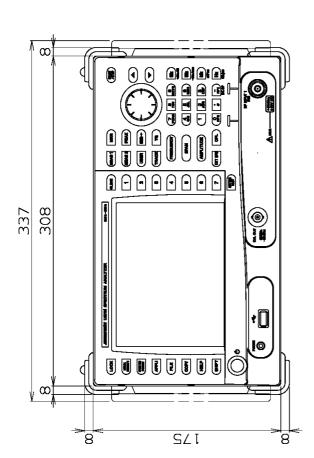

U3771 DIMENSIONAL OUTLINE DRAWING

This drawing shows external dimensions of


Unit:mm


NOTE

this instrument.

The difference in products and options used can cause a change in the appearance


of the instrument.

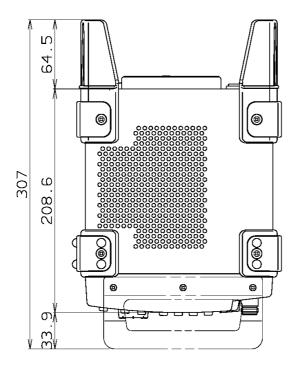

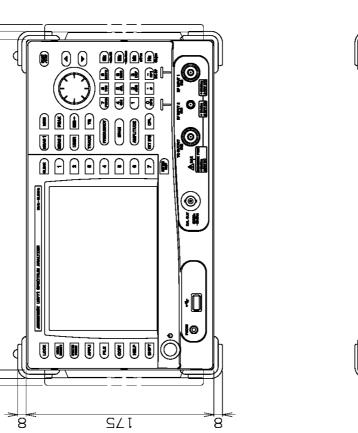

337

 ∞

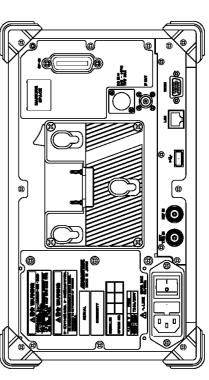


NOTE

Unit:mm

This drawing shows external dimensions of this instrument.


The difference in products and options used can cause a change in the appearance of the instrument.


U3772 DIMENSIONAL OUTLINE DRAWING

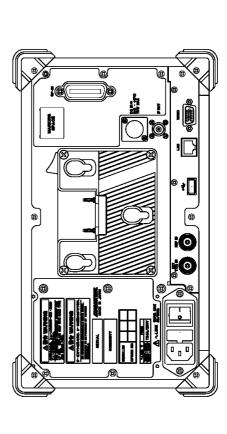



308

For Basic Operation

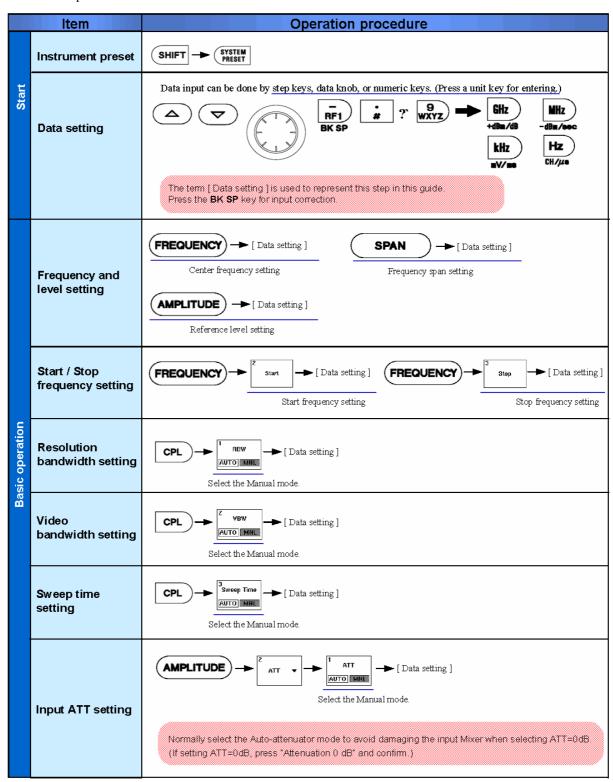

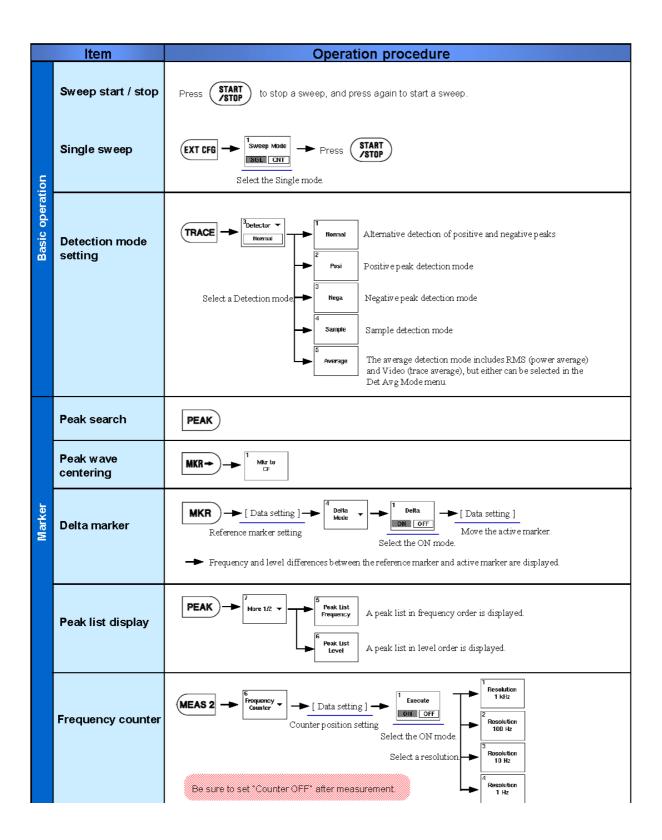

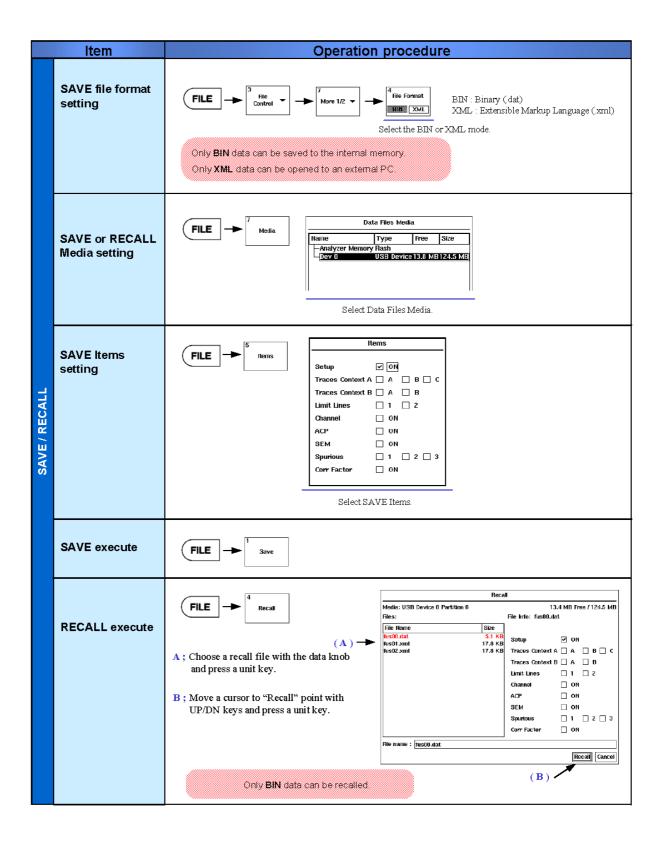

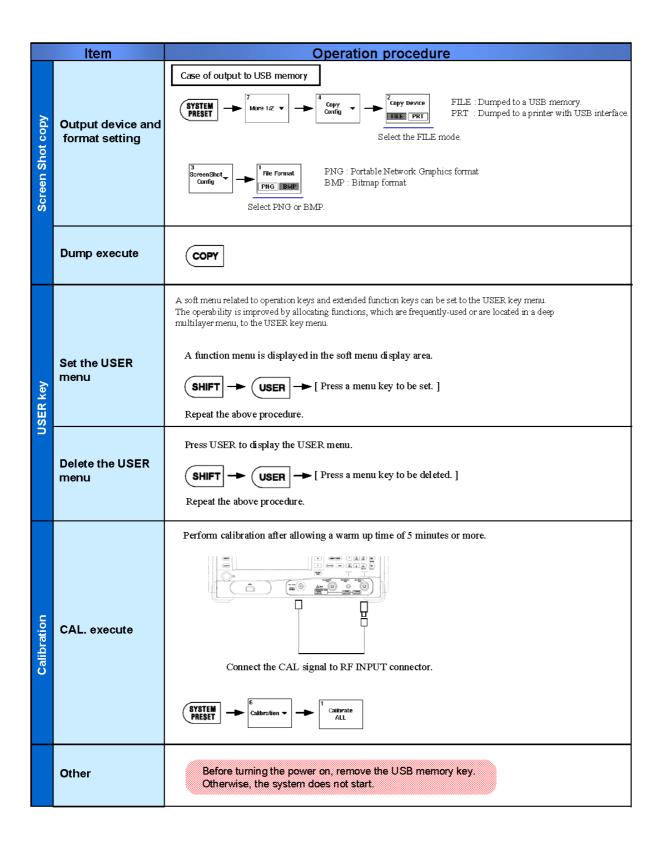

ALPHABETICAL INDEX

[Symbol]				5-32,	
%AM Meas ON/OFF	5-37,	5-40		5-38,	
%OBW			Average ONCE/SLIDE		
				5-27,	
[Numorice]				5-29,	
[Numerics]	5.60	5 62		5-32,	5-36,
0.5 dB/div				5-38,	5-40,
1 dB/div				5-43,	5-44,
1/Delta Mkr ON/OFF				5-45	
10 dB/div		5-63	Average PAUSE/CONT	5-36,	5-38,
110 CS (CS-IF Band)				5-40,	5-43,
2 Channel ON/OFF				5-44	
2 Channel Preset			Average Power	5-25,	5-29
2 Channels Viewer			Average START/STOP		
2 dB/div			•	5-39,	
5 dB/div	5-62,	5-63		5-44	
			Averaging ON/OFF	5-25,	5-26,
[A]				5-27,	
A-B→A	5 12	5 16		5-29,	
A-B→A A-B→B				5-32	,
A-B→B A-B→C				0 02	
		3-40	rp:		
About Parlagement of Limited Life Parts			[B]		
About Replacement of Limited-Life Parts			B-A→A		
Accessories		5.20	B-A→B		
ACP			B-A→C		
A-DL→A			Bands Definition	5-26,	5-33,
All Auto		5-73		5-34	
AMPLITUDE			Bandwidth	6-28	
Amplitude		7-7,	Basic Measurement	4-13	
	7-11		Basic Operation	4-10	
Amplitude Accuracy		7-8,	Basic Steps for GPIB Bus Control	6-55	
	7-12		B-DL→B	5-43,	5-46
Annotations ON/OFF	-	5-9	Black and White	5-8,	5-12
APPLI			Blank	5-43,	5-44
Arrangement of the three status registers			Buffers	6-10	
AT Command Index					
AT Command List	6-25		IC1		
ATT			[C]	0.1	
ATT AUTO/MNL			Cabinet Cleaning		c 44
Attenuation 0 dB	5-62		Calc		
Auto		5-73	Calibrate ALL		
Auto Inc Index	,	5-13	Calibration		
Auto Inc ON/OFF	5-8,	5-13	G 111	5-11,	
Auto name Index	5-18,	5-20	Calibration Corrections ON/OFF		
Auto Tune			Calibration F Int Ref		5-11
Auto-name Radix	5-18,	5-20	Capture Normz Data		
Average			Carrier Bandwidth		5-31,
-	5-45			5-32	
Average Control	5-25,	5-26,	CATV		
-	5-27,		Caution when Connecting Peripherals		
	5-29,		Center	5-57	

Center CH ON/OFF		5-58	Couple to Line 2 OFF/ABV/BLW	5-47,	5-50,
CF Step Size AUTO/MNL				5-51	
Ch Windows ON/OFF	5-26,	5-31,	Couple to Win OFF/IN/OUT	5-47,	5-50,
	5-32			5-51	
Channel Definition	5-26,	5-31	CPL		
Channel Input			CPL (Coupled function)	5-72	
Channel Position	5-25,	5-27			
Channel Power	5-25,	5-27	[D]		
Channel Width	5-25,	5-27	Data format	6 12	
Channels Config	5-57,	5-58	Date Time		5 12
Charging the Battery	3-7		dB Conversion Formula		3-12
Cleaning			dB/div		5 63
Cleaning of Other Parts	9-2		dBc/Hz ON/OFF		
Clear All	5-47,	5-48			
Clear Others	5-47,	5-48	dBm		
CN Measurement in Terrestrial Digital			dBm/Hz ON/OFF		
Broadcasting	4-51		dBmV		
Coarse		5-11	dBμV		
Color Mode Color/Gray	5-8,	5-15	dBμV/sqrt(Hz) ON/OFF		
Color Pattern		5-12	dBμVemf		
Color1		5-12	dBpW		5-63
Color2		5-12	DC Power Requirements		
Command Reference Syntax			Default		
Command Syntax			Default Conditions		
Common Commands					5-28,
Condition Register					5-30,
Config		5-31,			5-34,
Č		5-47,		5-35,	5-36,
	5-50,	,	D 1	5-39	5 66
Config Driver	5-8,	5-15	Delay		
Connecting the DC Power Cable			Delete		
Contents of This Manual			Delete Band		5-33,
Context A/B	5-66,	5-70,		5-35	5 21
	5-71	•	Delete Channel		
Context RF2 RF1	5-17,	5-18	Delete Entry		
Continuous Down ON/OFF				5-52,	5-65,
Continuous Peak ON/OFF	5-47,	5-50	D. L. T.	5-69	5 50
Control from a Controller			Delete Line		
Conventions of Notation Used in This			Delta Mode	5-4/,	5-48
Document	1-2		Delta ON/OFF		
COPY			Delta Ref Line ON/OFF		5-56
Copy		5-13	Delta to CF		
Copy All to Flash			Delta to CF Step		
Copy All to USB			Delta to Mkr Step		
Copy Config			Delta to Span	5-54	
Copy Device FILE/PRT			Destination and Phone Number for		
Correction Factor ON/OFF			Contact		
Counter			Det Avg Mode RMS/Video		5-45
Counter Position		5-40	Details of the three status registers		
Couple to DL OFF/ABV/BLW			Detector	,	
•	5-51	,	Detector AUTO/MNL		5-45
Couple to Line 1 OFF/ABV/BLW	5-47.	5-50,	Display		- AC
	5-51	,	Display Line ON/OFF		
	- '			5-47,	5-50,

	5-51, 5-65,	File Control	5-8, 5-14,
	5-69		5-18, 5-19
Display List ON/OFF	5-47, 5-48,	File Format BIN/XML	
	5-50, 5-53	File Format PNG/BMP	5-8, 5-13
Display REL/ABL/ABR		File Management	6-50
Disposal and Recycle	9-10	File Output to USB Memory	
Dynamic Range	7-4, 7-8,	Fine	
	7-13	Fixed Mkr ON/OFF	5-47, 5-48
		FM Meas	5-37, 5-41
[E]		Format	
Each Item	5-7 5-11	Format Media	
Edit Channel Formula		Formula 1 ON/OFF	
Edit Channel Table		Formula 2 ON/OFF	
Edit Corr Factor		Formula 3 ON/OFF	
Edit Date Time		Free Run	
Edit Limit Lines		Freq Input Mode CALC/TABLE	
Edit Ellint Ellies	5-47, 5-50, 5-52	Freq vs Time	
Electromagnetic Interference		Freq vs Time ON/OFF	
EMC		Freq Zoom	
EMC Filter ON/OFF	,	FREQUENCY	5-57
Enable Register		Frequency	6-25, 7-2,
Error Messages			7-6, 7-10
Event Enable Register		Frequency Correction ON/OFF	
Event Register		Frequency Counter	
Example of Remote Control Programs		Frequency Offset ON/OFF	
Example Program for Screen Image	0-33	Frequency Pos	
Output	6-70	Frequency Reference	
Example Programs in which SCPI	0-70	Frequency Reference INT/EXT/XTL	
Commands Are Used	6-108	Frequency Zoom ON/OFF	
EXAMPLE REMOTE CONTROL	0-100	Front Panel	4-1
PROGRAMS	6.55	Full Span	5-61
Execute ON/OFF		Functional Descriptions	
Laceute ON/OTT	5-23, 5-26, 5-27, 5-28,	FUNCTIONAL EXPLANATION	
	5-27, 5-26, 5-29, 5-30,	Fundamental ON/OFF	5-36, 5-40
	5-32, 5-34,		
	5-36, 5-37,	[G]	
	5-38, 5-39,	Gate Delay	5-65 5-67
	5-40, 5-41	Gate Width	5-65, 5-67
Execute Self Test	· ·	Gated Sweep	
Execute X dB Down		Gated Sweep ON/OFF	
Execute X dB Left		General Specifications	
Execute X dB Right		Glossary	
EXT CFG		GPIB	
EXT CFG (Extended Configuration	5 05	GPIB Address	
options)	5-65	GPIB Bus Functions	
Ext Trigger Level		GPIB Interface Functions	
External		GPIB Remote Control System	
External DC Power Supply		GPIB Remote Programming	
Zittinui De Ferrei Suppiy	2.0	Graph ON/OFF	
FF-1		Graphic	
[F]		Graphic Z 1 Screen	
Factory Init		Graphic Z 2 Screens	
FILE	5-18	Graphic Zoom 1 ON/OFF	

Graphic Zoom 2 ON/OFF	5-66, 5-70	Line 1 ON/OFF		
		Line 2 ABV/BLW		
[H]		Line 2 ON/OFF		
Hard Copy Output	4-27	Link to Marker ON/OFF		5-40
Harmonic		List of Commands	6-79	
Harmonic Max Order		Locating This Instrument	3-3	
Header				
High Sensitivity ON/OFF		[M]		
How to Cancel an UNCAL Message		MAINTENANCE	9-1	
The water and entering the sough	. 22	Marker		
		Marker ON/OFF		5-48
[1]		Marker Trace A/B/C	5-47	5-48
Identifying an Image Signal		Math		
IF		Max Hold		
If a Fault Occurs		Max Hold Continuous		
Image Suppression ON/OFF		Max Order		
In Case of Difficulty		Max Sweep Count		
Init Table		wax sweep count		5-28,
	5-33, 5-35,			5-20,
	5-62, 5-64			5-36,
Initial Setting List	A-1			5-39,
Input and Output	7-5, 7-9,		5-43,	
	7-14	MEAS 1	-	3-44
Input Impedance 50/75		MEAS 2		
Input Saturation	A-4	Measurement		
Insert	5-62, 5-64	Measurement Examples		
Insert Band	5-26, 5-35	-	4-3/	
Insert Channel	5-26, 5-31	Measuring by using the TG	4.20	
Insert Entry	5-47, 5-50,	(OPT76/OPT77)		5 67
•	5-52, 5-65,	Measuring Window		
	5-69	Media		
Insert Line	5-57, 5-59	Medium	5-18,	
Inspection on Delivery	3-1			3-73
INSTRUMENT CONFIGURATION		Menu Index		
AND BASIC OPERATIONS	4-1	MENU MAP		5 1 4
Intermod	5-36, 5-38	Menu ON/OFF		5-14,
INTRODUCTION	1-1	Mana On antian and Data Foton	5-15	
Items	5-18, 5-21	Menu Operation and Data Entry		
		Message Exchange		
ri 1		Message Exchanging Protocol		
[L]	6.70	Method of Storing the Instrument		
LAN		Min ATT		5 4 4
LAN IP Address		Min Hold		
LAN Remote Control System		Min Max Peak		5-50,
Last Span		N. D. 1	5-52	5 50
Level		Min Peak		5-50,
	6-27		5-52	
Limit Line 1/2		MKR		5 40
	5-52, 5-65,	Mkr Step AUTO/MNL		5-48
	5-69	Mkr to CF		
Limit Line Edit		Mkr to CF Step		
Limit Lines		Mkr to Mkr Step		
Limit Setup		Mkr to Ref		
Line 1 ABV/BLW	5-65, 5-68	MKR→	5-54	

Mod. Freq to Sweep Time ON/OFF		Option 15 75 Ω Input	7-18
Mode FULL/CARR	*	Option 20 High Stability Frequency	
Mode Index/Value	*	Reference	
More 1/2		Option 28 EMC Filter	
	5-18, 5-20,	Option 53 Time Domain Analysis	7-20
	5-36, 5-38,	Option 54 2-Channel Time Domain	
	5-40, 5-43,	Analysis	7-20
	5-46, 5-47,	Option 55 Broadband Time Domain	
	5-48, 5-50,	Analysis	7-21
	5-52, 5-54,	Option 56 2-Channel Broadband Time	
	5-57, 5-60,	Domain Analysis	7-21
	5-62, 5-63,	Option 70 High C/N	7-21
	5-72, 5-73	Option 71 2-Channel High C/N	7-21
		Option 75 75 Ω Tracking Generator	7-23
[N]		Option 76 Tracking Generator	
Narrow	5 72 5 73	Option 77 6 GHz Tracking Generator	7-25
		Options	
Nega		OPTIONS AND ACCESSORIE	8-1
Next Band		Others	6-52
Next Min Peak		Others HIDE/SHOW	5-47, 5-48
Naut Daal	5-52	Output to a Printer	4-27
Next Peak	*	-	
Next Peak Left	*	[P]	
Next Peak Right			4 1
Noise/Hz		Panel and Screen Descriptions	
Noise/x Hz		Paper Format	
Normal		Parser AT/SCPI	
Normalize		Pass/Fail	
Normalize Correction ON/OFF		Pass/Fail Config	
Note when Turning on the Power	2-1	Pass/Fail ON/OFF	
Notes for Requesting Repair,		D. T.	5-65, 5-68
Replacement of Parts, and Periodic	0.2	Pause Time	
Calibration		PBW	
Nyq Roll Off Factor		PEAK	
N. C. LID.	5-33	Peak	
Nyq Symbol Rate		Peak + X dB Down	,
N P.11. ON OFF	5-33	Peak and Marker Move	
Nyquist Filter ON/OFF		Peak Delta Y	
	5-32	D 11:45	
		Peak List Frequency	
[O]		D 11'41 1	5-52
OBW	5-25, 5-30	Peak List Level	
OFF		D 114	5-53
On Trace A/B/C		Peak Menu	
	5-27, 5-28,	Peak to CF	
	5-29, 5-30,	Peak to Ref	
	5-32, 5-34,	Peak Zoom	
	5-36, 5-38,	PLL BW	
	5-40	Posi	
Operating Environment		Power	
Option 10 2-Channel Input		Power Average	
Option 11 75 Ω 2-Channel Input	-	Power Supply	3-4
(Can be Installed only in the U3741)	7-17	PRECAUTIONS WHEN USING THE	
()	· - ·	U3700	2-1

Preset	6-51	Resolution 10 Hz	5-36, 5-40
Previous Band		Resolution 100 Hz	
Principle of Operation		Responses to Interface Messages	
Print Config		Restore Defaults	
Product Overview			5-27, 5-28,
Program Examples Using VB			5-29, 5-30,
			5-32, 5-34,
[0]			5-35, 5-36,
[Q]			5-39
Quasi Peak		Results	
QUICK GUIDE	GUIDE-1	Root Nyquist Filter	
		Round Grid Values ON/OFF	
[R]		110414 0114 (4145 01 (011 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1	0 02, 0 0.
R3131 Mode ON/OFF	5-7, 5-11	[S]	
R3162 Mode ON/OFF	5-7, 5-10		5 42 5 45
Range FULL/WIN		Sample	
RBW 1 MHz		Satellite Broadcasting (BS-IF Band)	
RBW 120 kHz	5-72	Save	
RBW 200 Hz	5-72	Save as	
RBW 9 kHz		Save Defaults	
RBW Auto			5-27, 5-28,
RBW AUTO/MNL			5-29, 5-30,
RBW CAL			5-32, 5-34,
Reading Data			5-35, 5-36,
Reading the GPIB Control Library for	0.50		5-39
Visual Basic	6-55	Save/Recall	
Rear Panel		SCPI Command Reference	
Recall		Screen	
Ref Freq	*	Screen Shot Config	
Ref Freq 10 MHz		Select	
Ref Level		Select Marker	
Ref Object			5-50
Ref Offset ON/OFF		Selecting the Command Set	
Ref Power CHN/PEAK		Self Test	
Ref/Disp Lines		Setting the IP Address	
Reference Line		Setting up the GPIB	
Reference Line ON/OFF		Setting up the LAN	6-6
Reference Line ON/OTT	5-65, 5-69	SETUP	
Reference Marker		Shift X ON/OFF	5-65, 5-68
Refresh		Shift Y ON/OFF	
Refresh(Write)		Show Mask ON/OFF	
· · · · · · · · · · · · · · · · · · ·		Show ON/OFF	
Remote Control	5-7, 5-10, 6-1	Signal Identification ON/OFF	5-57, 5-60
Domario Eilo		Signal Track	5-47, 5-49
Remove File		Signal Track ON/OFF	5-47, 5-49
Domestine the Cose	5-18, 5-19	Slide Screen ON/OFF	5-62, 5-63
Removing the Case		Slope NEG/POS	
Rename File			5-67
Dan art HIDE/CHOW	5-18, 5-19	Sound	5-37, 5-41
Report HIDE/SHOW		Sound AM/FM	
Reset Context		Source	
Resolution			5-67
Resolution 1 Hz		SPAN	5-61
Resolution 1 kHz	5-30, 5-40	Span	5-61

SPAN/RBW ON/OFF		Television Signal Measurement		
SPECIFICATIONS		Terrestrial Digital Broadcasting		
Spectrum Analyzer		TG		6-53
Spectrum Emission		TG (Option)		
Spectrum RF1		TG Freq. Offset ON/OFF		
Spectrum RF2		TG Level		
Spurious		TG Level Offset ON/OFF		
Standard Event Register		TG ON/OFF		5.5 0
Standard Operation Status Register		Time vs Time		
Start		Title		
Start CH Offset ON/OFF		Total Gain RF Path 1		
Start CH ON/OFF		Total Gain RF Path 2		
Status Byte		Total Power		5-28
Status Byte Register		TRACE		
Status Register		Trace		5 4 A
Step ATT CAL		Trace A/B/C		
Stop				5-46,
Stop CH Offset ON/OFF		Turan Data	5-55,	5-56
Stop CH ON/OFF		Trace Data		<i>7</i> 11
Store		Trace Points 501/1001	-	5-11
C. I	5-43, 5-46	Transportation		5.46
Subsystem-CALCulate		$TRC \rightarrow A$		
Subsystem-CALibration		TRC→B		
Subsystem-CONFigure		TRC→C		
Subsystem-COUPle		Trigger		5-66,
Subsystem-DISPlay		TG (T-1 - G) 1	6-29	
Subsystem-FETch		TV Changel Table (Janear)		
Subsystem-FORMat		TV Channel Table (Japan)		
Subsystem-HCOPy		Types of Systems	0-1	
Subsystem-INITiate				
Subsystem-INPut		[U]		
Subsystem-MMEMory		U3741 Performance Specifications	7-2	
Subsystem-OUTPut		U3751 Performance Specifications	7-6	
Subsystem-READ		Unit	6-12	
Subsystem-SOURce		Units	5-62,	5-63,
Subsystem-SYSTem			6-54,	6-107
Subsystem-TRACe		USER Key	4-36	
Subsystem-TRIGger		User Password	5-8,	5-12
Subsystem-UNIT		Using a Battery	3-6	
· · · · · ·		Using the Normalize Function and		
Subtract	5-43, 5-46	Using the Normalize Function and Level Correction Table	4-37	
· · · · · ·	5-43, 5-46 6-29, 7-3,		4-37	
Subtract	5-43, 5-46 6-29, 7-3, 7-7, 7-11	Level Correction Table	4-37	
Sweep Mode SGL/CNT	5-43, 5-46 6-29, 7-3, 7-7, 7-11 5-65, 5-66	Level Correction Table[V]		
Sweep Mode SGL/CNT	5-43, 5-46 6-29, 7-3, 7-7, 7-11 5-65, 5-66 5-72	Level Correction Table [V] VBW AUTO/MNL	5-72	5-73
Sweep Mode SGL/CNT	5-43, 5-46 6-29, 7-3, 7-7, 7-11 5-65, 5-66 5-72	Level Correction Table	5-72 5-72,	
Sweep Mode SGL/CNT Sweep Time AUTO/MNL SYSTEM	5-43, 5-46 6-29, 7-3, 7-7, 7-11 5-65, 5-66 5-72	Level Correction Table [V] VBW AUTO/MNL VBW/RBW ON/OFF Version	5-72 5-72, 5-7,	5-9
Sweep Mode SGL/CNT Sweep Time AUTO/MNL SYSTEM	5-43, 5-46 6-29, 7-3, 7-7, 7-11 5-65, 5-66 5-72 5-7	Level Correction Table [V] VBW AUTO/MNL VBW/RBW ON/OFF Version Vertical Scale LIN/LOG	5-72 5-72, 5-7, 5-62,	5-9
Sweep Mode SGL/CNT Sweep Time AUTO/MNL SYSTEM	5-43, 5-46 6-29, 7-3, 7-7, 7-11 5-65, 5-66 5-72 5-7	Level Correction Table [V] VBW AUTO/MNL VBW/RBW ON/OFF Version Vertical Scale LIN/LOG VHF/UHF	5-72 5-72, 5-7, 5-62, A-29	5-9 5-63
Sweep Mode SGL/CNT Sweep Time AUTO/MNL SYSTEM	5-43, 5-46 6-29, 7-3, 7-7, 7-11 5-65, 5-66 5-72 5-7 5-47, 5-50, 5-52, 5-57,	Level Correction Table [V] VBW AUTO/MNL VBW/RBW ON/OFF Version Vertical Scale LIN/LOG VHF/UHF Video	5-72 5-72, 5-7, 5-62, A-29 5-65,	5-9 5-63 5-66
Sweep Mode SGL/CNT Sweep Time AUTO/MNL SYSTEM	5-43, 5-46 6-29, 7-3, 7-7, 7-11 5-65, 5-66 5-72 5-7 5-47, 5-50, 5-52, 5-57, 5-59, 5-65,	Level Correction Table [V] VBW AUTO/MNL	5-72 5-72, 5-7, 5-62, A-29 5-65, 5-43,	5-9 5-63 5-66 5-44
Sweep Mode SGL/CNT	5-43, 5-46 6-29, 7-3, 7-7, 7-11 5-65, 5-66 5-72 5-7 5-47, 5-50, 5-52, 5-57, 5-59, 5-65, 5-69	Level Correction Table [V] VBW AUTO/MNL	5-72 5-72, 5-7, 5-62, A-29 5-65, 5-43, 5-62,	5-9 5-63 5-66 5-44 5-63
Sweep Mode SGL/CNT Sweep Time AUTO/MNL SYSTEM	5-43, 5-46 6-29, 7-3, 7-7, 7-11 5-65, 5-66 5-72 5-7 5-47, 5-50, 5-52, 5-57, 5-59, 5-65, 5-69	Level Correction Table [V] VBW AUTO/MNL	5-72 5-72, 5-7, 5-62, A-29 5-65, 5-43, 5-62,	5-9 5-63 5-66 5-44 5-63

VSWR Measurement	4-59	
VSWR ON/OFF	5-55,	5-56
[W]		
Watts	5-62,	5-63
W-CDMA Adjacent Channel Leakage		
Power (ACP) Measurement	4-45	
W-CDMA Channel Power Measurement		
White and Black	5-8,	5-12
Window	5-25,	
Window HIDE/SHOW		
Window Position	5-25,	5-29
	5-47,	5-50
	5-51,	5-65
	5-66,	5-67
	5-69,	5-70
Window Sweep ON/OFF	5-65,	5-67
Window Width	5-25,	5-29
	5-47,	
	5-51,	
	5-66,	
	5-69,	5-70
Work Request	9-3	
Write	5-43,	
Write Protect ON/OFF		
	5-18,	5-19
ſ Y 1		
[X]	5 (5	5 (0
X ABS/CF/FA	5-65,	5-08
X dB Down	5-36,	5-37
X dB Level	5-30,	5-5/
X-Search Domain	5-47,	5-50
[Y]		
Y ABS/REF/DL	5-65	5-68
Y Range ON/OFF		
Y- Search Domain		
	<i>E E</i> 1	
[Z]	5 (1	
Zero Span	5-61	5 60
Zoom and Contexts	5-65,	5-69
Zoom Position		
Zoom Width	5-66,	5-70

ADVANTEST_®

ADVANTEST CORPORATION

U3700 Series OPT10/OPT11 2 Channel Input Option User's Guide

MANUAL NUMBER FOE-8440267C00

Applicable Models U3741 U3751 U3771 U3772

TABLE OF CONTENTS

1.	INTRODUCTION
1.1	Contents of This Manual
1.2	Product Overview
2.	INSTRUMENT CONFIGURATION AND BASIC OPERATIONS 2
2.1	Panel and Screen Descriptions
2.1.1	Names and Functions of Each Part on the Front Panel
2.1.2	Names and Functions of Each Part on the Screen
2.2	Basic Operation
2.2.1	Selecting Active Channel
2.2.2	Switching Two Channel Display Modes
2.2.3	Synchronizing Channels 1 and 2
2.2.4	Switching to Single Channel Mode
2.2.5	Example of Operation
2.2.6 2.3	Note when Displaying 2 Screens
2.4	Measurement Example 2-
2.4.1	W-CDMA Signal Channel Power Measurement and
2.4.2	Adjacent Channel Leakage Power (ACP) Measurement
2.4.2	Characteristics Evaluation of Frequency Converter2-
3.	MENU MAP AND FUNCTION DESCRIPTION
3.1	Menu Index
3.2	Restrictions
3.3	Functional Descriptions
3.3.1	APPLI
3.3.2	EXT CFG
3.3.3 3.3.4	TRACE
3.3.5	MKR
3.3.6	System
5.5.0	System
4.	OVERVIEW OF REMOTE CONTROL
4.1	Status Byte
4.2	Operation of TS command at Dual CH
4.3	GPIB Remote Programming
4.4	AT Command Code List
4.4.1	APPLI (Mode setting)
4.4.2	Sweep
4.4.3	Trigger
4.4.4	Trace
4.4.5	Marker
4.4.6	TG
4.4.7	Save/Recall

U3700 Series OPT10/OPT11 User's Guide

Table of Contents

4.4.8	Calibration	
4.4.9	GPIB	
4.5	Example Program for Remote Control	4
4.5.1	Access Channel Example Program	
4.6	SCPI Command Code List	4
4.6.1	APPLI (Mode setting)	
4.6.2	Sweep	
4.6.3	Trigger	
4.6.4	Trace	
4.6.5	Marker	
4.6.6	TG	
5.	SPECIFICATIONS	
5.1	Option 10 2-Channel Input	
5.2	Option 11 75 Ω 2-Channel Input (Can be Installed only in the U3741)	
6.	LIST OF ERROR MESSAGES	
ALPI	HABETICAL INDEX	

LIST OF ILLUSTRATIONS

No.	Title	Page
2-1	Front Panel	2-1
2-2	U3741 + OPT10/OPT11 Input and Output Connectors Block	2-2
2-3	U3751 + OPT10 Input and Output Connectors Block	2-3
2-4	U3771/U3772 + OPT10 Input and Output Connectors Block	2-4
2-5	Screen Display of DUAL CH ON 2 Screens	2-5
2-6	Screen Display when DUAL CH OFF	2-6
2-7	Initial Setting Screen	2-18
2-8	Connecting the CAL Signal (Channel 1)	2-19
2-9	Connecting the CAL Signal (Channel 2)	2-20
4-1	Status Registers	4-1

LIST OF TABLES

No.	Title	Page
1-1	OPT10 Standard Accessories	1-2
1-2	OPT11 Standard Accessories	1-2
4-1	Standard Operation Status Register	4-2

1. INTRODUCTION

This chapter describes the content of this manual and the product overview of the U3700 series spectrum analyzer two channel input option (OPT10/OPT11) to help the user get the most out of this guide.

For more information on the basic descriptions, refer to "U3700 Series User's Guide."

1.1 Contents of This Manual

The contents of each chapter are as follows:

CHAPTER 1. INTRODUCTION	This chapter describes the contents of this manual and the product overview.
CHAPTER 2. INSTRUMENT CONFIGURATION AND BASIC OPERATIONS	This chapter describes an example of measurement.
CHAPTER 3. MENU MAP AND FUNCTION DESCRIPTION	This chapter describes the menu structure and functions of soft keys.
CHAPTER 4. OVERVIEW OF REMOTE CONTROL	This chapter describes commands for the AT and SCPI command reference in order of functions for the added and changed items in options 10 and 11. Contents are as follows: • Function description • Parameter • Query reply
CHAPTER 5. SPECIFICATIONS	This chapter describes options 10 and 11 specifications.
CHAPTER 6. LIST OF ERROR MESSAGES	This chapter describes additional error messages for options 10 and 11.

1.2 Product Overview

1.2 Product Overview

The two channel input option (OPT10) expands the RF measurement input of the U3700 series spectrum analyzer to two inputs. The measurement frequency range of the input channels to be added is 9 kHz to 3 GHz.

	Measurement frequency range	
Model name	Channel 1	Channel 2
U3741	9 kHz - 3 GHz	9 kHz - 3 GHz
U3751	9 kHz - 8 GHz	9 kHz - 3 GHz
U3771	10 MHz - 31.8 GHz	9 kHz - 3 GHz
U3772	10 MHz - 43 GHz	9 kHz - 3 GHz

The 75 Ω two channel input option (OPT11) uses channels 1 and 2 as 75 Ω impedance input. OPT11 can only be set on the U3741.

Features

• Two channel independent setting operations

Channels 1 and 2 operate under independent setting conditions.

Two different signals can be measured at the same time as though two spectrum analyzers are used.

Also, measurements including OBW and ACP measurements can be performed at each channel independently.

Synchronous operation of two channel setting conditions

Channels 1 and 2 operate under the same setting conditions.

By using the setting condition copy function, the same setting conditions can be specified for both channels easily.

The Couple CH function enables settings to both channels at the same time by a single key operation.

• Two channel synchronous sweep function

Measurement for both channels can be started at the same time without using an external trigger signal. Time interval measurement between channels can be performed.

Table 1-1 OPT10 Standard Accessories

Name	Model	Quantity	Remarks
N(m)-BNC(f) adapter	JUG-201A/U	1	
U3700 Series OPT10/OPT11 User's Guide	EU3700OPT10	(1)	Included on the U3700 CD-ROM manual.

Table 1-2 OPT11 Standard Accessories

Name	Model	Quantity	Remarks
Input cable (75 Ω)	A01045	1	
C15-type adapter	NCP-NFJ	2	
NC-BNC adapter	BA-A165	2	
U3700 Series OPT10/OPT11 User's Guide	EU3700OPT10	(1)	Included on the U3700 CD-ROM manual.

2. INSTRUMENT CONFIGURATION AND BASIC OPERATIONS

This chapter describes the added or changed items of OPT10 and OPT11 on the panel, functions of each part on the screens, and basic operations of this instrument.

2.1 Panel and Screen Descriptions

This section describes the front panel, screen displays, and names and functions of each part.

2.1.1 Names and Functions of Each Part on the Front Panel

This section describes the names and functions of each part on the front panel.

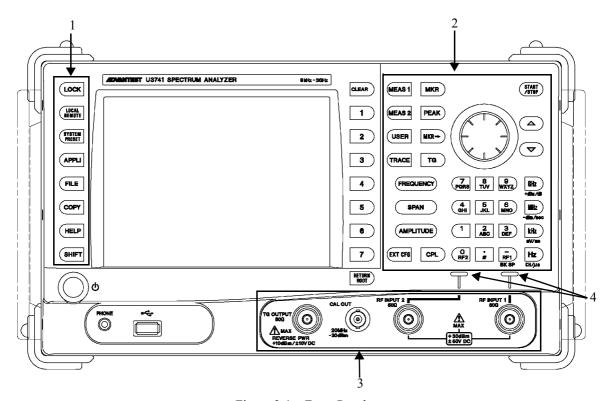


Figure 2-1 Front Panel

- 1. Extended function key block The keys in this block set the extended functions. Specifies common settings regardless of channels.
- 2. Operation key block The keys in this block are used to change settings. Specifies settings for each channel independently.
- 3. Input and output connectors block The input and output connectors in this block are used for measurements.
- 4. Input connector lamp Indicates an active channel by illumination.

2.1.1 Names and Functions of Each Part on the Front Panel

U3741 + OPT10/OPT11 Input and output connectors block

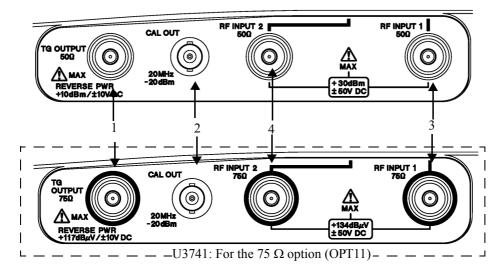


Figure 2-2 U3741 + OPT10/OPT11 Input and Output Connectors Block

1.	TG OUTPUT connector	Outputs the tracking generator signal. (Option)
2.	CAL OUT connector	Outputs the calibration signal.
3.	RF INPUT 1 connector (Channel 1)	Inputs the signal to be measured. Measurement frequency range: 9 kHz - 3 GHz
4.	RF INPUT 2 connector (Channel 2)	Inputs the signal to be measured. Measurement frequency range: 9 kHz - 3 GHz

CAUTION:

- 1. Do not apply an RF power or DC voltage that exceeds the limited value to the INPUT and OUT connectors.
- Be careful of static electricity. Internal circuit components such as the input attenuator and mixer may be damaged.
- 3. For the 75 Ω option (OPT11), input and output connectors are changed to 75 Ω type connectors. If a 50 Ω cable or connector is connected to a 75 Ω connector, the center contact of the 75 Ω connector may be damaged. Verify that cables and connectors, which are used, are 75 Ω type.

2.1.1 Names and Functions of Each Part on the Front Panel

U3751 + OPT10 Input and output connectors block

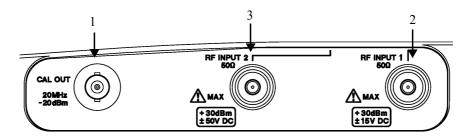


Figure 2-3 U3751 + OPT10 Input and Output Connectors Block

1.	CAL OUT connector	Outputs the calibration signal.
2.	RF INPUT 1 connector (Channel 1)	Inputs the signal to be measured. Measurement frequency range: 9 kHz - 8 GHz
3.	RF INPUT 2 connector	Inputs the signal to be measured.
	(Channel 2)	Measurement frequency range: 9 kHz - 3 GHz

CAUTION:

- Do not apply an RF power or DC voltage that exceeds the limited value to the INPUT and OUT connectors. DC voltage tolerances of INPUT 1 and INPUT 2 are different. RF INPUT 1: ±15V DC

 - RF INPUT 2: ±50V DC
- Be careful of static electricity. Internal circuit components such as the input attenuator and mixer may be damaged.

2.1.1 Names and Functions of Each Part on the Front Panel

U3771/U3772 + OPT10 Input and output connectors block

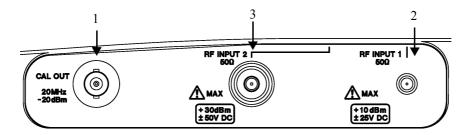


Figure 2-4 U3771/U3772 + OPT10 Input and Output Connectors Block

1.	CAL OUT connector	Outputs the calibration signal.
2.	RF INPUT 1 connector	Inputs the signal to be measured.
	(Channel 1)	Measurement frequency range: 10 MHz - 31.8 GHz (U3771) 10 MHz - 43 GHz (U3772)
3.	RF INPUT 2 connector	Inputs the signal to be measured.
	(Channel 2)	Measurement frequency range: 9 kHz - 3 GHz

CAUTION:

- Do not apply an RF power or DC voltage that exceeds the limited value to the INPUT and OUT connectors.
 DC voltage tolerances of INPUT 1 and INPUT 2 are different.
 RF INPUT 1: ±25V DC
 RF INPUT 2: ±50V DC
- 2. Be careful of static electricity. Internal circuit components such as the input attenuator and mixer may be damaged.
- 3. The precision microwave connector is used as the RF INPUT 1 connector. This connector is compatible with the K connector (K connector is a trademark of Anritsu Corporation.) and can be connected to a common SMA connector. Be careful when handling this connector because the connector is delicate and is damaged easily. Use the included adapter (HE-A-PJ) if the connection and disconnection to this connector are performed frequently.

2.1.2 Names and Functions of Each Part on the Screen

2.1.2 Names and Functions of Each Part on the Screen

This section describes the names and functions of the screens regarding OPT10.

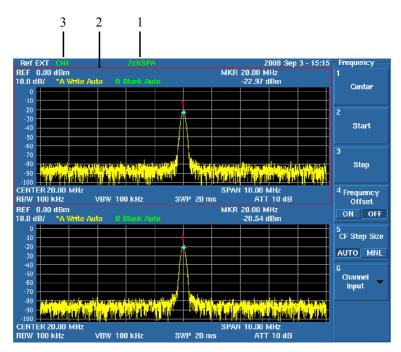


Figure 2-5 Screen Display of DUAL CH ON 2 Screens

Operation mode When DUAL CH ON: Displays 2chSPA. When DUAL CH OFF: Nothing is displayed.

Active channel display Indicates the active channel, where settings can be changed, by

using the red rectangular box.

Active channel display Channel 1: CH1 Channel 2: CH2 Couple CH ON: CPL

2.1.2 Names and Functions of Each Part on the Screen

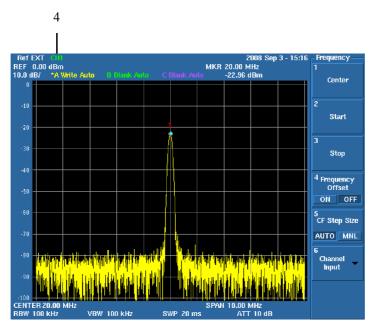


Figure 2-6 Screen Display when DUAL CH OFF

4. Operating channel

Indicates the selected operating channel.

2.2 Basic Operation

This section describes the menu operations, data entry, and usage of the basic measurement functions.


Panel key operation

Extended function key: Specifies common settings regardless of channels.

Operation key: Specifies settings for each channel independently.

As an exception, the USER key is common regardless of chan-

nels.

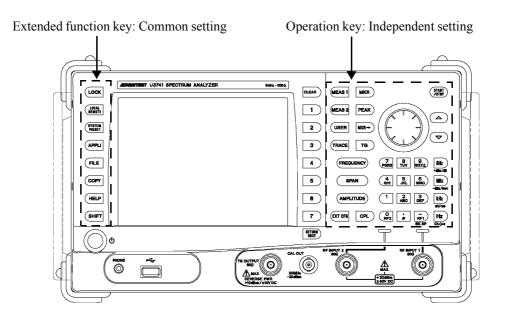


2.2.1 Selecting Active Channel

2.2.1 Selecting Active Channel

The active channel is the target channel for changing settings.

There are two methods to select the active channel.

1. Use the **SHIFT** key + -(RF1) or **SHIFT** key + **0** (RF2).

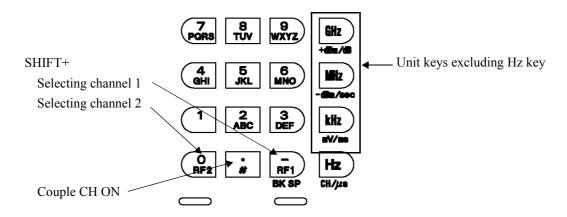

• RF1 Activates channel 1.

• RF2 Activates channel 2.

• # Sets the Couple CH mode ON.

Activates both channels 1 and 2.

Key operations for **FREQUENCY**, **SPAN**, and **CPL** become enabled for both channel settings (except some functions).

2. Unit keys excluding Hz key is used.

If a unit key is pressed when the setting input was complete, the active channels switch.

Example: If the active channel is CH1, press **FREQUENCY**, **1**, and **GHz**.

Set the center frequency of channel 1 to 1 GHz.

Press GHz (one of the unit keys).

The active channel is switched to channel 2.

Display regarding the active channel

1. Display the active channel on the top line of screen

CH1: Channel 1 is selected as the active channel.

CH2: Channel 2 is selected as the active channel.

CPL On: This mode enables settings for both channels.

2. The red rectangular box surrounds the active channel window.

Couple CH does not affect the rectangular display.

3. The front panel LED illuminates by corresponding to the active channel connector

When Couple CH is ON, both LEDs illuminate.

2.2.2 Switching Two Channel Display Modes

2.2.2 Switching Two Channel Display Modes

The display mode for two-channel measurement can be selected from the following two modes:

2 Screens
 Displays channel 1 in the upper window and channel 2 in the

lower window.

Full Screen Displays the specified channel full screen.

The displayed channel becomes active.

The function setting remains the same by switching the 2 Screens ⇔ Full Screen display.

2.2.3 Synchronizing Channels 1 and 2

The Couple CH function can change settings for both channels by a single key operation.

Also by using the Setup copy function, the same channel setting conditions can be set.

CAUTION:

When Setup copy is executed, data such as the ACP table, level correction table, and normalization data are copied with the setting conditions.

The table content at the copied destination is overwritten to the blank table at the copy source.

Also, there are some setting items which are not copied.

After the copy, specify the setting again or obtain the correction again, if necessary.

2.2.4 Switching to Single Channel Mode

DUAL CH ON/OFF switches the operation between two channels and a single channel.

In the 2 channel mode, both channels perform measurement regardless of the display mode.

In the single channel mode, only the selected channel operates.

CAUTION:

- 1. The following functions are canceled by switching Dual ON \Leftrightarrow OFF (single channel).
 - MEAS function
 - VSWR measurement
- 2. In the single channel mode, an independent setting can be performed for each channel. Even if the channel is switched, the setting remains.

(There are some common settings in channels 1 and 2 such as the Window setting.)

2.2.5 Example of Operation

2.2.5 Example of Operation

Required equipment

This instrument

Conversion adapter: N(m)-BNC(f) Input cable: BNC (m)-BNC (m) Signal generator: 20 MHz

Turn on the power and initialize the settings of this instrument.

Press SHIFT and SYSTEM(PRESET).

Initial setting conditions are loaded.

Connecting the input signal


Connecting the signal which is used for measurement.

Attach the N(m)-BNC(f) adapter to the RF INPUT connector on the front panel.

Connect the RF INPUT 2 connector (CH2) and the CAL OUT connector by using the supplied BNC (m)-BNC (m) cable.

Connect the RF INPUT 1 connector (CH1) to the signal generator.

Specify the setting so that a signal with a frequency of 20 MHz and a level of -20 dBm is output from the signal generator.

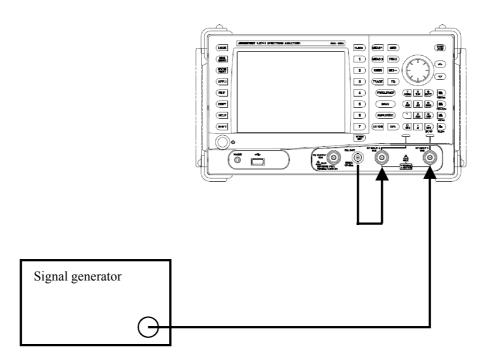

Setting measurement conditions Setting the active channel

1. Press **SHIFT** and 0 (RF2).

Channel 2 is selected.


The red rectangular box surrounds the channel 2 window. Also, CH2 is displayed on the top line of the screen.

2. Press FREQUENCY, 2, 0, and MHz.

The center frequency of channel 2 is set to 20 MHz.

3. Press SPAN, 1, 0, and MHz.

The frequency span is set to 10 MHz.

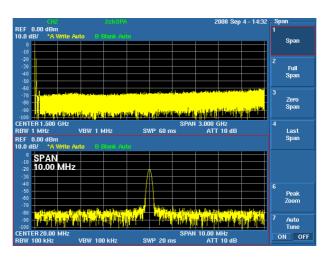


2.2.5 Example of Operation

Changing the two channel display mode

4. Press APPLI, Display, and Full Screen CH1.

Display channel 1 full screen.


Channel 1 becomes an active channel.

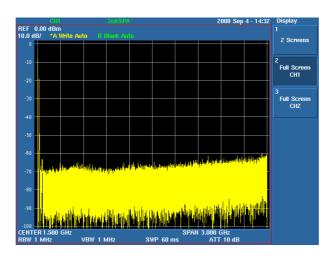

5. Press Full Screen CH2.


Display channel 2 full screen.

Channel 2 becomes an active channel.

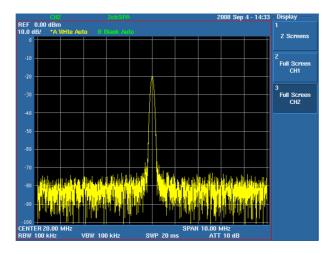

6. Press 2 Screens.


The screen returns to a two-screen display.

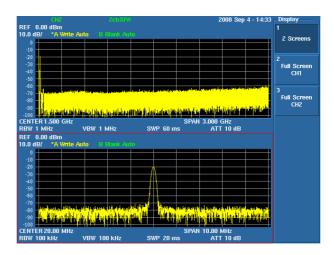

Synchronizing channels 1 and 2

7. Press **APPLI**, *Setup copy*, and *CH2>>CH1*.

The setting conditions of channel 2 are copied to channel 1, and channels 1 and 2 have the same settings.

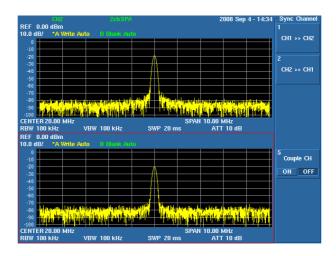

8. Press *Couple CH ON*.


The Couple CH mode turns ON and key operations are enabled for both channels.

NOTE: Only some functions of FREQUENCY, SPAN, and CPL keys are enabled.


The AMPLITUDE key only allows an independent setting even if the Couple CH mode is ON.

2.2.5 Example of Operation

9. Press **SPAN**, **1**, **MHz**, **CPL**, **RBW**, **△**, **FREQUENCY**, and **△**. Channel 1 and 2 settings are changed to the same setting.

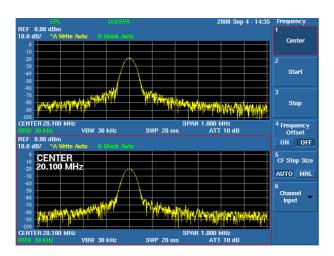


10. Press **AMPLITUDE**, *Ref Level*, **4**, **0**, and **GHz**. The Ref Level of only channel 2 is changed to 40 dBm.

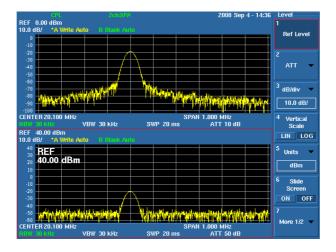

Switching to single channel mode

11. Press **APPLI**, *Return*, and *Dual CH ON/OFF (OFF)*. Channel 2, which is the active channel, is displayed full screen.

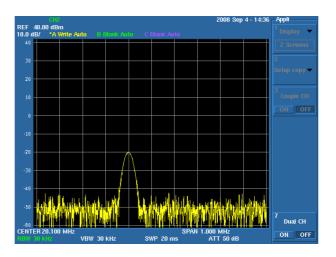


2.2.6 Note when Displaying 2 Screens

2.2.6 Note when Displaying 2 Screens

When a combination of the MEAS function and marker list is displayed at the same time, the result may not be displayed correctly because of the display area.


If this occurs, use Full Screen as shown below.

Example: 5th order harmonic measurement by using the Harmonics function




Display the maker list.

The measurement window is compressed.



Enlarge the result display area in the Full Screen display.



2.3 Calibration

2.3 Calibration

Correcting the measurement by using the calibration factor, which is acquired from the calibration, can increase the measurement accuracy.

IMPORTANT: Perform calibration after allowing a warm up time of 5 minutes or more.

Required equipment

OPT10

This instrument

Conversion adapter: N(m)-BNC(f)

Conversion adapter: BNC(f)-SMA(m) (U3771/U3772)

Input cable: BNC(m)-BNC(m)

OPT11

This instrument 75 Ω NC-BNC adapter

75 Ω input cable: BNC(m)-BNC(m)

Turning on the power

- 1. Verify that the AC power switch on the rear panel is set to OFF.
- 2. Connect the included power cable to the AC power connector on the rear panel.

CAUTION: To prevent damage, do not supply a voltage and frequency, which exceed the specified range, to this instrument.

- 3. Connect the power cable to a power outlet.
- 4. Turn on the AC power switch on the rear panel.
 After turning on the AC power switch, wait for three seconds or more.
- 5. Turn on the power switch on the front panel.

NOTE: The display may be different depending on the status when the power was last turned off.

CAUTION: Before turning the power on, remove the USB memory key. Otherwise, the system does not start.

2.3 Calibration

Initializing the setting

Initializing the settings of this instrument.

6. Press **SHIFT** and **SYSTEM(PRESET)**. Initial setting conditions are loaded.

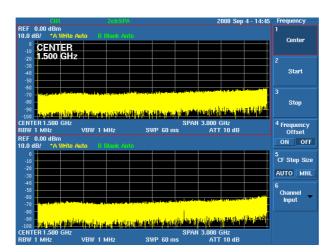


Figure 2-7 Initial Setting Screen

Selecting the input connector

Select the input to perform the calibration.

Press **SHIFT** and **- (RF1)**. RF INPUT 1 (channel 1) is selected. Press **SHIFT** and **0 (RF2)**. RF INPUT 2 (channel 2) is selected.

The calibration of either RF INPUT 1 or RF INPUT 2 can be performed first.

The following describes the procedure in which the calibration of RF INPUT 1 (channel 1) is performed first.

Connecting the input signal

Connecting the calibration signal which is used for measurement.

7. Attach the N(m)-BNC(f) adapter to the RF INPUT 1 connector on the front panel. Connect the included BNC(m)-BNC(m) input cable to the CAL OUT connector on the front panel and the N(m)-BNC(f) adapter.

For the U3771 and U3772, the BNC(f)-SMA(m) adapter is used.




Figure 2-8 Connecting the CAL Signal (Channel 1)

- 8. Press SYSTEM.
- 9. Press 6 Calibration.

The Calibration menu is displayed.

10. Press Calibrate All.

Calibration starts.

The following message is displayed if the calibration of RF INPUT 1 (channel 1) is complete.

The calibration is canceled if **Hz** is pressed.

To perform the calibration of RF INPUT 2 (channel 2), change the cable connection.

2.3 Calibration

11. Attach the BNC(f)-SMA(m) adapter to the RF INPUT 2 connector on the front

panel.
Connect the included BNC(m)-BNC(m) input cable to the CAL OUT connector on the front panel and the BNC(f)-SMA(m) adapter.

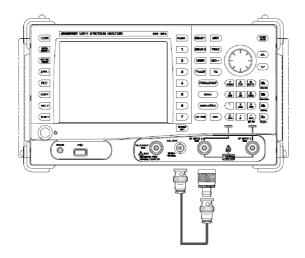


Figure 2-9 Connecting the CAL Signal (Channel 2)

12. Press ▼ and select OK. Press **Hz** to restart the calibration.


CAUTION: If an error is displayed in calibration, contact Advantest Instrument Call Center.

2.4 Measurement Example

2.4.1 W-CDMA Signal Channel Power Measurement and Adjacent Channel Leakage Power (ACP) Measurement

This section describes measurement of input and output signals of the amplifier by using the W-CDMA signal.

Connecting the signal

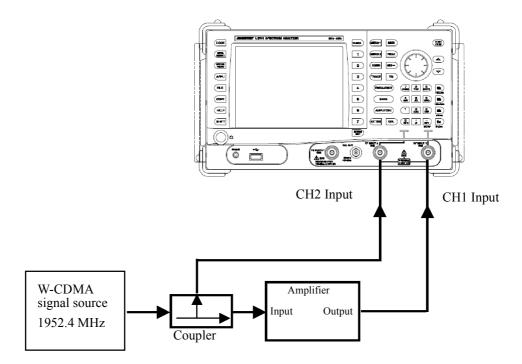


2.4.1 W-CDMA Signal Channel Power Measurement and Adjacent Channel Leakage Power (ACP) Measurement

Operation

1. Press SHIFT and SYSTEM(PRESET).

Initial setting conditions are loaded. Channel 1 is set to the active channel.

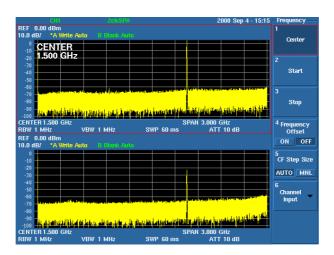

2. Press SHIFT and 0(RF2).

Channel 2 is set to the active channel.

3. Press FREQUENCY, 1, 9, 5, 2, ., 4, MHz, SPAN, and 1, 0, MHz.


Channel 2 is set as follows:

Center frequency: 1952.4 MHz

Frequency span: 10 MHz

4. Press MEAS1, Channel Power, Channel Width, 3, ., 8, 4, MHz, and Execute ON/OFF(ON).

The channel width is set to 3.84 MHz and the channel power measurement starts. The measurement result is displayed at the right side of the trace window.

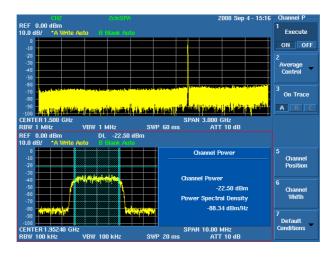

2.4.1 W-CDMA Signal Channel Power Measurement and Adjacent Channel Leakage Power (ACP) Measurement

5. Press SHIFT, and - (RF1).

Channel 1 is set to the active channel.

6. Press FREQUENCY, 1, 9, 5, 2, ., 4, MHz, SPAN, and 2, 5, MHz.

Channel 1 is set as follows:

Center frequency: 1952.4 MHz

Frequency span: 25 MHz

7. Press MEAS1, RETURN, ACP, and Channel Definition.

The CS/BS table is displayed.

The cursor is positioned at the Channel Space 1 setting text field.

8. Press 5 and MHz.

Channel Space 1 is set to 5 MHz.

The cursor moves to the Channel Bandwidth 1 setting text field.

9. Press 3, ., 8, 4, and MHz.

Channel Bandwidth 1 is set to 3.84 MHz.

The cursor moves to the Channel Space 2 setting text field.

10. Press 1, 0, and MHz.

Channel Space 1 is set to 10 MHz.

The cursor moves to the Channel Bandwidth 2 setting text field.

11. Press 3, ., 8, 4, and MHz.

Channel Bandwidth 2 is set to 3.84 MHz.

12. Press **RETURN**.

CS/BS Table					
[No]	[Channel Space]	[Channel Bandwidth]			
1	5.000 MHz	3.840 MHz			
2	10.000 MHz	3.840 MHz			
3					
4					
5					

2.4.1 W-CDMA Signal Channel Power Measurement and Adjacent Channel Leakage Power (ACP) Measurement

13. Press Execute ON/OFF (ON).

The ACP measurement starts.

The measurement result is displayed at the right side of the trace window.




Displaying MEAS function


The measurement result of the MEAS function is simplified because it is displayed along with the trace waveform.

In the Full Screen waveform display, the waveform in the two screens are simply enlarged and displayed.

To display the measurement result without simplifying, perform measurement in Dual CH OFF (single channel mode).



Displaying Dual CH ON



Displaying Dual CH OFF

2.4.2 Characteristics Evaluation of Frequency Converter

2.4.2 Characteristics Evaluation of Frequency Converter


This section describes measurement of a frequency response of a frequency converter such as a mixer or TV tuner, whose input and output frequencies differ.

Channel 1 sets the frequency range by using a tracking generator as an input signal.

Channel 2 observes the output signal of the converter.

The measurement target here is a down-converter module of a mixer + IF filter.

RF frequency: 1900 MHz IF frequency: 182 MHz

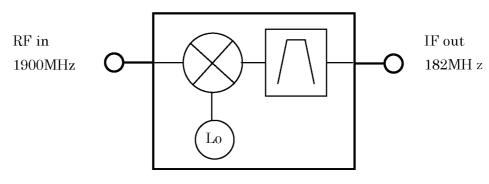


Mixer under test

CAUTION: The frequency converter enables measurement with an up/down-converter, however measurements cannot be performed when the relationship of the frequency is Lo - RF = IF.

2.4.2 Characteristics Evaluation of Frequency Converter

Connecting the signal

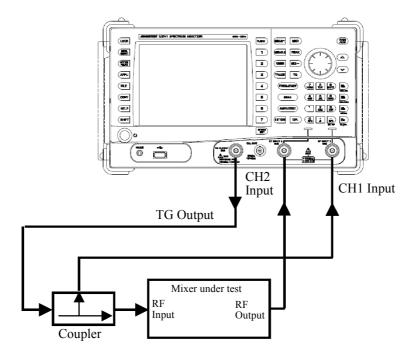

Required setting condition

Set the frequency span, sweep time, and trigger source of channels 1 and 2 the same.

Functions used in this measurement

Synchronizes sweep of channels 1 and 2 by using the CH Sync function.

Operation

1. Press SHIFT and SYSTEM(PRESET).

Initial setting conditions are loaded.

Channel 1 is set to the active channel.

2. Press FREQUENCY, 1, 9, 0, 0, MHz, SPAN, 5, 0, MHz, TG, and TG ON/ OFF(ON).

Channel 1 is set as follows: Center frequency: 1900 MHz Frequency span: 50 MHz

TG output ON

The input of channel 1 observes the input signal of the mixer.

Therefore, the trace of channel 1 displays the TG response by corresponding to the sweep.

3. Press **SHIFT** and **0**.


Channel 2 is set to the active channel.

4. Press FREQUENCY, 1, 8, 2, MHz, SPAN, and 5, 0, MHz.

In channel 2, the center frequency is set to $182~\mathrm{MHz}$ and frequency span is set to $50~\mathrm{MHz}$.

The TG synchronizes channel 1 and outputs a signal with a frequency of 1900 MHz ± 25 MHz.


The IF output of the mixer corresponds to this input, and it outputs a frequency of $182 \text{ MHz} \pm 25 \text{ MHz}$, however it cannot be observed by channel 2.

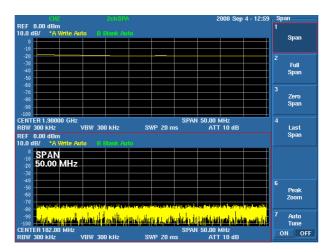

2.4.2 Characteristics Evaluation of Frequency Converter

5. Press **TG** and *CH Sync ON/OFF(ON)*.

Sweep of channels 1 and 2 is synchronized, and the frequency response of the frequency-converted mixer is displayed in the trace of channel 2.

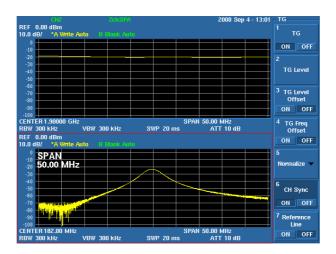

3. MENU MAP AND FUNCTION DESCRIPTION

3. MENU MAP AND FUNCTION DESCRIPTION

This chapter describes the functions of the panel keys and soft keys in the items shown below.

Menu Index: This section can be used to refer to the keys in Chapter 3.

Menu Map: This section shows the menu configurations of the panel keys.

Restrictions: Describes the restriction of the two channel input option.

Functional Descriptions: This section describes the functions of the panel keys and soft keys.

3.1 Menu Index

Operation Key	Pages	Operation Key	Pages
2 Screens	3-3		
APPLI	3-3		
Alternate IF	3-5		
Alternate Video	3-5		
CH Sync ON/OFF	3-7		
CH1>>CH2			
CH2>>CH1	3-3		
Couple CH ON/OFF	3-3, 3-4		
EXT CFG			
Delta Mode	3-6		
Display	3-3		
Dual CH ON/OFF			
Dual Delta ON/OFF	3-6		
Gated Sweep	3-5		
Full Screen CH1	3-3		
Full Screen CH2	3-3		
MKR	3-6		
Math	3-6		
More 1/2	3-9		
Self Test	3-9		
Self Test ALL	3-9		
Self Test CH1	3-9		
Self Test CH2	3-9		
Setup Copy	3-3		
Source	3-5		
Store	3-6		
TG	3-7		
TRACE	3-6		
$TRC \rightarrow (A)$	3-6		
TRC→(B)			
Trig Sync ON/OFF	3-5		
Trigger	3-5		

3.2 Restrictions

3.2 Restrictions

In some functions of the two channel input option, there are some parts whose operations differ from the U3741 function which does not have optional settings.

Also, there are functions which cannot be used in both channels because of the hardware restrictions.

1. Trace

In Dual mode: Two traces, A and B, can be used.

In Single mode: Three traces, A, B, and C can be used.

2. Trigger

Setting the trigger level

The level setting of the IF trigger is the same setting as channels 1 and 2.

(The IF trigger level cannot be set independently.)

The level setting of the EXT trigger is internally the same as the IF trigger.

Note the level setting value when setting the IF trigger and the EXT trigger at the same time.

3. Zoom function

In Dual mode: Zoom function cannot be used.

In Single mode: The Zoom function can be used, but when the Zoom function is On, the MEAS func-

tion cannot be used.

4. Sound monitor function

The sound demodulation function can use only channel 1.

5. TG (tracking generator) option

The TG option corresponds to channel 1.

6. 21.4 MHz IF output

The IF signal corresponds to channel 1.

7. GPIB command

R3131 and R3162 compatibility modes cannot be used.

3.3 Functional Descriptions

3.3 Functional Descriptions


This section describes the functions of the panel keys and soft keys.

МЕМО:

- indicates a panel key.
- All other names are soft menus.

3.3.1 **APPLI**

Displays the APPLI menu

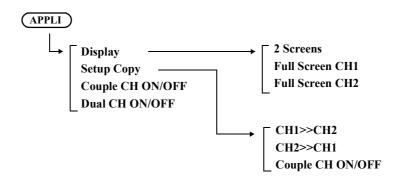

Display Displays the Display menu.

2 Screens Displays two screens in the upper and lower parts.

Upper screen: CH1 Lower screen: CH2

Full Screen CH1 Displays channel 1 on the entire screen.

The active channel is channel 1.

Full Screen CH2 Displays channel 2 on the entire screen.

The active channel is channel 2.

Setup Copy Displays the Sync Channel menu.

CH1>>CH2 Copies the setting condition of channel 1 to channel 2 and applies

it.

CH2>>CH1 Copies the setting condition of channel 2 to channel 1 and applies

it.

After the copy, the setting conditions and contents of the setting table for channels 1 and 2 are all the same.

CAUTION: If there is data such as a table that the user does not

want to change, save it to a USB memory before

copying.

3.3.1 APPLI

ON: Couple CH ON/OFF Couples and operates channels 1 and 2. The key settings operate for both channels regardless of the active or non-active channel. Coupled functions Frequency Center Start Stop **SPAN SPAN** Full Span Zero Span Last Span **CPL RBW VBW** Sweep Time All Auto OFF: Cancels the coupling. Couples and operates channels 1 and 2. The key settings operate for both channels regardless of Couple CH ON/OFF ON: the active or non-active channel. Coupled functions Frequency Center Start Stop **SPAN SPAN** Full Span Zero Span Last Span CPL RBW **VBW** Sweep Time All Auto OFF: Cancels the coupling.

ON:


OFF:

Operates in the 2CH mode.

Operates in the single channel mode. Only the active channel operates.

Dual CH ON/OFF

3.3.2 **EXT CFG**

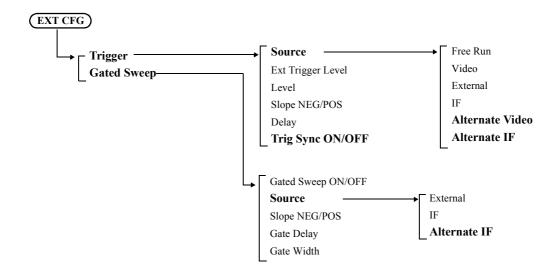

Trigger Displays the Trigger menu.

> Source Displays the Trig Source menu.

> > Alternate Video Selects the Video trigger signal of the other channel.

Alternate IF Selects the IF trigger signal of the other channel.

Trig Sync ON/OFF ON: When the trigger source of both channels is the same,

sweep starts at the same time.

When turning it ON, select the setting so that the trigger

source of both channels is the same. When the sweep time of each channel is different, the

sweep cycle corresponds to the slower channel.

OFF: Cancels the trigger sync function.

Each channel performs an asynchronous sweep.


Gated Sweep

Source

Alternate IF Selects the IF trigger signal of the other channel.

3.3.3 TRACE

3.3.3 TRACE

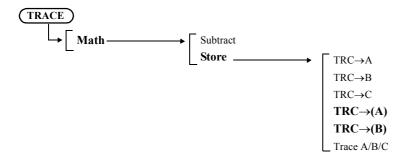

Math

Store


TRC \rightarrow (A) Stores the data of the active trace to trace A memory of the other

channel

 $TRC \rightarrow (B)$ Stores the data of the active trace to trace B memory of the other

channel.

3.3.4 MKR

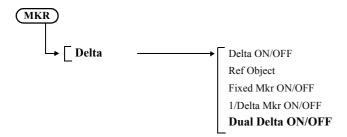

Delta Mode


Dual Delta ON/OFF Switches the delta marker display function between both channels ON and OFF.

ON: Positions the reference marker in the other channel, and

displays the relative value (frequency and level) of the active channel to the normal marker in the marker area.

OFF: Deletes the delta marker display.

3.3.5 TG



CH Sync ON/OFF Sets the channel synchronous function ON. Synchronizes sweep of channels 1 and 2. ON:

OFF: Cancels the channel synchronous function.

CH Sync is a function which performs sweep synchronizing with channels 1 and 2.

By using CH Sync, the tracking generator, which normally corresponds to channel 1, can also be used with channel 2.


To use CH Sync, set the frequency span, sweep time, and trigger source of channels 1 and 2 the same.

3.3.5 TG

Example: Input the TG output to channels 1 and 2 at the same time.

CH Sync ON:


TG responds to both channels 1 and 2.

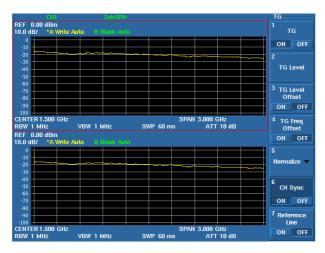

CH Sync OFF:

TG responds to channel 1.

Because channel 2 performs an asynchronous sweep with channel 1, there is not any response in channel 2.

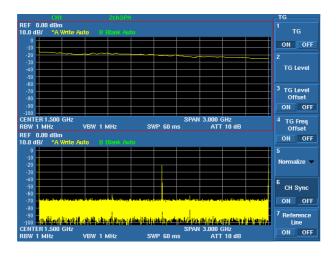

3.3.6 System



Self Test Displays the Self Test menu.

Self Test ALL Executes the self-test.

Self Test CH1 Tests an item regarding channel 1.
Self Test CH2 Tests an item regarding channel 2.

4. OVERVIEW OF REMOTE CONTROL

This chapter describes the added and changed items in OPT10 regarding the remote control system.

4.1 Status Byte

Statuses regarding channel 2 are allocated from bit 11 to bit 15 of the standard operation status register.

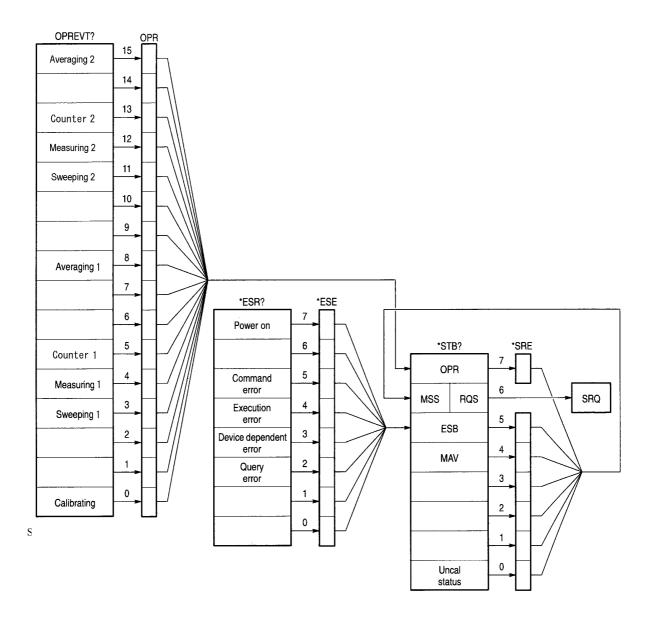


Figure 4-1 Status Registers

4.1 Status Byte

Table 4-1 Standard Operation Status Register

Bit	Function definition	Description
15	Averaging 2	Set to 1 when averaging of channel 2 is complete.
14		
13	Counter 2	Set to 1 when the counter measurement of channel 2 is complete.
12	Measuring 2	Set to 1 when the sequence measurement of channel 2 is complete.
11	Sweeping 2	Set to 1 when sweep of channel 2 is complete.
10		
9	Printing	Set to 1 when printing is complete.
8	Averaging 1	Set to 1 when averaging of channel 1 is complete.
7		
6		
5	Counter 1	Set to 1 when the counter measurement of channel 1 is complete.
4	Measuring 1	Set to 1 when the sequence measurement of channel 1 is complete.
3	Sweeping 1	Set to 1 when sweep of channel 1 is complete.
2		
1		
0	Calibrating	Set to 1 when correction data acquisition is complete.

4.2 Operation of TS command at Dual CH

TS (Take Sweep)


When the TS command is executed, the specified channel becomes a single sweep mode and starts sweep.

The GPIB bus maintains the hold state during the sweep, and the next command waits for the completion of the sweep and then it is executed

Operation

1. TS

Starts sweep of the active channel, and holds the GPIB bus until the sweep of the active channel has been complete.

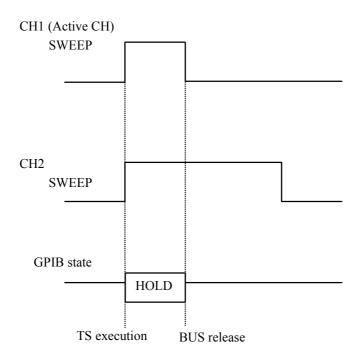


Note: The non-active CH does not relate to TS.

4.2 Operation of TS command at Dual CH


2. TSM

Starts sweep of channels 1 and 2 at the same time, and holds the GPIB bus until the sweep of both channels has been complete.

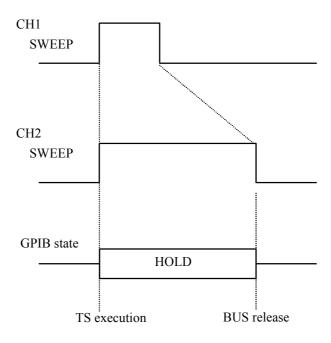

3. TSS

Starts sweep of channels 1 and 2 at the same time, and holds the GPIB bus until either channel, whichever completes the sweep faster, completes the sweep.

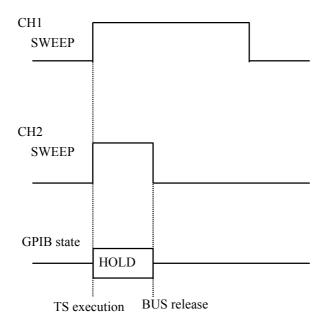

4.3 GPIB Remote Programming

4.3 GPIB Remote Programming

This section shows the AT command list for each OPT10 function:

- Command code
 - The command code "*" indicates a function that numeric or character strings data follows after the code. Data in [] can be omitted.
- Output format
 - A comma "," indicates that two or more data items are output.
 - ON or OFF indicates that 1 or 0 is output.
 - Frequency is output in Hz and time is output in sec.
- Level data is output in the currently set display unit.

4.4 AT Command Code List

4.4.1 APPLI (Mode setting)

Function	Command (EXE, SET)		Query (GET)	
Function	Code	Argument Format	Code	Output Format
Dual Channel	DUAL*	ON OFF	DUAL?	0 = OFF 1 = ON
Active Channel Select	ACTCH*	CH1 CH2	ACTCH?	1 = CH1 2 = CH2
Couple Channel	CPLCH*	ON OFF	CPLCH?	0 = OFF 1 = ON
Display mode	DISP*	SPLIT FULL1 FULL2	DISP?	0 = SPLIT 1 = FULL1 2 = FULL2
Copy Settings				
Copy CH1 → CH2	CP1TO2			
Copy CH2 → CH1	CP2TO1			

4.4.2 Sweep

4.4.2 Sweep

Function	Command	(EXE, SET)	Qı	uery (GET)
Function	Code	Argument Format	Code	Output Format
Sweep Time	SW ST*	Time	SW? ST?	Time
Sweep Auto	AS[*]	[ON] OFF	AS?	0 = OFF (manual) 1 = ON (auto)
Sweep Mode			SWM?	0 = Single 1 = Normal
Sweep Mode Normal				
active Ch	SN CONTS			
both Ch	SNALL CONTSALL			
Ch1	SN1 CONTS1			
Ch2	SN2 CONTS2			
Sweep Mode Single				
active Ch	SI SNGLS			
both Ch	SIALL SNGLSALL			
Ch1	SI1 SINGLS1			
Ch2	SI2 SINGLS2			
Take Sweep				
active Ch	TS			
both Ch (*1)	TSM			
both Ch (*2)	TSS			
Sweep Start / Stop				
active Ch	SR			
both Ch	SRALL			
Ch1	SR1			
Ch2	SR2			
Gated Sweep Mode	GTSWP*	ON OFF	GTSWP?	0 = OFF 1 = ON
Gate Source	GTSRC*	EXT IF XIF	GTSRC?	2 = EXT 3 = IF 5 = XIF
Gate Slope	GTSLP*	(FALL NEG -) (RISE POS +)	GTSLP?	0= RISE POS + 1= FALL NEG -
Gate Delay	GTPOS*	Time	GTPOS?	Time
Gate Width	GTWID*	Time	GTWID?	Time

^(*1) Completed when both channels are "Sweep end."(*2) Completed when either channel is "Sweep end."

4.4.3 Trigger

Function	Command	(EXE, SET)	Query (GET)	
Function	Code	Argument Format	Code	Output Format
Trigger Mode	TRGSRC*	FREE IF EXT VIDEO XVIDEO XIF	TRGSRC?	0 = FREE 1 = TRG_VIDEO 2 = TRG_EXT 3 = TRG_IF 4 = XVIDEO 5 = XIF
Video or IF Trigger Level	TRGLVL*	Level	TRGLVL?	Level
External Trigger Level	TRGTTLLVL*	Voltage	TRGTTLLVL?	Voltage
Trigger Slope	TRGSLP*	(FALL NEG -) (RISE POS +)	TRGSLP?	0 = RISE POS + $1 = FALL NEG -$
Trigger Delay	TRGDLY*	Time	TRGDLY?	Time
Trigger Sync ON/OFF	SYNCTRIG	ON OFF	SYNCTRIG?	0 = OFF 1 = ON

4.4.4 Trace

Function	Command (EXE, SET)		Query (GET)	
1 unction	Code	Argument Format	Code	Output Format
Math : Trace Store (Current trace \rightarrow trace n)	STORE*	TRA TRB TRC		
→ trace n of Non-active channel	STORE*	TRXA TRXB		
Trace Data Binary Out Channel1 TraceA Channel2 TraceA Channel1 TraceB Channel2 TraceB Channel1 TraceC Channel2 TraceC			TBA1? TBA2? TBB1? TBB2? TBC1? TBC2?	Depends on FORM commands

4.4.5 Marker

4.4.5 Marker

Function	Command (EXE, SET)		Query (GET)	
runction	Code	Argument Format	Code	Output Format
Dual Delta Mode	MKDD*	ON OFF	MKDD?	0 = OFF 1 = ON

4.4.6 TG

Function	Command (EXE, SET)		Query (GET)	
runction	Code	Argument Format	Code	Output Format
CH Sync ON/OFF	SYNCCH	ON OFF	SYNCCH?	0 = OFF 1 = ON

4.4.7 Save/Recall

Function	Commar	Command (EXE, SET)		y (GET)
Function	Code	Argument Format	Code	Output Format
Save Normalize Context A Trace A	SVNRM1A	ON OFF	SVNRM1A?	0 = OFF 1 = ON
Save Normalize Context A Trace B	SVNRM1B	ON OFF	SVNRM1B?	0 = OFF 1 = ON
Save Normalize Context A Trace C	SVNRM1C	ON OFF	SVNRM1C?	0 = OFF 1 = ON
Save Normalize Context B Trace A	SVNRM2A	ON OFF	SVNRM2A?	0 = OFF 1 = ON
Save Normalize Context B Trace B	SVNRM2B	ON OFF	SVNRM2B?	0 = OFF 1 = ON

4.4.8 Calibration

Function	Comman	d (EXE, SET)	Quer	y (GET)
runction	Code	Argument Format	Code	Output Format
Calibration All	CLALL[*]	[RFC1] RFC2		
Total Gain Calibration	CLGAIN[*]	[RFC1] RFC2	CLGAIN [RFC1] RFC2?	Integer 0 = OK >0 = Warning <0 = Error
RBW Calibration	CLRBW[*]	[RFC1] RFC2	CLRBW [RFC1] RFC2?	Integer 0 = OK >0 = Warning <0 = Error
PBW Calibration	CLPBW[*]	[RFC1] RFC2	CLPBW [RFC1] RFC2?	Integer 0 = OK >0 = Warning <0 = Error
ATT step Calibration	CLATT[*]	[RFC1] RFC2	CLATT [RFC1] RFC2?	Integer 0 = OK >0 = Warning <0 = Error

4.4.9 GPIB

Function	Command (EXE, SET)		Query (GET)	
	Code	Argument Format	Code	Output Format
Access Channel CH1	X1			
Access Channel CH2	X2			

4.5 Example Program for Remote Control

4.5 Example Program for Remote Control

This section describes an example program for remote control.

For more information on the GPIB bus controller and reading the Visual Basic GPIB control library, refer to manuals of the main unit.

4.5.1 Access Channel Example Program

To set or read data to or from channels 1 and 2 by remote control, an active channel must be set.

When setting only one command for the inactive channel, it can be done with two commands of "X2" and "command" by using the Access Channel command.

The channel setting with the Access Channel command is applied to only one command that follows "X1" or "X2".

GPIB code	Description
X1	Only one subsequent command is set to channel 1.
X2	Only one subsequent command is set to channel 2.

Example: To read the peak frequency of channels 1 and 2:

```
Dim Rdbuff1 as String, Rdbuff2 as String
Call ibdev(0,8,0,T10S,1,0,SPA) 'GPIB device initialization
                                'Device clear
Call ibclr(spa)
Call ibwrt(spa, "IP")
                                'preset
Call ibwrt(spa, "TSM")
                                'Sweeps both channels once
Call ibwrt(spa, "PS")
                              'Peak search for channel 1
                            'Peak search for channel 1
'Peak search for channel 2
Call ibwrt(spa, "X2;PS")
                                'Allocates 30 bytes to the buffer area
Rdbuff = Space(30)
Call ibwrt(spa, "MF?")
                                'Reads the marker frequency of channel 1
                                'Reads data
Call ibrd(spa, Rdbuff1)
Call ibwrt(spa, "X2;MF?")
                               'Reads the marker frequency of channel 2
Call ibrd(spa, Rdbuff2)
                                'Reads data
```

4.6 SCPI Command Code List

4.6 SCPI Command Code List

4.6.1 APPLI (Mode setting)

Function description	SCPI command	Parameter	Query reply
Dual Channel	:DISPlay:DUAL @1 \$1= :DISPlay:DUAL?	ON OFF	0=OFF 1=ON
Active Channel Select	:DISPlay:ACT @1 \$1= :DISPlay:ACT?	CH1 CH2	CH1 CH2
Couple Channel	:SOURce:COUPle @1 \$1=: SOURce:COUPle?	ON OFF	0=OFF 1=ON
Display Mode	:DISPlay:MODE @1 \$1=:DISPlay:MODE?	SPLIT FULL1 FULL2	SPLIT FULL1 FULL2
Copy Settings	:COPY:CHANnel @1,@2 (*1)	Channel Index, Channel Index	

(*1) @1: Source @2: Destination

Channel Index

1|2

1 = Ch 1

2 = Ch 2

4.6.2 Sweep

4.6.2 Sweep

Function description	SCPI command	Parameter	Query reply
Sweep Mode Normal/Single			
Set CH1/CH2	:INITiate#1:CONT @1 \$1=:INITiate#1:CONT?	Channel Index ON OFF	0 = OFF 1 = ON
active Ch	:INITiate:CONT @1	ON OFF	
both Ch	:INITiate:MCONT @1	ON OFF	
Take Sweep			
active Ch	:INITiate:TS		
both Ch (*1)	:INITiate:TSM		
both Ch (*2)	:INITiate:TSS		
Sweep Start / Stop			
Set CH1/CH2	:INITiate#1:RESTart	Channel Index	
active Ch	:INITiate:RESTart		

^(*1) Completed when both channels are "Sweep end."

Channel Index

1|2

1 = Ch 1

2 = Ch 2

When omitted = Active Channel

4.6.3 Trigger

Function description	SCPI command	Parameter	Query reply
Trigger Mode	:TRIGer#1[:SEQuence]:SOURce@2 \$1=:TRIGer#1[:SEQuence]:SOURce?	Channel index, IMMediate IF VIDeo EXT XVID XIF	IMM IF VID EXT XVID XIF
Trigger Sync ON/OFF	:TRIGer[:SEQuence]:SYNChronize: @1 \$1=:TRIGer[:SEQuence]:SYNChronize?	ON OFF	0 = OFF 1 = ON

^(*2) Completed when either channel is "Sweep end."

4.6.4 Trace

Function description	SCPI command	Parameter	Query reply
Math:Trace Store	:TRACe:COPY @1,@2 (*1)	TRACE1 TRACE2 TRACE3, TRACE1 TRACE2 TRACE3 TRACEX1 TRACEX2 (*2)	

(*1) @1: Source @2: Destination

4.6.5 Marker

Function description	SCPI command	Parameter	Query reply
Dual Delta Mode	:CALCulate#1:MARKer:DDELT [:STATe]@2 \$1=:CALCulate#1:MARKer:DDELT [:STATe]?	Context index ON OFF	0 = OFF 1 = ON

4.6.6 TG

Function description	SCPI command	Parameter	Query reply
CH Sync ON/OFF	:TRIGer[:SEQuence]:SYNChronize:CHANnel @1 \$1=:TRIGer[:SEQuence]:SYNChronize:CHANnel?	ON OFF	0 = OFF 1 = ON

5. SPECIFICATIONS

5.1 Option 10 2-Channel Input

Item	Description
Frequency	Conforms to the U3741 standard specifications.
Sweep	Applied to RF INPUT 2 (channel 2)
Amplitude range	
Amplitude accuracy	
Dynamic range	

• Differences from U3741/U3751 input output standard specifications

Item	Description		
Crosstalk between input channels	< -90 dBc (Input level -10 dBm, Input attenuator 0 dB)		
RF input 2			
Connector	N type female		
Impedance	50 Ω (nom.)		
VSWR	<1.5:1 Input attenuator > 10 dB		
External trigger input	Can be selected as the trigger input of RF input 2 when OPT10 is installed. The input connector is a single line only.		
21.4 MHz IF output	When OPT10 is installed, it is only the IF output which corresponds to RF input 1.		

• Differences from U3771/U3772 standard specifications

Item	Description				
Frequency range [RF INPUT 1]	10 MHz - 31.8 GHz (U3771)				
	10 MHz - 43 GHz	(U3772)			
Crosstalk between input channels	s < -90 dBc (Input level -10 dBm, Input attenuator 0 dB)				
RF input 1					
Connector	K type female				
Impedance	50 Ω (nom.)				
VSWR	1.7:1 (typ.)	Band 0	Input attenuator ≥ 10 dB		
	2.0 : 1 (typ.) Band 1, Band 2, Band 3 Input attenuator ≥ 10 dB				
	2.5 : 1 (typ.)	Band 4	Input attenuator ≥ 10 dB		
RF input 2					
Connector	N type female				
Impedance	50 Ω (nom.)				
VSWR	<1.5:1 Input attenuator > 10 dB				
External trigger input	Can be selected as the trigger input of RF input 2 when OPT10 is installed. The input connector is a single line only.				
21.4 MHz IF output	When OPT10 is in	When OPT10 is installed, it is only the IF output which corresponds to RF input 1.			

5.2 Option 11 75 Ω 2-Channel Input (Can be Installed only in the U3741)

5.2 Option 11 75 Ω 2-Channel Input (Can be Installed only in the U3741)

Item	Description
Frequency	Conforms to the specifications given when U3741 is equipped with OPT15.
Sweep	
Amplitude range	
Amplitude accuracy	
Dynamic range	

• Difference with the standard specifications

Item	Description
Crosstalk between input channels	< -90 dBc (Input level -10 dBm, Input attenuator 0 dB)
RF input 2	
Connector	N type female
Impedance	75 Ω (nom.)
VSWR	<1.6:1 Input attenuator > 10 dB
External trigger input	Can be selected as the trigger input of RF input 2 when OPT11 is installed. The input connector is a single line only.
21.4 MHz IF output	When OPT11 is installed, it is only the IF output which corresponds to RF input 1.

6. LIST OF ERROR MESSAGES

6. LIST OF ERROR MESSAGES

This chapter describes error messages regarding OPT10 and OPT11.

Error code	Туре	Displayed Message	Description of Message
0/33	WARNING	CH Sync has been turned off.	CH Sync was cancelled because the span, sweep time, or trigger source setting was changed when CH Sync was ON.
0/34	WARNING	This functionality is not allowed if the SPAN, SWP, or TRG are not same on CH1 and CH2.	CH Sync cannot be set to ON because the span, sweep time, or trigger source setting for both channels differ. Match the settings of the span and sweep time.

ALPHABETICAL INDEX

[Numerics]			[1]		
2 Screens	3-3		INSTRUMENT CONFIGURATION INTRODUCTION		
[A]					
Access Channel Example Program	4-10		[L]		
Alternate IF			LIST OF ERROR MESSAGES	6-1	
Alternate Video					
APPLI	3-3		rm1		
APPLI (Mode setting)	4-5,	4-11	[M]	1.0	4 12
AT Command Code List	4-5		Marker		4-13
			Math		
[B]			Measurement Example Menu Index		
Basic Operation	2.7		MENU MAP		
BASIC OPERATIONS			MKR		
BASIC OI ERATIONS	2-1		More 1/2		
[6]			141016 1/2	5	
[C]			FAIT		
Calibration		4-9	[N]		
CH Sync ON/OFF			Names and Functions of Each Part	2 1	
CH1>>CH2			on the Front Panel	2-1	
CH2>>CH1	3-3		Names and Functions of Each Part	2.5	
Characteristics Evaluation of	2.25		on the Screen		
Frequency Converter			Note when Displaying 2 Screens	2-10	
Course CH ON/OFF		2 4			
Couple CH ON/OFF	3-3,	3-4	[0]		
			Operation of TS command at Dual CH	4-3	
[D]			Option 10 2-Channel Input	5-1	
Delta Mode			Option 11 75 Ω 2-Channel Input		
Display			(Can be Installed only in the U3741)		
Dual CH ON/OFF	3-3,	3-4	OVERVIEW OF REMOTE CONTROL	4-1	
Dual Delta ON/OFF	3-6				
			[P]		
(E)			Panel and Screen Descriptions	2-1	
Example of Operation	2-10		Product Overview		
Example Program for Remote Control					
EXT CFG	3-5		[R]		
			Restrictions	3-2	
[F]			Restrictions	3-2	
Full Screen CH1	3-3		F01		
Full Screen CH2			[S]		
FUNCTION DESCRIPTION			Save/Recall		
Functional Descriptions			SCPI Command Code List		
			Selecting Active Channel		
[6]			Self Test		
[G]	2.5		Self Test ALL		
Gated Sweep			Self Test CH1		
GPIB			Self Test CH2		
GPIB Remote Programming	4-5		Setup Copy		
			SourceSPECIFICATIONS	5-3 5-1	
			OLI A ALLIN (ALLIN / NO.)	. , = 1	

U3700 Series OPT10/OPT11 User's Guide

Alphabetical Index

Status Byte	4-1		
Store	3-6		
Sweep	4-6,	4-12	
Switching to Single Channel Mode			
Switching Two Channel Display Modes	2-9		
Synchronizing Channels 1 and 2	2-9		
System	3-9		
[T]			
TG	3-7	4-8	
	4-13	. 0,	
TRACE			
Trace		4-13	
TRC→(A)		_	
TRC→(B)			
Trig Sync ON/OFF			
Trigger		4-7,	
	4-12		
[W]			
W-CDMA Signal Channel Power Measur	ement		
and Adjacent Channel Leakage Power			
(ACP) Measurement	2-21		
(1101) 111000010110110			

ADVANTEST

ADVANTEST CORPORATION

U3700 Series **OPT53/OPT54/OPT55/OPT56** Time Domain Analysis Option User's Guide

MANUAL NUMBER FOE-8440269C00

Applicable Models

U3741

U3751

U3771

U3772

TABLE OF CONTENTS

Product Overview	1.	INTRODUCTION
INSTRUMENT CONFIGURATION AND BASIC OPERATIONS Instrument of Each Part on Screen Instrument of In	1.1	Contents of This Manual
Names and Functions of Each Part on Screen 1.1.1 Freq-Time, Phase-Time, Power-Time, or IQ-Time Display Screen 2.1.2 Partial FFT Display Screen 2.1.3 OPT54 2-channel Display Window Operating Method 2.2.1 Capturing I/Q Waveforms of RF Signal 2.2.1.1 Setting Center Frequency, Reference Level, and Sweep Mode 2.2.1.2 Setting Waveform Capture Time and Capture Bandwidth 2.2.1.3 Starting and Stopping RF Signal Capture 2.2.2 Analyzing RF Signal 2.2.2.1 Freq-Time Analysis 2.2.2.2 Phase-Time Analysis 2.2.2.2 Phase-Time Analysis 2.2.2.3 Power-Time Analysis 2.2.2.4 IQ-Time Analysis Using Position View Function 2.2.2.5 Partial FFT Analysis Using Position View Function (Freq-Time and Phase-Time) OPT55 Pulse Modulation Signal Measurement Example 2-Channel Time Domain Analysis Option (OPT54/OPT56) 4.1 Main Basic Operations with 2-Channel Specifications Example of Four-Value FSK Signal Analysis MENU MAP AND FUNCTION DESCRIPTION 5.1 Time Domain MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS Option 53, Option 54 Time Domain Analysis Option Copposition 54 Time Domain Analysis Option	1.2	Product Overview
Names and Functions of Each Part on Screen 1.1.1 Freq-Time, Phase-Time, Power-Time, or IQ-Time Display Screen 2.1.2 Partial FFT Display Screen 2.2.2 OPT54 2-channnel Display Window Operating Method 2.2.1 Capturing I/Q Waveforms of RF Signal 2.2.1.1 Setting Center Frequency, Reference Level, and Sweep Mode 2.2.1.2 Setting Waveform Capture Time and Capture Bandwidth 2.2.1.3 Starting and Stopping RF Signal Capture 2.2.2.1 Freq-Time Analysis 2.2.2.1 Freq-Time Analysis 2.2.2.2 Phase-Time Analysis 2.2.2.3 Power-Time Analysis 2.2.2.4 IQ-Time Analysis 2.2.2.5 Partial FFT Analysis 2.2.2.6 Freq-Time Analysis Using Position View Function Two-Type Simultaneous Analysises Using Dual Meas Function (Freq-Time and Phase-Time) OPT55 Pulse Modulation Signal Measurement Example 2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) Main Basic Operations with 2-Channel Specifications Example of Four-Value FSK Signal Analysis MENU MAP AND FUNCTION DESCRIPTION 3.1 Time Domain MKR	1.3	Conventions of Notation Used in This Document
2.1.1 Freq-Time, Phase-Time, Power-Time, or IQ-Time Display Screen 2.1.2 Partial FFT Display Screen 2.1.3 OPT54 2-channnel Display Window 2.2 Operating Method 2.2.1 Capturing I/Q Waveforms of RF Signal 2.2.1.1 Setting Center Frequency, Reference Level, and Sweep Mode 2.2.1.2 Setting Waveform Capture Time and Capture Bandwidth 2.2.1.3 Starting and Stopping RF Signal Capture 2.2.2.1 Freq-Time Analysis 2.2.2.1 Freq-Time Analysis 2.2.2.2 Phase-Time Analysis 2.2.2.2 Phase-Time Analysis 2.2.2.3 Power-Time Analysis 2.2.2.4 IQ-Time Analysis 2.2.2.4 IQ-Time Analysis Using Position View Function 2.2.2.5 Partial FFT Analysis Using Position View Function 2.2.2.6 Freq-Time and Phase-Time) 2.3 OPT55 Pulse Modulation Signal Measurement Example 2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) 2.4.1 Main Basic Operations with 2-Channel Specifications 2.4.2 Example of Four-Value FSK Signal Analysis 3. MENU MAP AND FUNCTION DESCRIPTION 3.1.1 Time Domain 3.1.2 MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 5.1 Option 53, Option 54 Time Domain Analysis Option 5. Option 53, Option 54 Time Domain Analysis Option 5. Option 53, Option 54 Time Domain Analysis Option	2.	INSTRUMENT CONFIGURATION AND BASIC OPERATIONS
2.1.2 Partial FFT Display Screen 2.1.3 OPT54 2-channnel Display Window 2.2.1 Capturing I/Q Waveforms of RF Signal 2.2.1.1 Setting Center Frequency, Reference Level, and Sweep Mode 2.2.1.2 Setting Waveform Capture Time and Capture Bandwidth 2.2.1.3 Starting and Stopping RF Signal Capture 2.2.1 Starting and Stopping RF Signal Capture 2.2.2 Analyzing RF Signal 2.2.2.1 Freq-Time Analysis 2.2.2.2 Phase-Time Analysis 2.2.2.2 Phase-Time Analysis 2.2.2.3 Power-Time Analysis 2.2.2.4 IQ-Time Analysis 2.2.2.5 Partial FFT Analysis 2.2.2.6 Freq-Time Analysis Using Position View Function 2.2.2.7 Two-Type Simultaneous Analysises Using Dual Meas Function (Freq-Time and Phase-Time) 2.3 OPT55 Pulse Modulation Signal Measurement Example 2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) 2.4.1 Main Basic Operations with 2-Channel Specifications 2.4.2 Example of Four-Value FSK Signal Analysis 3. MENU MAP AND FUNCTION DESCRIPTION 3.1 Functional Descriptions 3.1.1 Time Domain 3.1.2 Time Domain 3.1.2 MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 5.1 Option 53, Option 54 Time Domain Analysis Option	2.1	
OPT54 2-channel Display Window Operating Method Capturing I/Q Waveforms of RF Signal Setting Center Frequency, Reference Level, and Sweep Mode Setting Waveform Capture Time and Capture Bandwidth Setting Waveform Capture Time Analysis Capture Analyzing RF Signal Measurement Example Capture Firm Analysis Capture Firm Analysis Using Position View Function (Freq-Time Analysis Usin	2.1.1	Freq-Time, Phase-Time, Power-Time, or IQ-Time Display Screen
2.2.1 Operating Method 2.2.1.1 Setting Center Frequency, Reference Level, and Sweep Mode 2.2.1.2 Setting Waveform Capture Time and Capture Bandwidth 2.2.1.3 Starting and Stopping RF Signal Capture 2.2.2.1 Analyzing RF Signal 2.2.2.2 Analyzing RF Signal 2.2.2.3 Phase-Time Analysis 2.2.2.4 IQ-Time Analysis 2.2.2.5 Partial FFT Analysis 2.2.2.6 Freq-Time Analysis Using Position View Function 2.2.2.7 Two-Type Simultaneous Analysises Using Dual Meas Function (Freq-Time and Phase-Time) 2.3 OPT55 Pulse Modulation Signal Measurement Example 2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) 2.4.1 Main Basic Operations with 2-Channel Specifications 2.4.2 Example of Four-Value FSK Signal Analysis 3. MENU MAP AND FUNCTION DESCRIPTION 3.1 Functional Descriptions 3.1.1 Time Domain 3.1.2 MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output	2.1.2	
C.2.1 Capturing I/Q Waveforms of RF Signal C.2.1.1 Setting Center Frequency, Reference Level, and Sweep Mode C.2.1.2 Setting Waveform Capture Time and Capture Bandwidth Starting and Stopping RF Signal Capture Analyzing RF Signal C.2.2 Analyzing RF Signal C.2.2.1 Freq-Time Analysis C.2.2.2 Phase-Time Analysis C.2.2.3 Power-Time Analysis C.2.2.4 IQ-Time Analysis C.2.2.5 Partial FFT Analysis C.2.2.6 Freq-Time Analysis Using Position View Function C.2.2.7 Two-Type Simultaneous Analysises Using Dual Meas Function (Freq-Time and Phase-Time) C.3 OPT55 Pulse Modulation Signal Measurement Example C.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) Main Basic Operations with 2-Channel Specifications Example of Four-Value FSK Signal Analysis MENU MAP AND FUNCTION DESCRIPTION MENU MAP AND FUNCTION DESCRIPTION Time Domain MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 5.1 Option 53, Option 54 Time Domain Analysis Option		
2.2.1.1 Setting Center Frequency, Reference Level, and Sweep Mode 2.2.1.2 Setting Waveform Capture Time and Capture Bandwidth 2.2.1.3 Starting and Stopping RF Signal Capture 2.2.2 Analyzing RF Signal 2.2.2.1 Freq-Time Analysis 2.2.2.2 Phase-Time Analysis 2.2.2.2 Phase-Time Analysis 2.2.2.3 Power-Time Analysis 2.2.2.4 IQ-Time Analysis 2.2.2.5 Partial FFT Analysis 2.2.2.6 Freq-Time Analysis Using Position View Function 2.2.2.7 Two-Type Simultaneous Analysises Using Dual Meas Function (Freq-Time and Phase-Time) 2.3 OPT55 Pulse Modulation Signal Measurement Example 2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) 2.4.1 Main Basic Operations with 2-Channel Specifications 2.4.2 Example of Four-Value FSK Signal Analysis 3. MENU MAP AND FUNCTION DESCRIPTION 3.1 Functional Descriptions 3.1.1 Time Domain 3.1.2 MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 5.1 Option 53, Option 54 Time Domain Analysis Option		
2.2.1.2 Setting Waveform Capture Time and Capture Bandwidth 2.2.1.3 Starting and Stopping RF Signal Capture 2.2.2 Analyzing RF Signal 2.2.2.1 Freq-Time Analysis 2.2.2.2 Phase-Time Analysis 2.2.2.3 Power-Time Analysis 2.2.2.4 IQ-Time Analysis 2.2.2.5 Partial FFT Analysis Using Position View Function Two-Type Simultaneous Analysises Using Dual Meas Function (Freq-Time and Phase-Time) OPT55 Pulse Modulation Signal Measurement Example 2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) 2.4.1 Main Basic Operations with 2-Channel Specifications 2.4.2 Example of Four-Value FSK Signal Analysis 3. MENU MAP AND FUNCTION DESCRIPTION 3.1 Functional Descriptions 3.1.1 Time Domain 3.1.2 MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 5.1 Option 53, Option 54 Time Domain Analysis Option		Setting Center Frequency Reference Level and Sween Mode
2.2.1.3 Starting and Stopping RF Signal Capture 2.2.2 Analyzing RF Signal 2.2.2.1 Freq-Time Analysis 2.2.2.2 Phase-Time Analysis 2.2.2.3 Power-Time Analysis 2.2.2.4 IQ-Time Analysis 2.2.2.5 Partial FFT Analysis 2.2.2.6 Freq-Time Analysis Using Position View Function 2.2.2.7 Two-Type Simultaneous Analysises Using Dual Meas Function (Freq-Time and Phase-Time) 2.3 OPT55 Pulse Modulation Signal Measurement Example 2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) 2.4.1 Main Basic Operations with 2-Channel Specifications 2.4.2 Example of Four-Value FSK Signal Analysis 3. MENU MAP AND FUNCTION DESCRIPTION 3.1 Functional Descriptions 3.1.1 Time Domain 3.1.2 MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 5.1 Option 53, Option 54 Time Domain Analysis Option	2.2.1.2	Setting Waveform Capture Time and Capture Bandwidth
2.2.2 Analyzing RF Signal 2.2.2.1 Freq-Time Analysis 2.2.2.2 Phase-Time Analysis 2.2.2.3 Power-Time Analysis 2.2.2.4 IQ-Time Analysis 2.2.2.5 Partial FFT Analysis 2.2.2.6 Freq-Time Analysis Using Position View Function 2.2.2.7 Two-Type Simultaneous Analysises Using Dual Meas Function (Freq-Time and Phase-Time) 2.3 OPT55 Pulse Modulation Signal Measurement Example 2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) 2.4.1 Main Basic Operations with 2-Channel Specifications 2.4.2 Example of Four-Value FSK Signal Analysis 3. MENU MAP AND FUNCTION DESCRIPTION 3.1 Functional Descriptions 3.1.1 Time Domain 3.1.2 MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 5.1 Option 53, Option 54 Time Domain Analysis Option	2.2.1.3	Starting and Stopping RF Signal Capture
Phase-Time Analysis 2.2.2.3 Power-Time Analysis 2.2.2.4 IQ-Time Analysis 2.2.2.5 Partial FFT Analysis 2.2.2.6 Freq-Time Analysis Using Position View Function Two-Type Simultaneous Analysises Using Dual Meas Function (Freq-Time and Phase-Time) 2.3 OPT55 Pulse Modulation Signal Measurement Example 2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) 2.4.1 Main Basic Operations with 2-Channel Specifications Example of Four-Value FSK Signal Analysis 3. MENU MAP AND FUNCTION DESCRIPTION 3.1 Functional Descriptions 3.1.1 Time Domain 3.1.2 MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 5.1 Option 53, Option 54 Time Domain Analysis Option	2.2.2	Analyzing RF Signal
2.2.2.3 Power-Time Analysis 2.2.2.4 IQ-Time Analysis 2.2.2.5 Partial FFT Analysis Using Position View Function 2.2.2.6 Freq-Time Analysis Using Position View Function (Freq-Time and Phase-Time) 2.3 OPT55 Pulse Modulation Signal Measurement Example 2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) 2.4.1 Main Basic Operations with 2-Channel Specifications 2.4.2 Example of Four-Value FSK Signal Analysis 3. MENU MAP AND FUNCTION DESCRIPTION 3.1 Functional Descriptions 3.1.1 Time Domain 3.1.2 MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 5. Option 53, Option 54 Time Domain Analysis Option		Freq-Time Analysis
2.2.2.4 IQ-Time Analysis 2.2.2.5 Partial FFT Analysis 2.2.2.6 Freq-Time Analysis Using Position View Function 2.2.2.7 Two-Type Simultaneous Analysises Using Dual Meas Function (Freq-Time and Phase-Time) 2.3 OPT55 Pulse Modulation Signal Measurement Example 2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) 2.4.1 Main Basic Operations with 2-Channel Specifications 2.4.2 Example of Four-Value FSK Signal Analysis 3. MENU MAP AND FUNCTION DESCRIPTION 3.1 Functional Descriptions 3.1.1 Time Domain 3.1.2 MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 5. Option 53, Option 54 Time Domain Analysis Option		Power-Time Analysis
2.2.2.5 Partial FFT Analysis	2.2.2.4	IO-Time Analysis
2.2.2.6 Freq-Time Analysis Using Position View Function Two-Type Simultaneous Analysises Using Dual Meas Function (Freq-Time and Phase-Time) 2.3 OPT55 Pulse Modulation Signal Measurement Example 2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) 2.4.1 Main Basic Operations with 2-Channel Specifications 2.4.2 Example of Four-Value FSK Signal Analysis 3. MENU MAP AND FUNCTION DESCRIPTION 3.1 Functional Descriptions 3.1.1 Time Domain 3.1.2 MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 5.1 Option 53, Option 54 Time Domain Analysis Option	2.2.2.5	Partial FFT Analysis
(Freq-Time and Phase-Time) OPT55 Pulse Modulation Signal Measurement Example 2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) 2.4.1 Main Basic Operations with 2-Channel Specifications 2.4.2 Example of Four-Value FSK Signal Analysis 3. MENU MAP AND FUNCTION DESCRIPTION 3.1 Functional Descriptions 3.1.1 Time Domain 3.1.2 MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 5.1 Option 53, Option 54 Time Domain Analysis Option	2.2.2.6	Freq-Time Analysis Using Position View Function
OPT55 Pulse Modulation Signal Measurement Example 2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) 2.4.1 Main Basic Operations with 2-Channel Specifications 2.4.2 Example of Four-Value FSK Signal Analysis 3. MENU MAP AND FUNCTION DESCRIPTION 3.1 Functional Descriptions 3.1.1 Time Domain 3.1.2 MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 5.1 Option 53, Option 54 Time Domain Analysis Option	2.2.2.7	Two-Type Simultaneous Analysises Using Dual Meas Function
2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56) 2.4.1 Main Basic Operations with 2-Channel Specifications Example of Four-Value FSK Signal Analysis 3. MENU MAP AND FUNCTION DESCRIPTION 3.1 Functional Descriptions 3.1.1 Time Domain 3.1.2 MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 5.1 Option 53, Option 54 Time Domain Analysis Option	2 2	(Freq-11me and Phase-11me) OPT55 Pulse Modulation Signal Massurament Example
Main Basic Operations with 2-Channel Specifications Example of Four-Value FSK Signal Analysis MENU MAP AND FUNCTION DESCRIPTION Functional Descriptions Time Domain MKR→ OVERVIEW OF REMOTE CONTROL GPIB Remote Programming AT Command Code List J/Q Data Output SPECIFICATIONS Option 53, Option 54 Time Domain Analysis Option		
Example of Four-Value FSK Signal Analysis MENU MAP AND FUNCTION DESCRIPTION B.1. Functional Descriptions Time Domain MKR→ OVERVIEW OF REMOTE CONTROL GPIB Remote Programming AT Command Code List I/Q Data Output SPECIFICATIONS Option 53, Option 54 Time Domain Analysis Option		, , , , , , , , , , , , , , , , , , , ,
MENU MAP AND FUNCTION DESCRIPTION S.1 Functional Descriptions Time Domain MKR→ OVERVIEW OF REMOTE CONTROL GPIB Remote Programming AT Command Code List I/Q Data Output SPECIFICATIONS Option 53, Option 54 Time Domain Analysis Option	2.4.2	
Functional Descriptions Time Domain MKR→ OVERVIEW OF REMOTE CONTROL GPIB Remote Programming AT Command Code List I/Q Data Output SPECIFICATIONS Option 53, Option 54 Time Domain Analysis Option		
Time Domain MKR→ OVERVIEW OF REMOTE CONTROL GPIB Remote Programming AT Command Code List I/Q Data Output SPECIFICATIONS Option 53, Option 54 Time Domain Analysis Option	3.	
MKR→ 4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 6.1 Option 53, Option 54 Time Domain Analysis Option	3.1	•
4. OVERVIEW OF REMOTE CONTROL 4.1 GPIB Remote Programming	3.1.1	
4.1 GPIB Remote Programming 4.2 AT Command Code List 4.3 I/Q Data Output 5. SPECIFICATIONS 6.1 Option 53, Option 54 Time Domain Analysis Option	3.1.2	MKR→
AT Command Code List I/Q Data Output SPECIFICATIONS Option 53, Option 54 Time Domain Analysis Option	4.	OVERVIEW OF REMOTE CONTROL
AT Command Code List I/Q Data Output SPECIFICATIONS Option 53, Option 54 Time Domain Analysis Option	4.1	GPIB Remote Programming
5.1 Option 53, Option 54 Time Domain Analysis Option	4.2	
Option 53, Option 54 Time Domain Analysis Option	4.3	
Option 53, Option 54 Time Domain Analysis Option	5.	SPECIFICATIONS
	5.1	
5.2 Option 55, Option 56 Time Domain Analysis Option	5.2	Option 55, Option 56 Time Domain Analysis Option

Table of Contents

6.	UNCAL MESSAGE, LIST OF ERROR MESSAGES,				
	AND RESTRICTIONS	6-1			
6.1	How to Delete UNCAL Message for Partial FFT Analysis	6-1			
6.2	List Of Error Messages 6-2				
6.3	Restrictions	6-2			
6.3.1 6.3.2					
ALPF	HABETICAL INDEX	I-1			

LIST OF TABLES

No.	Title	Page
3-1	OPT53/OPT54 Capture BW Setting Value and Partial FFT Frequency Resolution	3-5
3-2	OPT55/OPT56 Capture BW Setting Value and Partial FFT Frequency Resolution	3-5
3-3	OPT53/OPT54 Capture BW Setting Value and Capture Time Maximum Value	3-6
3-4	OPT55/OPT56 Capture BW Setting Value and Capture Time Maximum Value	3-6

1. INTRODUCTION

1. INTRODUCTION

This chapter describes the content of this manual and the product overview of the U3700 series spectrum analyzer time domain analysis option (OPT53/OPT54/OPT55/OPT56) to help the user get the most out of this guide.

For more information on the basic descriptions, refer to "U3700 Series User's Guide."

1.1 Contents of This Manual

The contents of each chapter are as follows:

CHAPTER 1. INTRODUCTION	This chapter describes the contents of this manual and the product overview.
CHAPTER 2. INSTRUMENT CONFIGURATION AND BASIC OPERATIONS	This chapter describes the functions and operating methods of option with measurement examples.
CHAPTER 3. MENU MAP AND FUNCTION DESCRIPTION	This chapter describes the menu structure and functions of soft keys.
CHAPTER 4. OVERVIEW OF REMOTE CONTROL	This chapter describes commands in order of functions for the added and changed items in option.
CHAPTER 5. SPECIFICATIONS	This chapter describes option specifications.
CHAPTER 6. UNCAL MESSAGE, LIST OF ERROR MESSAGES, AND RESTRICTIONS	This chapter describes error messages and restrictions related to option.

1.2 Product Overview

1.2 Product Overview

The time domain analysis options, OPT53, OPT54, OPT55, and OPT56, add a function, which captures and analyzes changes of RF signal characteristics with time, to the U3700 series spectrum analyzer.

OPT53 and OPT55: Option for single channel input.

OPT54 and OPT56: Option for 2-channel input. The time domain analysis function is added to both chan-

nels 1 and 2.

Features

It performs quadrature separation for an RF signal and captures it as time domain I/Q waveforms.
 OPT53/OPT54

Measurement bandwidth (BW) 100 Hz to 3 MHz (1 to 3 steps)

Number of I/Q waveform record samples 1 M Samples (I/Q)

I/Q sampling rate 713 Hz (BW 100 Hz) to 21.4 MHz (BW 3 MHz) I/Q waveform record time 49 msec (BW 3 MHz) to 1000 sec (BW 100 Hz)

OPT55/OPT56

Measurement bandwidth (BW) 100 Hz to 30 MHz (1 to 3 steps), 40 MHz

Number of I/Q waveform record samples 8 M Samples (I/Q)

I/Q sampling rate 500 Hz (BW 100 Hz) to 65 MHz (BW 40 MHz) I/Q waveform record time 120 msec (BW 40 MHz) to 1000 sec (BW 100 Hz)

It analyzes changes of RF signal characteristics with time as changes of fundamental quantities.

Freq-Time: Frequency versus time
Phase-Time: Phase versus time
Power-Time: Power versus time
IQ-Time: I/Q voltage versus time
FFT: FFT spectrum analysis

Data output function

It outputs I/Q waveform capture data and analysis results to an external PC via GPIB/LAN.

1.3 Conventions of Notation Used in This Document

The panel and soft key notations used in this manual are described below.

Panel key: Bold Example: FREQUENCY, SPAN

Soft keys: Bold italics Example: *Center*, *Span*


2. INSTRUMENT CONFIGURATION AND BASIC OPERATIONS

This chapter describes operating methods of the time domain analysis function through function descriptions of each part on screens related to OPT53, OPT54, OPT55, and OPT56 and measurement examples.

2.1 Names and Functions of Each Part on Screen

This section describes names and functions on screens related to OPT53, OPT54, OPT55, and OPT56.

2.1.1 Freq-Time, Phase-Time, Power-Time, or IQ-Time Display Screen

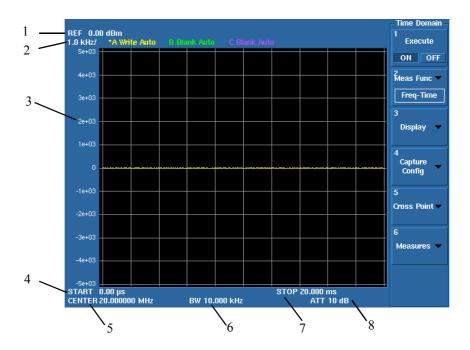

Reference level Displays a value set for the reference level. Vertical scale Displays a value set for the vertical scale. A value set for Vertical Scale/div is displayed. 3. Vertical scale display Displays vertical scales. 4. Analysis start time Displays the analysis start time. A value set for Analysis Offset is displayed. Center frequency Displays a center frequency. Capture bandwidth Displays a bandwidth in which a time domain waveform is captured and analyzed. A value set for Capture BW is displayed.


2.1.2 Partial FFT Display Screen

7. Analysis stop time Displays the analysis stop time.

A value for [Analysis Time + Analysis Offset] is displayed.

8. RF attenuator Displays a value set for the attenuator.

2.1.2 Partial FFT Display Screen

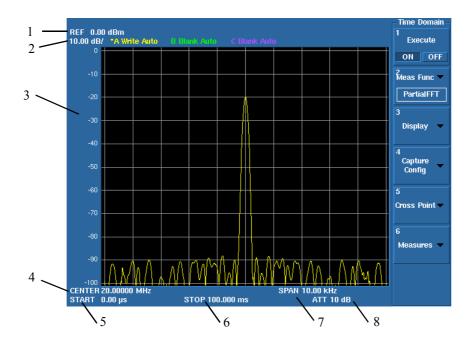

1. Reference level Displays a value set for the reference level.

Vertical scale Displays a value set for the vertical scale.
 A value set for Vertical Scale/div is displayed.

3. Vertical scale display Displays the vertical scales.

4. Center frequency Displays a center frequency.

5. Analysis start time Displays the analysis start time.

A value set for Analysis Offset is displayed. Displays the start time of Partial FFT analysis.

6. Analysis stop time Displays the analysis stop time.

The analysis stop time for Freq-Time, Phase-Time, Power-Time,

or IQ-Time is displayed.

Regardless of this value, the analysis time for Partial FFT is set to a specific value for each value set for Capture BW. For more information, refer to Chapter 3, "MENU MAP AND FUNCTION

DESCRIPTÍON."

7. Capture bandwidth Displays a bandwidth in which a time domain waveform is cap-

tured and analyzed.

8. RF attenuator Displays a value set for the attenuator.

2.1.3 OPT54 2-channnel Display Window

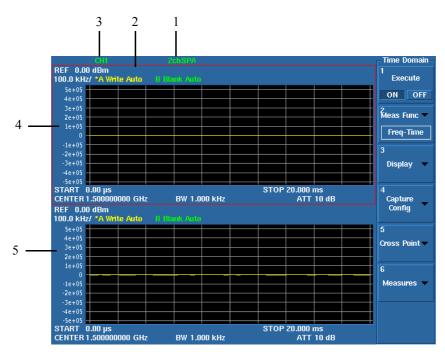


Figure 2-1 Screen Display of DUAL CH ON 2 Screens

1. Operation mode When DUAL CH ON: Displays 2chSPA. When DUAL CH OFF: Nothing is displayed.

2. Active channel display Indicates the active channel, where settings can be changed, by using the red rectangular box.

3. Active channel display

Channel 1: CH1
Channel 2: CH2
Couple CH ON: CPL

4. CH1 display window

5. CH2 display window

2.2 Operating Method


2.2 Operating Method

This section describes the functions and operating methods of the time domain analysis option through measurement examples.

By using the time domain analysis function, changes of RF signal characteristics with time can be measured as each waveform of frequency, phase, power, I/Q waveforms, or spectrum.

For more information on this instrument configuration and basic operations, refer to the U3700 series user's manual.

This section describes the FSK (Frequency Shift Keying) modulated signal measurement as an example.

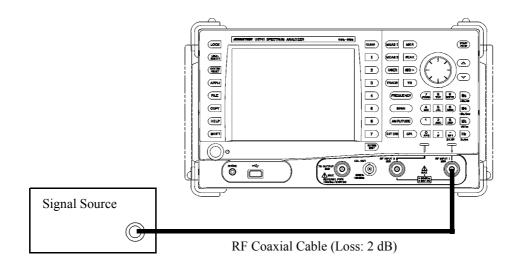

Signal Source output

Frequency: 2.45 GHz

Power: 0 dBm

Modulation Type: FSK

Frequency Deviation: 40 kHzp-p

Baseband Signal: 2 kHz PRBS

2.2.1 Capturing I/Q Waveforms of RF Signal

This section describes procedures for capturing an RF signal into the internal memory of this instrument as I/O waveforms.

2.2.1.1 Setting Center Frequency, Reference Level, and Sweep Mode

1. Press FREQUENCY, 2, ., 4, 5, and GHz.

The center frequency is set to 2.45 GHz.

2. Press **AMPLITUDE**, **0**, and **GHz**.

The reference level is set to 0 dBm.

3. Press EXT CFG and Sweep Mode SGL/CNT to select SGL.

The sweep mode is set to Single.

2.2.1.2 Setting Waveform Capture Time and Capture Bandwidth

1. Press MEAS 2, More 1/2, and Time Domain.

The time domain analysis menu is displayed.

2. Press Capture Config.

The waveform capture setting menu is displayed.

3. Press *Capture BW*, 1, 0, 0, and kHz.

The waveform capture bandwidth is set to 100 kHz.

4. Press Capture Time, 2, 0, 0, and kHz.

The waveform capture time is set to 200 msec.

5. Press **RETURN**.

The display returns to the time domain analysis menu.

2.2.1.3 Starting and Stopping RF Signal Capture

1. Press *Execute ON/OFF* and select ON.

The time domain analysis function is enabled.

2. Press START/STOP.

Capturing an RF signal starts.

That automatically stops 200 msec after the capture start according to settings of Capture Time (200 ms) and Sweep Mode (Single).

2.2.2 Analyzing RF Signal

2.2.2 Analyzing RF Signal

This section describes procedures for performing various analyses from waveform data captured in the internal memory of this instrument.

Captured I/Q waveforms can be analyzed from various viewpoints of frequency, phase, power, I/Q waveforms, and FFT spectrum by using each function of the Meas Func menu.

2.2.2.1 Freq-Time Analysis

Function setting

1. Press *Meas Func*.

The analysis function selection menu is displayed.

2. Press *Freq-Time*.

The analysis function for "frequency versus time" is selected.

3. Press **RETURN**.

The display returns to the time domain analysis menu.

The currently selected analysis function is displayed on the Meas Func key.

Display setting

4. Press Display.

Menus for analysis time range setting (horizontal axis) and data display setting (vertical axis) are displayed.

5. Press *Analysis Offset*, **0**, and MHz.

The analysis time offset is set to 0 sec.

6. Press Analysis Window, 2, 0, and kHz.

The analysis time length is set to 20 msec.

7. Press *Vertical Position*, **0**, and **Hz**.


The vertical offset of the data display is set to 0 Hz.

8. Press Vertical Scale/div, 1, 0, and kHz.

The vertical scale of the data display is set to 10 kHz/div.

9. Press MKR.

An instant frequency at the marker display position can be measured.

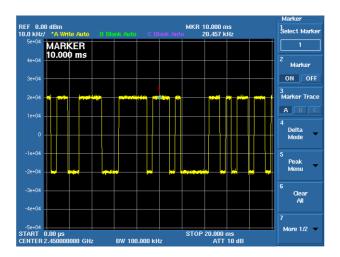

10. Press MEAS 2 and RETURN.

The display returns to the time domain analysis menu.

2.2.2.2 Phase-Time Analysis

Function setting

1. Press *Meas Func*.

The analysis function selection menu is displayed.

2. Press *Phase-Time*.

The analysis function for "phase versus time" is selected.

3. Press **RETURN**.

The display returns to the time domain analysis menu.

The currently selected analysis function is displayed on the Meas Func key.

Display setting

4. Press Display.

Menus for analysis time range setting (horizontal axis) and data display setting (vertical axis) are displayed.

5. Press Analysis Offset, 0, and MHz.

The analysis time offset is set to 0 sec.


6. Press Analysis Window, 1, and kHz.

The analysis time length is set to 1 msec.

2.2.2 Analyzing RF Signal

The change of "time versus phase" can be measured.

The phase is displayed turning back at ± 180 degree.

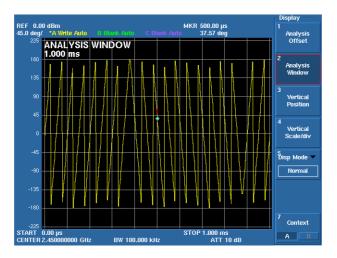

7. Press **RETURN**.

The display returns to the time domain analysis menu.

The currently selected analysis function is displayed on the Meas Func key.

2.2.2.3 Power-Time Analysis

Function setting

1. Press *Meas Func*.

The analysis function selection menu is displayed.

2. Press *Power-Time*.

The analysis function for "power versus time" is selected.

3. Press **RETURN**.

The display returns to the time domain analysis menu.

The currently selected analysis function is displayed on the Meas Func key.


Display setting


4. Press Display.

Menus for analysis time range setting (horizontal axis) and data display setting (vertical axis) are displayed.

5. Press *Vertical Scale/div*, 1, and GHz.

The vertical display scale is set to 1 dB/div.



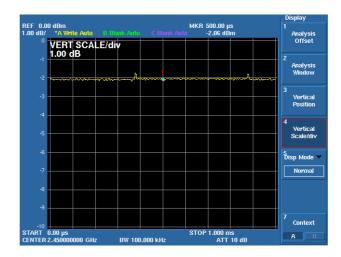

6. Press **RETURN**.

The display returns to the time domain analysis menu.

The currently selected analysis function is displayed on the Meas Func key.

2.2.2.4 IQ-Time Analysis

Function setting

1. Press **TRACE**, *Trace(B)*, *Refresh*, and *Refresh(Write)*.

Trace B is set to Write.

When the IQ-Time analysis function is selected, an I and Q waveform is allocated to Trace A and Trace B, respectively.

2. Press *Trace(C)* and *Trace(A)* in order.

The selected state of Active Trace is changed as Trace $B \to Trace \ C \to Trace \ A$ in order. In this case, Trace A is Active Trace and the Trace A waveform is displayed at the front.

3. Press MEAS 2.

The display returns to the time domain analysis menu.

The currently selected analysis function is displayed on the Meas Func key.

4. Press Meas Func.

The analysis function selection menu is displayed.

5. Press IQ-Time.

The analysis function for "I/Q voltage versus time" is selected.

6. Press **RETURN**.

2.2.2 Analyzing RF Signal

The display returns to the time domain analysis menu.

The currently selected analysis function is displayed on the Meas Func key.

Display setting


7. Press *Display*.

Menus for analysis time range setting (horizontal axis) and data display setting (vertical axis) are displayed.

8. Press Vertical Scale/div, 1, 0, 0, and kHz.

The vertical display scale is set to 100 mV/div.

For I and Q, the change of "time versus voltage" can be measured.

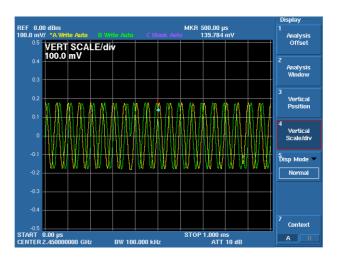

9. Press **RETURN**.

The display returns to the time domain analysis menu.

The currently selected analysis function is displayed on the Meas Func key.

2.2.2.5 Partial FFT Analysis

Function setting

1. Press *Meas Func*.

The analysis function selection menu is displayed.

2. Press *Partial FFT*.

The Partial FFT spectrum analysis function is selected.

Frequency components included in the specified part of the time waveform can be measured.

The analysis start point is set by Analysis Offset. The FFT analysis time length is set to a specific value for each setting value of Capture BW but not set by Analysis Time.

For more information, refer to Chapter 3, "MENU MAP AND FUNCTION DESCRIPTION."

The frequency Span on the FFT spectrum display is the same as the frequency bandwidth set by Capture BW and the frequency resolution is one hundredth of Span.

In this measurement example, Span is 100 kHz, frequency resolution is 1 kHz, and FFT analysis time length is 10 ms because Capture BW=100 kHz. (For the horizontal axis of 1001 points)

3. Press **RETURN**.

The display returns to the time domain analysis menu.

The currently selected analysis function is displayed on the Meas Func key.

Display setting


4. Press Display.

Menus for analysis time range setting (horizontal axis) and data display setting (vertical axis) are displayed.

5. Press Vertical Scale/div, 1, 0, and GHz.

The vertical display scale is set to 10 dB/div.

The Partial FFT spectrums are displayed and frequency components included in the specified part of the time waveform can be measured.

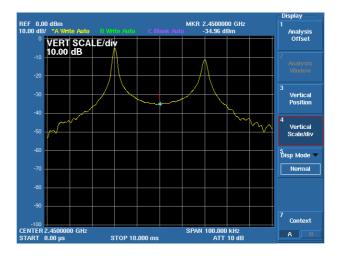

6. Press **RETURN**.

The display returns to the time domain analysis menu.

The currently selected analysis function is displayed on the Meas Func key.

2.2.2 Analyzing RF Signal

2.2.2.6 Freq-Time Analysis Using Position View Function

Function setting

1. Press *Meas Func*.

The analysis function selection menu is displayed.

2. Press *Freq-Time*.

The analysis function for "frequency versus time" is selected.

3. Press **RETURN**.

The display returns to the time domain analysis menu.

The currently selected analysis function is displayed on the Meas Func key.

Display setting

4. Press Display.

Menus for analysis time range setting (horizontal axis) and data display setting (vertical axis) are displayed.

5. Press Analysis Window, 2, 0, and kHz.

The analysis time length is set to 20 msec.

6. Press Analysis Offset, 1, 0, and kHz.

The analysis time offset is set to 10 msec.

7. Press *Vertical Position*, **0**, and **Hz**.

The vertical offset of the data display is set to 0 Hz.

8. Press Vertical Scale/div, 1, 0, and kHz.

The vertical scale of the data display is set to 10 kHz/div.

9. Press *Display Mode* and *Position View* to select the Position View function.

The lower screen displays the analysis result for the entire waveform capture time. The window displayed in the lower screen indicates the position of the set analysis time.


The upper screen displays the analysis result for the time set by analysis time length and offset.

10. Press EXT CFG and Sweep Mode SGL/CNT to select SGL.

The sweep mode is set to Single.

11. Press START/STOP.


Capturing an RF signal starts.

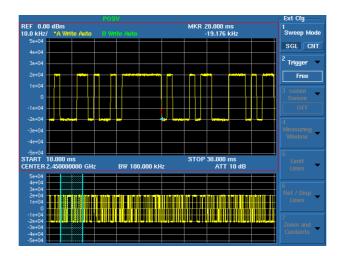

12. Press MEAS2 and RETURN.

Press Analysis Offset and Analysis Window in the Display menu and change the set value.

The analysis position and analysis result can be checked.

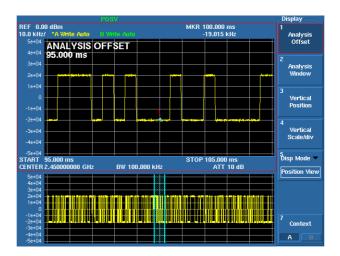

13. Press *Disp Mode* and *Normal*.

The Position View mode is canceled.

14. Press **RETURN** twice.

The display returns to the time analysis menu.

15. Press EXT CFG and Sweep Mode SGL/CNT to select CNT.

The sweep mode is set to CNT.

CAUTION: To make the analysis window content in the lower screen match the analysis result in the upper screen, set the sweep mode to Single and capture data by pressing START/STOP.

2.2.2 Analyzing RF Signal

2.2.2.7 Two-Type Simultaneous Analysises Using Dual Meas Function (Freq-Time and Phase-Time)

Function setting

1. Press **MEAS2** and *Meas Func*.

The analysis function selection menu is displayed.

2. Press *Freq-Time*.

The analysis function for "frequency versus time" is selected.

3. Press **RETURN**.

The display returns to the time domain analysis menu.

The currently selected analysis function is displayed on the Meas Func key.

Display setting

4. Press Display.

Menus for analysis time range setting (horizontal axis) and data display setting (vertical axis) are displayed.

5. Press Analysis Window, 1, and kHz.

The analysis time length is set to 1 msec.

6. Press Analysis Offset, 0, and kHz.

The analysis time offset is set to 0 sec.

7. Press *Vertical Position*, **0**, and **Hz**.

The vertical offset of the data display is set to 0 Hz.

8. Press Vertical Scale/div, 1, 0, and kHz.

The vertical scale of the data display is set to 10 kHz/div.

9. Press *Disp Mode* and *Dual Measure* to select the Dual Measure function.

At this time, Analysis Offset and Analysis Window values are copied to the lower screen.

Display setting (lower screen)

10. Press Context A/B to select B.

11. Press **RETURN** twice.

The display returns to the time domain analysis menu.

12. Press Meas Func.

The analysis function selection menu is displayed.

13. Press *Phase-Time*.


The analysis function for "phase versus time" is selected.

14. Press EXT CFG and Sweep Mode SGL/CNT to select SGL.

The sweep mode is set to Single.

15. Press START/STOP.

Capturing an RF signal starts.

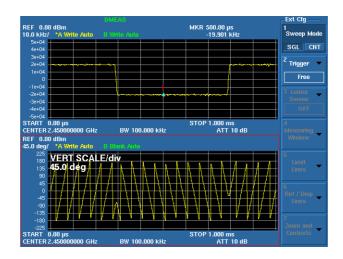

16. Press MEAS2 and RETURN.

Press *Analysis Offset* and *Analysis Window* in the Display menu and change the set value.

Only the analysis time in the lower screen can be changed.

Based on the captured data, analysis can be performed with independent settings for the upper and lower screens.


17. Press *Disp Mode* and *Normal*.

The Dual Measure mode is canceled.

2.3 OPT55 Pulse Modulation Signal Measurement Example

2.3 OPT55 Pulse Modulation Signal Measurement Example

In this section, a PM (Pulse Modulation) signal is measured.

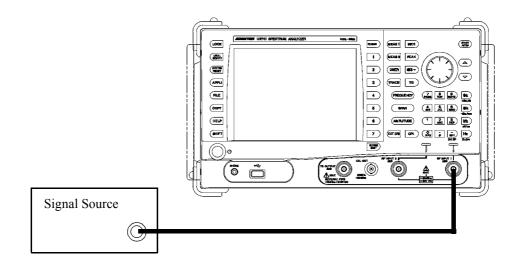

Signal Source output

Frequency: 1.5 GHz Power: -20 dBm

Modulation Type: Pulse Modulation


Period: $10 \mu s$ Width: $1 \mu s$

Operation

Setting the Center Frequency:

- 1. Press **SHIFT** and **SYSTEM(PRESET)**. Initial setting conditions are loaded.
- 2. Press **FREQUENCY**, **1**, **5**, **0**, **0**, and **MHz**. The center frequency is set to 1500 MHz.
- 3. Press **SPAN**, **1**, **0**, and **MHz**. The frequency span is set to 10 MHz.

2.3 OPT55 Pulse Modulation Signal Measurement Example

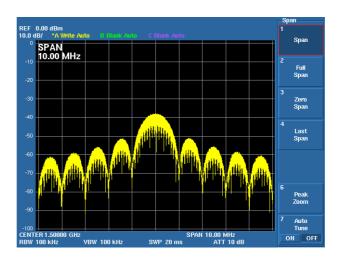

Power-Time analysis

4. Press MEAS2, More1/2, and Time Domain.

The time domain analysis menu is displayed.

5. Press *Meas Func* and *Power-Time*.

The analysis function for "power versus time" is selected.

6. Press **RETURN**.

The display returns to the time domain analysis menu.

The currently selected analysis function is displayed on the Meas Func key.

7. Press Capture Config.

The waveform capture setting menu is displayed.

8. Press Capture BW, 3, 0, and MHz.

The waveform capture bandwidth is set to 30 MHz.

9. Press *Capture Time*, **5**, **0**, and **Hz**.

The waveform capture time is set to 50 µs.

10. Press **RETURN** and *ExecuteON/OFF(ON)*.

Execute the Power-Time analysis function.

Pulse width measurement

11. Press EXT CFG, Trigger, Source, and IF.

The IF trigger is selected.

12. Press MEAS2, Display, Analysis Window, 2, 0, and Hz.

The analysis time length is set to 20 µs.


2.3 OPT55 Pulse Modulation Signal Measurement Example

13. Press RETURN, Measures, Threshold ON/OFF(ON), -, 3, 0, and GHz.

The Threshold line used as reference of Measures is set to -30 dBm.

14. Press Width and Positive Width.

The pulse width measurement result across the -30 dBm level is displayed in the lower part of the screen.

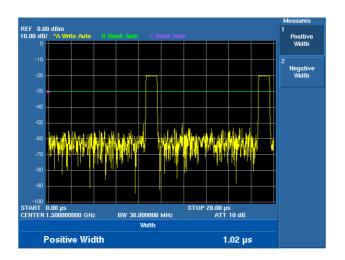

2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56)

2.4 2-Channel Time Domain Analysis Option (OPT54/OPT56)

2.4.1 Main Basic Operations with 2-Channel Specifications

For more information, refer to U3700 Series OPT10/OPT11 2 Channel Input Option User's Guide.

Key operations are enabled for a selected active channel.

In addition, the Couple CH function enables settings to both channels at the same time by a single key operation.

Selecting Active Channel

Operation

SHIFT, - (RF1) Select channel 1.
 SHIFT, 0 (RF2) Select channel 2.
 APPLI, Couple CH ON/OFF (ON) or SHIFT, · (#)

Sets the Couple CH mode ON.


When Couple CH is ON, some of the functions set to both channels at the same time differ between ON and OFF of the Time Domain function.

Fun	ction	Time D	omain
Panel key	Menu	OFF	ON
FREQUENCY	Center	~	✓
	Start	~	
	Stop	~	
SPAN	Span	~	
	Full Span	~	
	Zero Span	~	
CPL	RBW	~	
	VBW	~	
	Sweep Time	~	
	All Auto	~	
(Display)	Analysis Offset	~	~
	Analysis Window	~	~
(Capture Config)	Capture Time	~	~
	Capture BW	~	✓
START/STOP		<u> </u>	<u> </u>

2.4.2 Example of Four-Value FSK Signal Analysis

2.4.2 Example of Four-Value FSK Signal Analysis

This section measures a frequency change for four-value FSK signal time on the time axis and frequency axis at the same time.

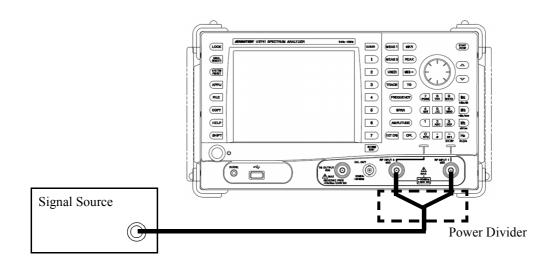

Signal Source output

Frequency: 150 MHz

Power: 0 dBm

Modulation Type: 4FSK

Frequency Deviation: 9.6 kHzp-p


Baseband Signal: 3.2 kHz PRBS

Operation

Setting the Center Frequency

1. Press SHIFT and SYSTEM(PRESET).

Initial setting conditions are loaded. Channel 1 is set to the active channel.

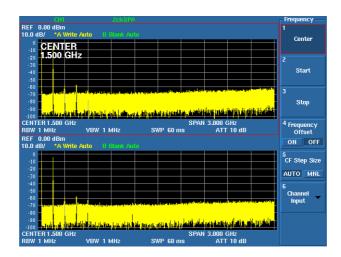

2. Press SHIFT and · (#).

The Couple CH mode turns ON and key operations are enabled for both channels. The red rectangular box on the screen surrounds the channel 1 window.

A function setting whose key operation is not enabled for both channels is only applied to channel 1.

3. Press FREQUENCY, 1, 5, 0, and MHz.

The center frequency is set to 150 MHz for both channels 1 and 2.

Channel 1: Freq-Time Analysis

4. Press MEAS2, More1/2, Time Domain, and Execute ON/OFF (ON).

Execute the Freq-Time analysis function.

5. Press Capture Config.

The waveform capture setting menu is displayed.

6. Press Capture BW, 1, 0, and kHz.

The waveform capture bandwidth is set to 10 kHz.

7. Press *Capture Time*, 1, 0, 0, and kHz.

The waveform capture time is set to 100 ms.

8. Press **RETURN**.

The display returns to the time domain analysis menu.


9. Press *Display*.

Menus for analysis time range setting (horizontal axis) and data display setting (vertical axis) are displayed.

10. Press Vertical Scale/div, 2, and kHz.

The vertical scale of the data display is set to 2 kHz/div.

2.4.2 Example of Four-Value FSK Signal Analysis

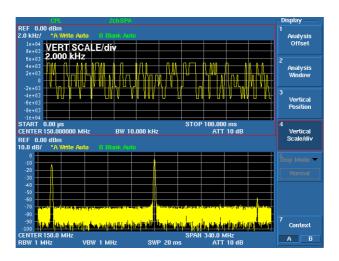

Channel2: Spectrum Display by Partial FFT Analysis

11. Press SHIFT and 0 (RF2).

Channel 2 is set to the active channel.

12. Press **RETURN**.

The display returns to the time domain analysis menu.

13. Press Meas Func and Partial FFT.

The Partial FFT spectrum analysis function is selected.

14. Press RETURN and Execute ON/OFF (ON).


Execute the Partial FFT spectrum analysis function.

At this time, the waveform capture bandwidth (10 kHz) and the capture time (100 ms) are set in steps 6 and 7, which are performed while Couple CH is ON.

15. Press TRACE, Calc, and Max Hold.

Max Hold starts.

2.4.2 Example of Four-Value FSK Signal Analysis

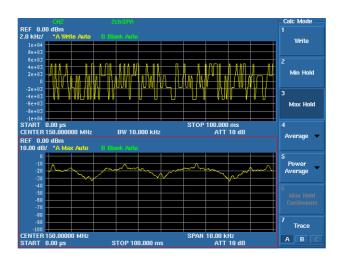

Changing Capture BW

16. Press MEAS2 and Capture Config.


The waveform capture setting menu is displayed.

17. Press Capture BW, 1, 0, 0, and kHz.

The waveform capture bandwidth is set to 100 kHz.

At this time, channel 2 is an active channel.

Because the Couple CH function is cancelled, the waveform capture bandwidth is set only for channel 2.

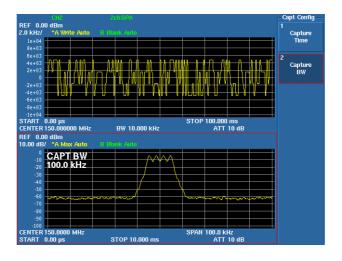

3. MENU MAP AND FUNCTION DESCRIPTION

3. MENU MAP AND FUNCTION DESCRIPTION

This chapter describes the functions of the panel keys and soft keys in the items shown below.

Menu Map: This section shows the menu configurations of the panel keys.

Functional Descriptions: This section describes the functions of the panel keys and soft keys.

3.1 Functional Descriptions


This section describes the functions of the panel keys and soft keys.

MEMO:

- indicates a panel key.
- All other names are soft menus.

3.1.1 Time Domain

Displays the Time Domain menu.

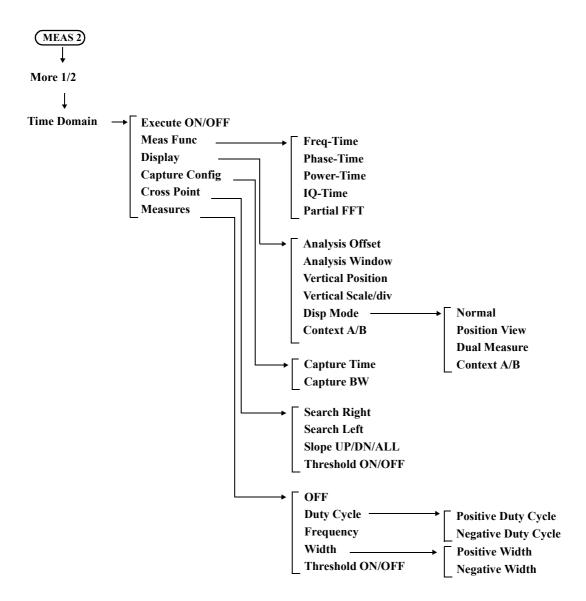

Time Domain Displays the time domain analysis menu.

Execute ON/OFF Selects ON or OFF of the time domain analysis function.

Meas Func Selects the time domain measurement function.

The currently selected analysis function is displayed on the Meas

Func key.

Freq-Time Displays a change of "measured signal frequency versus time"

based on the center frequency setting value of the analyzer.

Phase-Time Displays a change of "measured signal phase versus time" based

on the center frequency setting value of the analyzer.

Power-Time Displays a change of "measured signal power versus time".

IQ-Time Displays a change of "measured signal I/Q voltages versus time".

An I and Q waveform is captured and displayed on Trace A and

Trace B, respectively.

Partial FFT Displays frequency spectrums of the measured signal.

The frequency span is the same as Capture BW. The resolution

bandwidth is one hundredth of span.

The Partial FFT analysis start point is specified by Analysis Offset. The analysis data length is the fixed length but not set by

Analysis Window. (See Table 3-1 and Table 3-2.)

Display Sets the analysis time (horizontal axis) and analysis result (verti-

cal axis) display ranges.

Analysis Offset Sets the analysis start point (Offset time from the top of the cap-

tured waveform) of the measured signal waveform captured in the

analyzer.

Analysis Window Sets the analysis time length (time that starts at the Analysis Off-

set setting value) of the measured signal waveform captured in the

analyzer.

For the Partial FFT analysis, the analysis time length is a value

that depends on Capture BW and the number of horizontal points

(See Table 3-1 and Table 3-2.).

Vertical Position Sets the vertical display position of the analysis result.

For each analysis function selected by Meas Func, each indepen-

dent vertical display position is set.

Vertical Scale/div Sets the vertical display scale of the analysis result.

For each analysis function selected by Meas Func, each indepen-

dent vertical display scale is set.

Disp Mode Selects a screen mode.

Normal Sets the measurement screen to the single-screen display mode.

Position View Sets the Position View function. The display is divided into upper

and lower screens.

The upper and lower screens display the analysis results of the

same captured waveform data.

The upper screen displays the normal analysis result.

The lower screen displays the result for the entire captured time range of the obtained data.

The blue window in the lower screen displays the analysis start time and analysis time length for the upper screen.

Upper screen: Analysis Window=user set value,

Analysis Offset=user set value

Lower screen: Analysis Window=Capture Time (fixed),

Analysis Offset=0sec (fixed)

Dual Measure

Sets the Dual Measure function. The display is divided into upper and lower screens.

The upper and lower screens display the analysis results of the same captured waveform data.

Different analysis functions can be set individually to the upper and lower screens. Also, the vertical axis display position, vertical axis scale, analysis start time, and analysis time length can be set for each screen.

Context A/B

Switches the active screen between A (upper screen) and B (lower screen).

A: The upper screen settings can be changed.

B: The lower screen setting can be changed.

Context A/B

Selects the screen, for which the setting is to be made, when Dual Meas ON is set.

Capture Config

Sets the capture time length of the waveform captured in the analyzer and the frequency bandwidth.

Capture Time

Sets the capture time length of the waveform captured in the analyzer.

The maximum capture time depends on the Capture BW setting. (See Table 3-3 and Table 3-4.)

Capture BW

Sets the frequency bandwidth of the waveform captured in the analyzer

For the Capture BW setting, Capture Time is automatically limited to a value within the maximum capture time. (See Table 3-3 and Table 3-4.)

Table 3-1 OPT53/OPT54 Capture BW Setting Value and Partial FFT Frequency Resolution

Capture BW	Partial FFT	Partial FFT ana	lysis data length
Bandwidth setting value	Frequency resolution	Horizontal axis of 1001 points	Horizontal axis of 501 points
3 MHz	30 kHz	0.33 msec	0.165 msec
1 MHz	10 kHz	1 msec	0.5 msec
300 kHz	3 kHz	3.3 msec	1.65 msec
100 kHz	1 kHz	10 msec	5 msec
30 kHz	300 Hz	33 msec	16.5 msec
10 kHz	100 Hz	100 msec	50 msec
3 kHz	30 Hz	330 msec	165 msec
1 kHz	10 Hz	1 sec	500 msec
300 Hz	3 Hz	3.3 sec	1.65 sec
100 Hz	1 Hz	10 sec	5 sec

Table 3-2 OPT55/OPT56 Capture BW Setting Value and Partial FFT Frequency Resolution

Capture BW	Partial FFT	Partial FFT ana	lysis data length
Bandwidth setting value	Frequency resolution	Horizontal axis of 1001 points	Horizontal axis of 501 points
40 MHz	400 kHz	25 μsec	12.5 µsec
30 MHz	300 kHz	33 μsec	16.5 µsec
10 MHz	100 kHz	100 μsec	50 μsec
3 MHz	30 kHz	330 μsec	0.165 msec
1 MHz	10 kHz	1 msec	0.5 msec
300 kHz	3 kHz	3.3 msec	1.65 msec
100 kHz	1 kHz	10 msec	5 msec
30 kHz	300 Hz	33 msec	16.5 msec
10 kHz	100 Hz	100 msec	50 msec
3 kHz	30 Hz	330 msec	165 msec
1 kHz	10 Hz	1 sec	500 msec
300 Hz	3 Hz	3.3 sec	1.65 sec
100 Hz	1 Hz	10 sec	5 sec

Table 3-3 OPT53/OPT54 Capture BW Setting Value and Capture Time Maximum Value

Capture BW Bandwidth setting value	Capture Time Maximum capture time
3 MHz	50 msec
1 MHz	150 msec
300 kHz	500 msec
100 kHz	1.5 sec
30 kHz	5 sec
10 kHz	15 sec
3 kHz	50 sec
1 kHz	150 sec
300 Hz	500 sec
100 Hz	1000 sec

Table 3-4 OPT55/OPT56 Capture BW Setting Value and Capture Time Maximum Value

Capture BW Bandwidth setting value	Capture Time Maximum capture time
40 MHz	120 ms
30 MHz	120 ms
10 MHz	240 ms
3 MHz	600 msec
1 MHz	2.0 sec
300 kHz	6.0 sec
100 kHz	20 sec
30 kHz	60 sec
10 kHz	200 sec
3 kHz	600 sec
1 kHz	1000 sec
300 Hz	1000 sec
100 Hz	1000 sec

Cross Point Detects waveform edges (rising and falling).

Search Right Searches in the right direction from the active marker.

Search Left Searches in the left direction from the active marker.

Slope UP/DN/ALL

UP: Searches for waveform rising points and moves

the active marker there.

Waveform rising points refer to where the waveform

crosses the threshold line from down to up.

DN: Searches for waveform falling points and moves the

active marker there.

Waveform falling points refer to where the waveform

crosses the threshold line from up to down.

ALL: Searches for waveform rising and falling points

alternatively and moves the active marker there.

Threshold ON/OFF Select ON/OFF for the threshold line.

This is the reference line for Cross Point search.

Measures Performs measurement for the time domain screen.

OFF Quits measuring.

Duty Cycle Displays Duty Cycle measurement menus.

Positive Duty Cycle

Measures the ratio of the positive pulse width contained in the

first cycle.

Positive Duty Cycle(%) = Positive pulse width / Cycle * 100%

Negative Duty Cycle

Measures the ratio of the negative pulse width contained in the

first cycle.

Negative Duty Cycle(%) = Negative pulse width / Cycle * 100%

Frequency Measures the frequency in the first cycle.

Frequency(Hz) = 1 / Cycle

Width Displays Width measurement menus.

Positive Width Measures the positive pulse width.

Positive Width(sec) = (The point where a waveform first crosses the threshold line from up to down) - (The point where a wave-

form first crosses the threshold line from down to up)

Negative Width Measures the negative pulse width.

Negative Width(sec) = (The point where a waveform first crosses the threshold line from down to up) - (The point where a wave-

form first crosses the threshold line from up to down)

Threshold ON/OFF Select ON/OFF for the threshold line.

This is the reference line for Measures.

 $3.1.2 \text{ MKR} \rightarrow$

3.1.2 MKR→

When the time domain analysis function is on, the MKR→ function changes according to the selected measurement function.

Meas Func: Freq-Time, Phase-Time, Power-Time, or IQ-Time

MKR → Mkr to Analysis Ofs
Delta to Analysis Win
Mkr to Vertical Pos
Delta to V Scale/div
Mkr to Mkr Step

Mkr to Analysis Ofs Sets the time at the active marker as the analysis start point.

Delta to Analysis Win Sets the time difference between delta and normal markers as the

analysis time length.

Mkr to Vertical Pos Sets the level at the active marker as the vertical axis display posi-

tion.

Delta to V Scale/div Sets the level difference between delta and normal markers as the

vertical axis display scale.

Mkr to Mkr Step Sets the time at the active marker as the step size of the marker.

Meas Func: Partial FFT

MKR→ → Mkr to CF
Peak to CF
Mkr to Vertical Pos
Delta to V Scale/div
Mkr to CF Step
Mkr to Mkr Step
Peak to Ref

Mkr to CF Sets the frequency at the active marker as the center frequency.

Peak to CF Displays the marker at the highest peak in the search target range

and sets the frequency at the marker as the center frequency.

Mkr to Vertical Pos Sets the level at the active marker as the vertical axis display posi-

tion.

Delta to V Scale/div Sets the level difference between delta and normal markers as the

vertical axis display scale.

Mkr to CF Step Sets the frequency at the active marker as the step size of the cen-

ter frequency.

Mkr to Mkr Step Sets the frequency at the active marker as the step size of the

narker

Peak to Ref Displays the marker at the highest peak in the search target range

and sets the level at the marker as the reference level.

4. OVERVIEW OF REMOTE CONTROL

This chapter describes the AT command reference for this instrument.

4.1 GPIB Remote Programming

This section shows the AT commands in each function:

Command code

An asterisk "*" indicates a function that numeric or character strings data follows after the code. Numeric data and "ON" can be omitted from [].

- Output format
 - A comma "," indicates that two or more data are output.
 - ON or OFF indicates that 1 or 0 is output.
 - Frequency is output in Hz and time is output in sec.
 - Level data is output in the currently set display unit.

4.2 AT Command Code List

Function	Comm	and (EXE, SET)	Que	ry (GET)
runction	Code	Argument Format	Code	Output Format
Time Domain Analysis	TDANA	ON/OFF	TDANAON?	0:OFF 1:ON
Analysis Offset	TDAOFS	Time	TDAOFS?	Time
Analysis Window	TDATIM	Time	TDATIM?	Time
Vertical Scale IQ	VSCLIQ	Voltage	VSCLIQ?	Voltage
Vertical Scale Power	VSCLPWR	Power	VSCLPWR?	Power
Vertical Scale Freq	VSCLFRE	Frequency	VSCLFRE?	Frequency
Vertical Scale Phase	VSCLPHA	Phase	VSCLPHA?	Phase
Vertical Scale FFT	VSCLFFT	Level	VSCLFFT?	Level
Vertical Position IQ	VPOSIQ	Position	VPOSIQ?	Position
Vertical Position Power	VPOSPWR	Position	VPOSPWR?	Position
Vertical Position Freq	VPOSFRE	Position	VPOSFRE?	Position
Vertical Position Phase	VPOSPHA	Position	VPOSPHA?	Position
Vertical Position FFT	VPOSFFT	Position	VPOSFFT?	Position

4.2 AT Command Code List

Familian	Comm	and (EXE, SET)	Que	ery (GET)
Function	Code	Argument Format	Code	Output Format
Measurement Function	TMEAS	FRE/PHA/PWR/IQ/FFT	TMEAS?	0:FRE 1:PHA 2:PWR 3:IQ 4:FFT
Capture Time	CAPTIM	Time	CAPTIM?	Time
Capture BW	CAPBW	Frequency	CAPBW?	Frequency
Display Mode	TDDISP *	NORM POSV DUAL	TDDISP?	0=Normal 1=Position View 2=Dual Measure
Cross point Search Right	CRSPR			
Cross point Search Left	CRSPL			
Slope	CRSSLP *	UP DN ALL	CRSSLP?	0=Up 1=Down 2=All
Threshold	THRIQ * THRPWR * THRFRE * THRPHA * THRFFT * THRESH ON OFF	Volt dBm Frequency Phase dBm	THRIQ? THRPWR? THRFRE? THRPHA? THRFFT? THRESHON?	Volt dBm Frequency Phase dBm 0=OFF 1=ON
Measures	DMEAS *	OFF/DTYP/DTYN FREQ/WIDP/WIDN	DMEAS?	0:OFF 1:Pos Duty 2:Neg Duty 3:Freq 4:Pos Wid 5:Neg Wid
Measures Result			DMEASRES?	Real
Mkr to Analysis Offs	MKAO			
Delta Mkr to Analysis Win	MTAW			
Mkr to Vertical Pos	MKVP			
Delta Mkr to scale/div	MTDIV			
IQ Output Binary			IQB?	8 bytes x IQP (*1)
IQ Output Scale			IQS?	Real
IQ Output Points			IQP?	Points
IQ Sample Rate			IQR?	Frequency
ALL IQ Sample Points			IQPAL?	Points
Clear IQP value	IQPRST			

(*1) IQP: Number of IQ Pair Sample Points

4.3 I/Q Data Output

Data output by IQB? is in Binary (32bit) format, and I and Q are alternately output.

IQ-Pair data output (8xN bytes) of N obtained samples (0 to N-1)

Sample number	()]	1			N	-2	N	-1
IQB? Data	I ₀	Q_0	I ₁	Q ₁	•••	•••	I _{N-2}	Q _{N-2}	I _{N-1}	Q _{N-1}
Size Bytes	4	4	4	4	4	4	4	4	4	4

Data output by IQB? shows a relative value between I and Q, and it can be used for phase angle calculation.

Data output by IQS? shows scaling data for absolute value conversion of I and Q Pair.

Data output by IQPAL? shows the number of all I and Q Pairs which were captured.

Data output by IQP? shows the number of samples (N) of I and Q Pairs which is returned from the next-called IQB?.

Data output by IQR? shows a sampling frequency of I and Q Pair.

IQPRST returns the IQP? value to the initial value.

Voltages (V_{IN}, V_{QN}) that correspond the Nth data (I_N, Q_N) of I and Q output can be obtained by using the following equations.

$$V_{IN}=I_N \times IQS$$
 [V]

$$V_{ON} = Q_N \times IQS \quad [V]$$

Example:

Obtain all IQ data items when the return value of IQPAL? is the 4.5M sample.

- 1. The first IQP? returns 2Mi, so obtain the 2M sample data by IQB?.
- 2. The second IQP? also returns 2Mi, so obtain the 2M sample data by IQB?.
- 3. The third IQP? returns 0.5Mi, so obtain the 0.5M sample data by IQB?.
- 4. The fourth IQP? returns 0, so the obtaining of data is complete.

Repeat IQB? to obtain all data items until IQP? returns 0.

Using the TS or IQPRST command returns to the initial state.

5. SPECIFICATIONS

This chapter describes the specifications of this instrument.

The performance of this instrument is guaranteed under the following conditions unless otherwise specified.

- The specified calibration period must be adhered to.
- After turning on the power and warming-up for 5 minutes or more under the specified environmental conditions.
- After automatic calibration has been performed.

5.1 Option 53, Option 54 Time Domain Analysis Option

Item	Description
RF frequency range	Conforms to the frequency range for each model of the U3700 series.
RF amplitude range	Noise level to +30 dBm (*1)
Waveform capture format	I/Q vector time waveform
Measurement bandwidth (BW)	100 Hz to 3 MHz (1 to 3 steps)
I/Q sampling rate	713 Hz (BW 100 Hz) to 21.4 MHz (BW 3 MHz)
I/Q waveform capture time	49 msec (BW 3 MHz) to 1000 sec (BW 100 Hz)
Number of I/Q waveform capture samples	1 M Samples (I/Q)

^(*1) The noise level conforms to the dynamic range specifications for each model of the U3700 series.

5.2 Option 55, Option 56 Time Domain Analysis Option

Item	Description
RF frequency range	Conforms to the frequency range for each model of the U3700 series.
RF amplitude range	Noise level to +30 dBm (*1)
Waveform capture format	I/Q vector time waveform
Measurement bandwidth (BW)	100 Hz to 30 MHz (1 to 3 steps), 40 MHz
I/Q sampling rate	500 Hz (BW 100 Hz) to 65 MHz (BW 40 MHz)
I/Q waveform capture time	120 msec (BW 40 MHz) to 1000 sec (BW 100 Hz)
Number of I/Q waveform capture samples	8 M Samples (I/Q)

^(*1) The noise level conforms to the dynamic range specifications for each model of the U3700 series.

6. UNCAL MESSAGE, LIST OF ERROR MESSAGES, AND RESTRICTIONS

6. UNCAL MESSAGE, LIST OF ERROR MESSAGES, AND RESTRIC-TIONS

6.1 How to Delete UNCAL Message for Partial FFT Analysis

The Partial FFT analysis uses time length data that is related to the Capture BW setting value (equal to the displayed frequency Span). If the data length required for FFT analysis is insufficient, the UNCAL message is displayed to show the displayed value may not be correct.

The UNCAL message is displayed if a relationship among each setting value of the FFT analysis data length, which is shown in Table 3-1 "Capture BW Setting Value and Partial FFT Frequency Resolution" of Chapter 3, Capture Time, and Analysis Offset does not satisfy the following equation:

FFT analysis data length ≥ (Capture Time - Analysis Offset)

To delete the UNCAL message, perform either or both of the following (1) and (2).

- (1) Increase the Capture Time setting value.
- (2) Decrease the Analysis Offset setting value.

For more information on the Partial FFT analysis, refer to Chapter 3, "MENU MAP AND FUNCTION DESCRIPTION."

6.2 List Of Error Messages

6.2 List Of Error Messages

This chapter describes error messages regarding OPT53 and OPT54.

Error code	Туре	Displayed Message	Description of Message
0/500	WARNING	The Analysis Window is out of range. (Analysis Offset + Analysis Window <= Capture Time)	The Analysis Window value cannot be set. Ensure that the value of [Analysis Offset + Analysis Window] does not exceed the Capture Time value.
0/501	WARNING	The Analysis Offset is out of range. (Analysis Offset + Analysis Window <= Capture Time)	The Analysis Offset value cannot be set. Ensure that the value of [Analysis Offset + Analysis Window] does not exceed the Capture Time value.
3/500	WARNING	The Time Domain Analysis mode has been turned off.	The time domain analysis mode is canceled.

6.3 Restrictions

This section describes restrictions on the time domain analysis function.

6.3.1 Restrictions on Key Operation during Time Domain Analysis Function Use

When the time domain analysis function is set to ON, some key operations such as the frequency sweep Span setting are temporarily unavailable. Unavailable keys are displayed in gray.

These are available again by setting the time domain analysis function to OFF.

6.3.2 Restrictions for Trace Data Capture

When the time domain analysis function is set to ON or OFF, or the analysis function is switched by Meas Func, waveform data retained in the trace memory is invalid.

By operating **TRACE**, *Refresh*, and *Refresh(Write)*, the trace memory can be updated to the latest waveform.

ALPHABETICAL INDEX

Content of This Manual 1-1	[Numerics]			[G]		
[H] Analysis Offset Analysis Window Ascapture Time Contents of This Manual Co					4-1	
Image: content of the content of t		2-19				
Analysis Offset	(,			F1.13		
Analysis Offset 3.2, 3.3	FA1					
Analysis Window						
B			3-3	Partial FFT Analysis	6-1	
International Code List			3-3			
B	Analyzing RF Signal	2-6		[11		
B INSTRUMENT CONFIGURATION 2-1 INTRODUCTION 1-1 INTRODUCTI	AT Command Code List	4-1			1 2	
[B] BASIC OPERATIONS 2-1 INTRODUCTION 1-1 IQ-Time						
Capture BW 3-2, 3-4 Capture Config 3-2, 3-4 Capture Time 3-2, 3-7 Capture Time 3	[R]					
Capture BW		2 1				2 -
Capture BW	BASIC OPERATIONS	2-1				3-3
List Of Error Messages 6-2				IQ-Time Analysis	2-9	
List Of Error Messages 6-2	[C]					
Capture Config 3-2, 3-4 List Of Error Messages 6-2 Capture Time 3-2, 3-4 List Of Error Messages 6-2 Capturing I/Q Waveforms of RF Signal Contents of This Manual 1-1 Image: Conventions of Notation Used In This Document 1-1 Image: Conventions of Notation Used In This Document 1-2 Main Basic Operations with 2-Channel Specifications 2-19 MEAS 2 3-3 Mkr to Analysis Ofs 3-9 Mkr to CF 3-9 Mkr to CF Step 3-9 3-9 Mkr to Wertical Pos 3-9 Mkr to Wertical Pos 3-9 3-9 Mkr to Vertical Pos 3-9 Nama sand Functions of Each Part		3-2,	3-4	[L]		
Capture Time 3-2, 3-4 Capturing I/Q Waveforms of RF Signal 2-5 Contents of This Manual 1-1 Context A/B 3-2, 3-4 Convext A/B 3-2, 3-7 Conventions of Notation Used in This Document 1-2 Cross Point 3-2, 3-7 MEAS 2 3-2 Meas Func 3-2, 3-2 Measures 3-2, 3-2 MENU MAP 3-1 Mix to CF 3-9 Delta to Analysis Win 3-9 Mkr to CF 3-9 Disp Mode 3-2, 3-3 Mkr to Mkr Step 3-9 Display 3-2, 3-3 Mkr to Wertical Pos 3-9 Duty Cycle 3-2, 3-4 MKR→ 3-9 Duty Cycle 3-2, 3-7 More 1/2 3-2 EE IN Names and Functions of Each Part on Screen 2-1 Execute ON/OFF 3-2, 3-3 Names and Functions of Each Part on Screen 2-1 Ereq-Time Analysis Using Position View Function 2-1 Negative Duty Cycle 3-2, 3-2 Negative Duty Cycle 3-2, 3-2 3-2 3-2 Freq-Time, P					6-2	
Capturing I/Q Waveforms of RF Signal 2-5 [M] Contents of This Manual 1-1 A-2 Conventions of Notation Used in This Document 1-2 Main Basic Operations with 2-Channel Specifications 2-19 Cross Point 3-2, 3-7 3-7 Meas Func 3-2, 3-2 Measures 3-2, 3-7 3-2 3-2 Measures 3-2, 3-3 3-2 3-2 Measures 3-2, 3-3 3-2 3-2 Measures 3-2, 3-3 3-9 Mkr to CF 3-9 Delta to V Scale/div 3-9 Mkr to CF 3-9 Display 3-2, 3-3 Mkr to Wr tstep 3-9 Display 3-2, 3-3 Mkr to Vertical Pos 3-9 Duty Cycle 3-2, 3-3 Mkr to Vertical Pos 3-9 Duty Cycle 3-2, 3-7 More 1/2 3-2 Execute ON/OFF 3-2, 3-3 Names and Functions of Each Part on Screen 2-1 Execute ON/OFF 3-2, 3-3 Names and Functions of Each Part on Screen 2-3 Negative Width 3-2, 3-						
Contents of This Manual 1-1 Context A/B 3-2 3-4 Conventions of Notation Used in This Document 1-2 Cross Point 3-2 3-2 3-7 Meas Func 3-2 3-2 3-7 Measures 3-2 3-2 3-7 Measures 3-2 3-7			_	FBA3		
Context A/B 3-2, 3-4 Main Basic Operations with 2-Channel Specifications Specifi	Contents of This Manual	1-1				
Conventions of Notation Used in This Document			3-4			
In This Document		J _ ,	<i>J</i> .			
Cross Point 3-2, 3-7 Meas Func 3-2, 3-7 Measures 3-2, 3-7 Measures 3-2, 3-7 Measures 3-2, 3-7 Ment of Measures 3-2, 3-7 Ment of Measures 3-9 Ment of Me		1-2				
ID MESUURES 3-2, 3-3 MENU MAP 3-1 Mkr to Analysis Ofs 3-9 Delta to Analysis Win 3-9 Mkr to CF 3-9 Delta to V Scale/div 3-9 Mkr to CF Step 3-9 Disp Mode 3-2, 3-3 Mkr to Mkr Step 3-9 Display 3-2, 3-3 Mkr to Vertical Pos 3-9 Dual Measure 3-2, 3-4 MKR→ 3-9 Duty Cycle 3-2, 3-7 More 1/2 3-2 IE			3-7			3-3
ID Mkr to Analysis Ofs 3-9 Delta to Analysis Win 3-9 Mkr to CF 3-9 Delta to V Scale/div 3-9 Mkr to CF Step 3-9 Disp Mode 3-2, 3-3 Mkr to Mkr Step 3-9 Display 3-2, 3-3 Mkr to Vertical Pos 3-9 Dual Measure 3-2, 3-4 MKR→ 3-9 Duty Cycle 3-2, 3-7 More 1/2 3-2 Example of Four-Value FSK Signal Names and Functions of Each Part on Screen 2-1 Execute ON/OFF 3-2, 3-3 Names and Functions of Each Part on the Screen 2-3 Execute ON/OFF 3-2, 3-3 Negative Duty Cycle 3-2, 3-7 Freq-Time 3-2, 3-3 Negative Duty Cycle 3-2, 3-7 Normal 3-2, 3-3 Normal 3-2, 3-3 Normal 3-2, 3-3 Normal 3-2, 3-3 Normal 3-2, 3-3 Normal 3-2, 3-3 Normal 3-2, 3-3 Normal 3-2, 3-7 Preq-Time Analysis Using Position 2-12 IO Freq-Time, Phase-Time, Power-Time, Operating, Power-Time, Operating Method 2-4 <	C1035 1 OIIIt	5-2,	5-1			3-7
Delta to Analysis Win 3-9 Mkr to CF 3-9 Delta to V Scale/div 3-9 Mkr to CF Step 3-9 Disp Mode 3-2, 3-3 Mkr to Mkr Step 3-9 Display 3-2, 3-3 Mkr to Vertical Pos 3-9 Dual Measure 3-2, 3-4 MKR→ 3-9 Duty Cycle 3-2, 3-7 More 1/2 3-9 [Nample of Four-Value FSK Signal Names and Functions of Each Part on Screen 2-1 Execute ON/OFF 3-2, 3-3 Names and Functions of Each Part on the Screen 2-1 Execute ON/OFF 3-2, 3-3 Negative Duty Cycle 3-2, 3-7 Freq-Time 3-2, 3-3 Negative Width 3-2, 3-7 Normal 3-2, 3-3 Normal 3-2, 3-3 Freq-Time Analysis Using Position 2-6 Normal 3-2, 3-3 Freq-Time Analysis Using Position 2-12 [O] Freq-Time, Phase-Time, Power-Time, or IQ-Time Display Screen 2-1 Operating Method 2-4 Frequency 3-2, 3-7 Option 53, Option 54 Time Domain 5-1	rn:					
Delta to V Scale/div 3-9 Mkr to CF Step 3-9 Disp Mode 3-2, 3-3 Mkr to Mkr Step 3-9 Display 3-2, 3-3 Mkr to Vertical Pos 3-9 Dual Measure 3-2, 3-4 MKR→ 3-9 Duty Cycle 3-2, 3-7 More 1/2 3-9 Example of Four-Value FSK Signal Names and Functions of Each Part on Screen 2-1 Execute ON/OFF 3-2, 3-3 Names and Functions of Each Part on the Screen 2-1 Execute ON/OFF 3-2, 3-3 Negative Duty Cycle 3-2, 3-7 Freq-Time 3-2, 3-3 Negative Width 3-2, 3-7 Negative Width 3-2, 3-2 3-2 Normal 3-2, 3-3 3-2 Normal 3-2, 3-3 3-2 Normal 3-2, 3-3 Normal 3-2, 3-3 Normal 3-2, 3-3 Operating Method 2-4 Freq-Time Analysis Using Position 2-1 Freq-Time, Phase-Time, Power-Time, or IQ-Time Display Screen 2-1 Operating Method 2-4 </td <td></td> <td></td> <td></td> <td></td> <td></td> <td></td>						
Disp Mode 3-2, 3-3 Mkr to Mkr Step 3-9 Display 3-2, 3-3 Mkr to Vertical Pos 3-9 Dual Measure 3-2, 3-4 MKR→ 3-9 Duty Cycle 3-2, 3-7 More 1/2 3-9 INI Names and Functions of Each Part on Screen 2-1 Execute ON/OFF 3-2, 3-3 Names and Functions of Each Part on the Screen 2-1 Execute ON/OFF 3-2, 3-3 Negative Duty Cycle 3-2, 3-7 Freq-Time 3-2, 3-3 Negative Width 3-2, 3-7 Negative Width 3-2, 3-3 Normal 3-2, 3-3 Negative Width 3-2, 3-3 3-2, 3-3 Normal 3-2, 3-3 3-2, 3-3 Normal 3-2, 3-3 3-2, 3-3 Normal 3-2, 3-3 Operating Method 2-4 Freq-Time, Phase-Time, Power-Time, or IQ-Time Display Screen 2-1 Operating Method 2-4 Frequency 3-2, 3-7 Option 53, Option 54 Time Domain 5-1 Functional Descriptions 3-1 Op				Mkr to CF	3-9	
Display 3-2, 3-3 Mkr to Vertical Pos 3-9 Dual Measure 3-2, 3-4 MKR→ 3-9 Duty Cycle 3-2, 3-7 More 1/2 3-9 Duty Cycle 3-2, 3-7 More 1/2 3-2 IN IN Names and Functions of Each Part on Screen 2-1 Execute ON/OFF 3-2, 3-3 Names and Functions of Each Part on the Screen 2-3 Negative Duty Cycle 3-2, 3-7 Negative Duty Cycle 3-2, 3-7 Negative Width 3-2, 3-7 Normal 3-2, 3-7 Normal 3-2, 3-3 Screen 2-1 Negative Width 3-2, 3-3 Normal 3-2, 3-3 Normal 3-2, 3-3 Normal 3-2, 3-3 Operating Method 2-4 Frequency 3-2, 3-7 Option 53, Option 54 Time Domain Functional Descriptions 3-1 Option 55, Option 56 Time Domain	Delta to V Scale/div	3-9		Mkr to CF Step	3-9	
Dual Measure 3-2, 3-4 Duty Cycle MKR→ 3-9 Duty Cycle IE] IN] Example of Four-Value FSK Signal Analysis Names and Functions of Each Part on Screen 2-1 Execute ON/OFF 3-2, 3-3 Names and Functions of Each Part on the Screen 2-3 Freq-Time 3-2, 3-3 Negative Duty Cycle 3-2, 3-7 Negative Width 3-2, 3-7 Normal 3-2, 3-7 Normal 3-2, 3-3 3-2 3-2 Freq-Time Analysis Using Position View Function 2-12 IO] IO] Freq-Time, Phase-Time, Power-Time, or IQ-Time Display Screen 2-1 Operating Method 2-4 Frequency 3-2, 3-7 Option 53, Option 54 Time Domain 5-1 FUNCTION DESCRIPTION 3-1 Analysis Option 5-1 Functional Descriptions 3-1 Option 55, Option 56 Time Domain	Disp Mode	3-2,	3-3	Mkr to Mkr Step	3-9	
Example of Four-Value FSK Signal	Display	3-2,	3-3	Mkr to Vertical Pos	3-9	
Example of Four-Value FSK Signal Names and Functions of Each Part on Screen 2-1	Dual Measure	3-2,	3-4	MKR→	3-9	
Example of Four-Value FSK Signal	Duty Cycle	3-2,	3-7	More 1/2	3-2	
Example of Four-Value FSK Signal	•					
Example of Four-Value FSK Signal	r=1			[N]		
Analysis 2-20 Screen 2-1 Execute ON/OFF 3-2, 3-3 Names and Functions of Each Part on the Screen 2-3 Negative Duty Cycle 3-2, 3-7 Negative Width 3-2, 3-7 Normal 3-2, 3-3 Normal 3-2, 3-3 Normal 3-2, 3-3 Normal 3-2, 3-3 OFF 3-2, 3-7 Operating Method 2-4 Option 53, Option 54 Time Domain 5-1 Functional Descriptions 3-1 Option 55, Option 56 Time Domain						
Execute ON/OFF 3-2, 3-3 Names and Functions of Each Part on the Screen 2-3 IFI Negative Duty Cycle 3-2, 3-7 Negative Width 3-2, 3-7 Normal 3-2, 3-3 OFF 3-2, 3-7 Operating Method 2-4 Option 53, Option 54 Time Domain 5-1 Functional Descriptions 3-1 Option 55, Option 56 Time Domain		2 20			2 1	
the Screen 2-3 Negative Duty Cycle 3-2, 3-7 Negative Width 3-2, 3-7 Normal 3-2, 3-3 Freq-Time Analysis Using Position View Function 2-12 Freq-Time, Phase-Time, Power-Time, or IQ-Time Display Screen 2-1 Frequency 3-2, 3-7 Frequency 3-2, 3-7 Functional Descriptions 3-1 Functional Descriptions 3-1 Chapter 1			2.2		2-1	
Negative Duty Cycle	Execute ON/OFF	3-2,	3-3		2.2	
Freq-Time						
Freq-Time	[F]					
Freq-Time Analysis 2-6 Freq-Time Analysis Using Position View Function 2-12 Freq-Time, Phase-Time, Power-Time, or IQ-Time Display Screen 2-1 Frequency 3-2, 3-7 Option 53, Option 54 Time Domain FUNCTION DESCRIPTION 3-1 Functional Descriptions 3-1 Option 55, Option 56 Time Domain		3-2.	3-3			
Freq-Time Analysis Using Position View Function 2-12 Freq-Time, Phase-Time, Power-Time, or IQ-Time Display Screen 2-1 Frequency 3-2, 3-7 FUNCTION DESCRIPTION 3-1 Functional Descriptions 3-1 Option 55, Option 56 Time Domain OFF 3-2, 3-7 Option 53, Option 54 Time Domain Analysis Option 55, Option 56 Time Domain				Normal	3-2,	3-3
View Function2-12[O]Freq-Time, Phase-Time, Power-Time, or IQ-Time Display ScreenOFF3-2, 3-7Frequency3-2, 3-7Operating Method2-4Frequency3-2, 3-7Option 53, Option 54 Time DomainFUNCTION DESCRIPTION3-1Analysis Option5-1Functional Descriptions3-1Option 55, Option 56 Time Domain						
Freq-Time, Phase-Time, Power-Time, or IQ-Time Display Screen 2-1 Operating Method 2-4 Frequency 3-2, 3-7 FUNCTION DESCRIPTION 3-1 Analysis Option 54 Time Domain Functional Descriptions 3-1 Option 55, Option 56 Time Domain		2-12		[0]		
or IQ-Time Display Screen2-1Operating Method2-4Frequency3-2, 3-7Option 53, Option 54 Time DomainFUNCTION DESCRIPTION3-1Analysis Option5-1Functional Descriptions3-1Option 55, Option 56 Time Domain		L 1.L			3_2	3_7
Frequency		2-1				J-1
FUNCTION DESCRIPTION	- ·		3-7		∠ ¬	
Functional Descriptions			5-1		5_1	
					J-1	
	1 dilettolidi Descriptions	<i>J</i> 1			5-1	

Alphabetical Index

OVERVIEW OF REMOTE CONTROL	4-1	Ve	rtical Scale/div		3-2,	3-3
[P]				[W]		
Partial FFT	3_2	3-3 Wi	dth	r1	3_2	3-7
Partial FFT Analysis		J-J VV I	uii	•••••	J- <u>Z</u> ,	J=1
Partial FFT Display Screen						
Peak to CF						
Peak to Ref		2.2				
Phase-Time Applying		3-3				
Phase-Time Analysis		2.2				
Position View		3-3				
Positive Duty Cycle		3-7				
Positive Width		3-7				
Power-Time		3-3				
Power-Time Analysis						
Product Overview	1-2					
[R]						
Restrictions	6-2					
Restrictions for Trace Data Capture						
Restrictions on Key Operation during						
Time Domain Analysis Function Use	6-2					
[S]						
Search Left	2 2	2 7				
Search Right		3-7				
Setting Center Frequency, Reference Lev						
and Sweep Mode	2-3					
Setting Waveform Capture Time and	2.5					
Capture Bandwidth		2.7				
Slope UP/DN/ALL		3-7				
SPECIFICATIONS	5-1					
Starting and Stopping RF Signal	2.5					
Capture	2-5					
[T]						
Threshold ON/OFF	3-2	3-7.				
	3-8	5 7,				
Time Domain		3-2,				
Time Domain	3-1,	5-2,				
Two-Type Simultaneous Analysises	5 5					
Using Dual Meas Function						
(Freq-Time and Phase-Time)	2-14					
nn						
[U]						
UNCAL MESSAGE, LIST OF ERROR	<i>(</i> 1					
MESSAGES, AND RESTRICTIONS	6-1					
[V]						
Vertical Position	3-2	3-3				
	<i>-</i> −,					